

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026691.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2022 17:41
 Operator : AJ/MA
 Sample : BSF0316S1
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0316S1

Integration File: Calibration.e
 Quant Time: Mar 17 01:00:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	237936	22.675 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	522158	27.578 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	563612	27.192 ng/ml
3) t n-Heptane	7.751	187487	9.472 ng/ml
4) t Benzene	7.888	215666	9.346 ng/ml
6) t Toluene	10.620	619526	28.298 ng/ml
7) t Ethylbenzene	13.058	186846	9.297 ng/ml
8) t m-Xylene	13.191	372508	18.484 ng/ml
9) t O-Xylene	13.917	362640	18.177 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	359734	18.055 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026691.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2022 17:41
Operator : AJ/MA
Sample : BSF0316S1
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0316S1

Integration File: Calibration.e
Quant Time: Mar 17 01:00:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

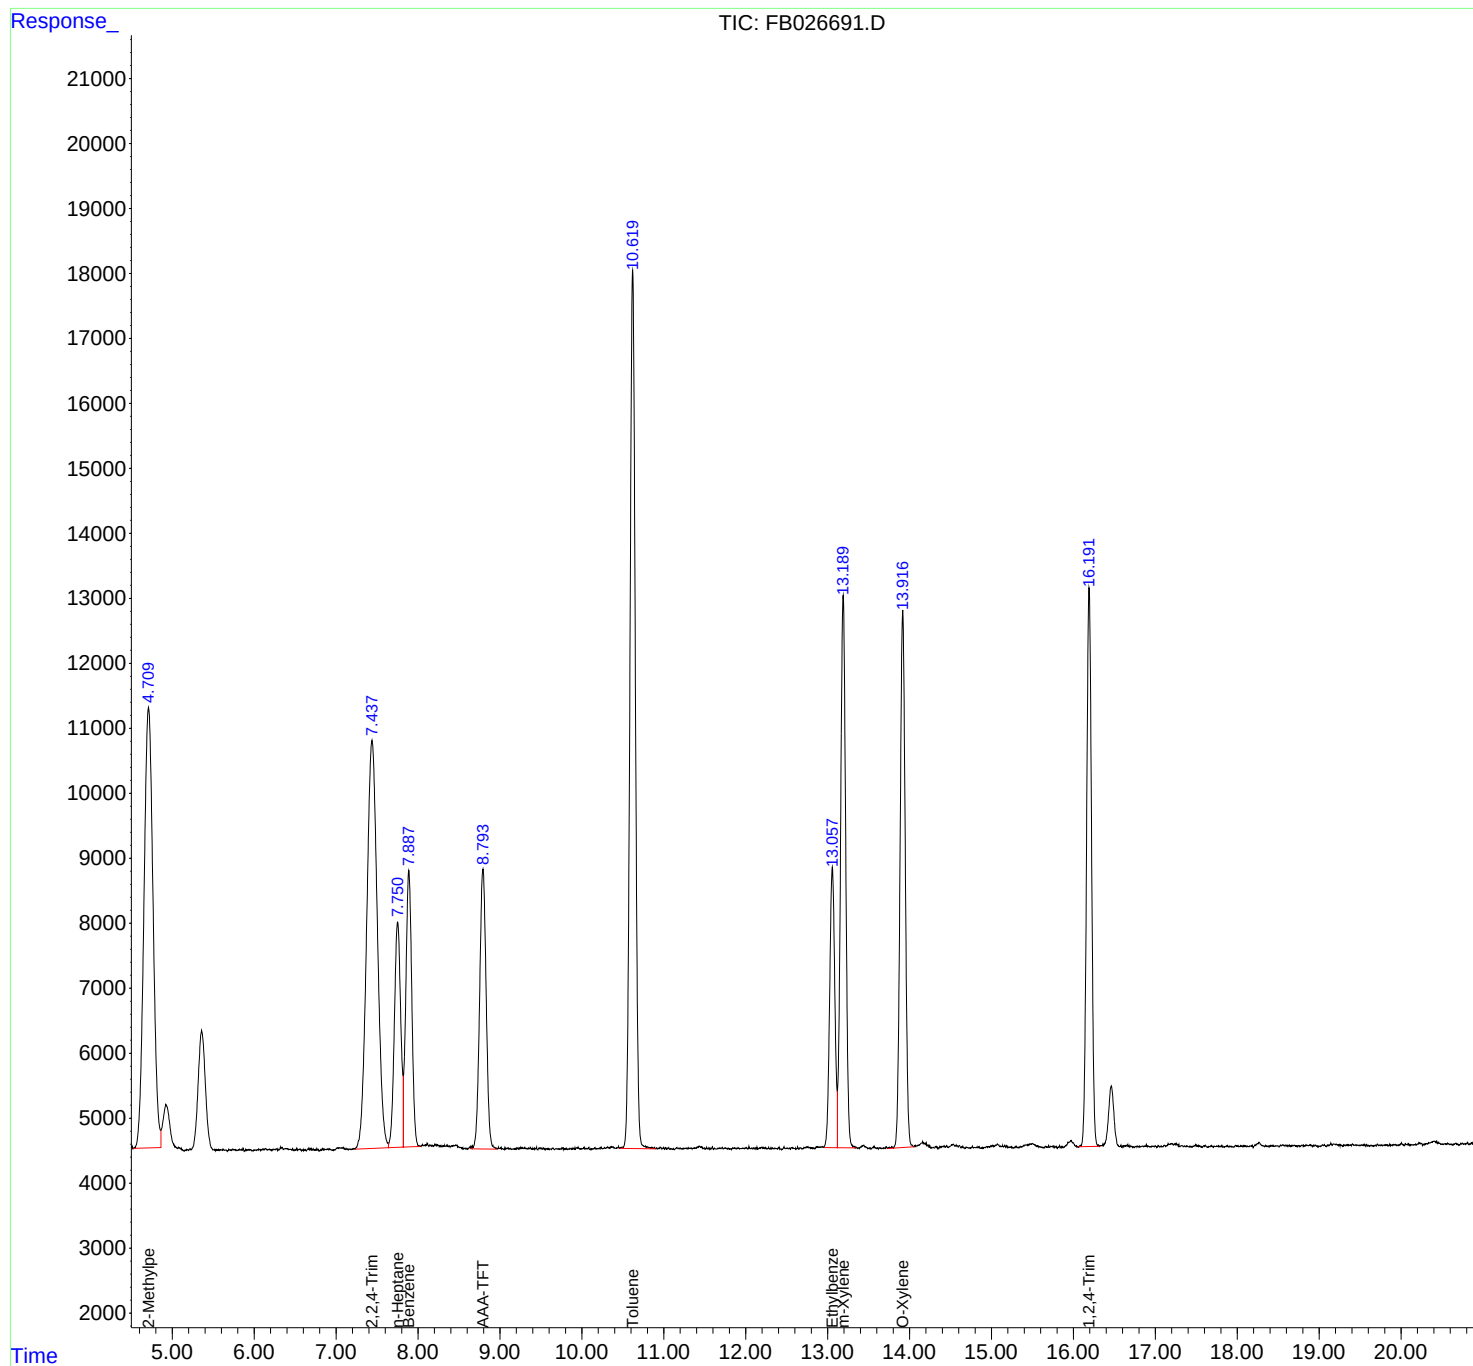


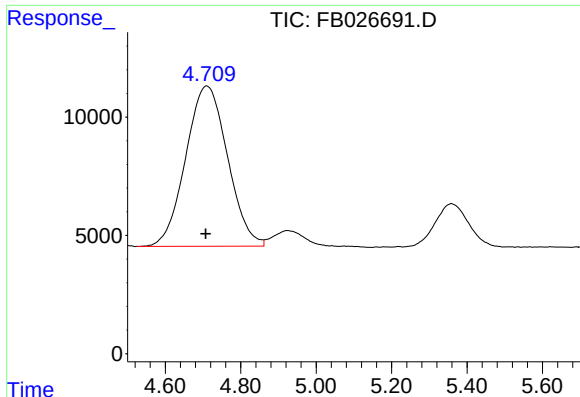

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 522158
Conc: 27.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0316S1

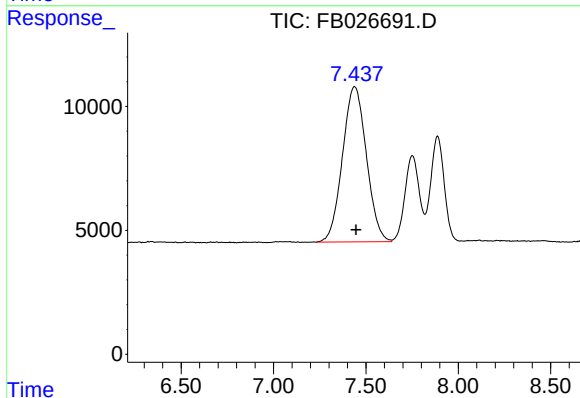


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: -0.009 min
Response: 563612
Conc: 27.19 ng/ml

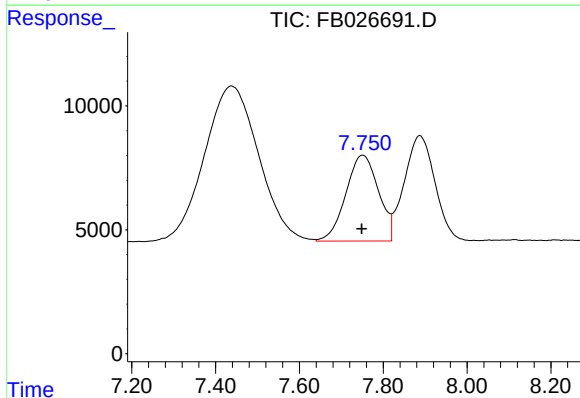


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.003 min
Response: 187487
Conc: 9.47 ng/ml

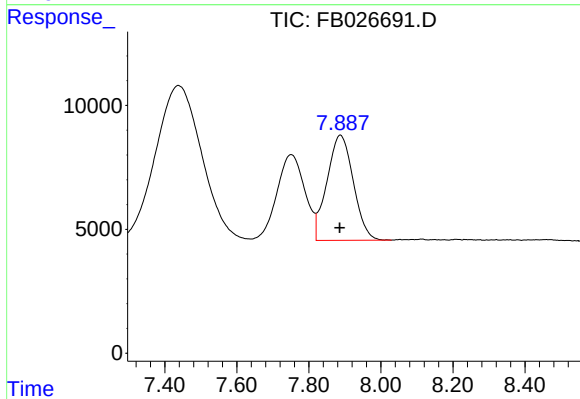

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 215666
Conc: 9.35 ng/ml

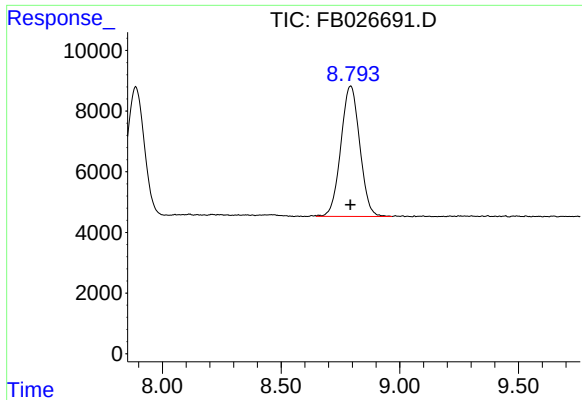

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 237936
Conc: 22.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0316S1

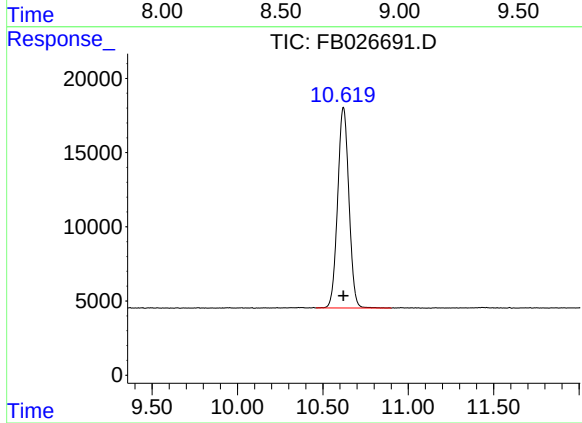


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 619526
Conc: 28.30 ng/ml

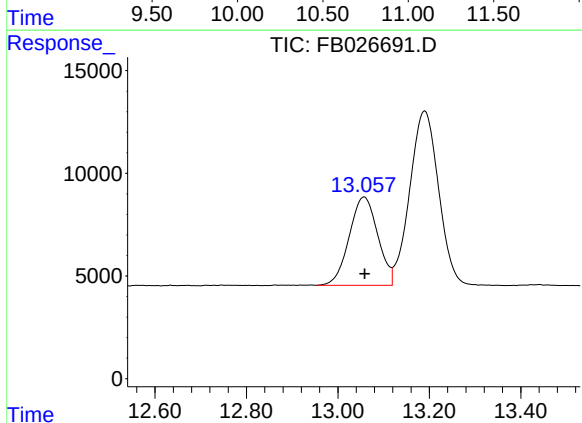


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 186846
Conc: 9.30 ng/ml

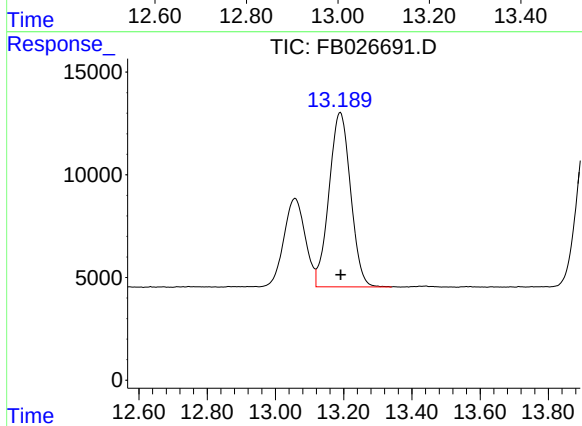

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: -0.001 min
Response: 372508
Conc: 18.48 ng/ml

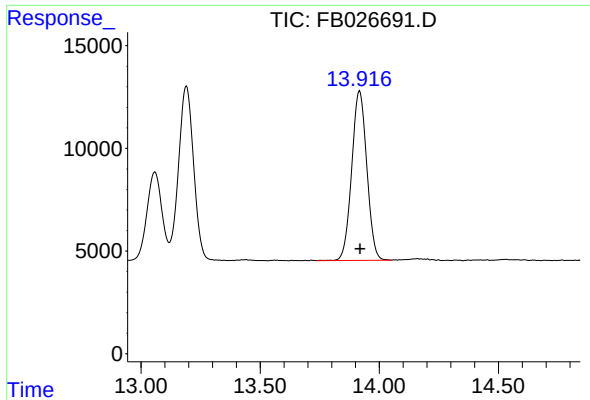

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.002 min
Response: 362640
Conc: 18.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0316S1

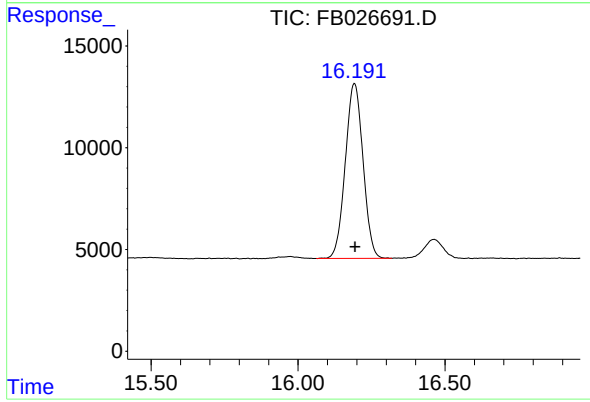

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.002 min
Response: 359734
Conc: 18.05 ng/ml