

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026712.D
 Signal(s) : FID2B.CH
 Acq On : 17 Mar 2022 8:20
 Operator : AJ/MA
 Sample : N1966-07MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G-1-7-13-14MS

Integration File: Calibration.e
 Quant Time: Mar 17 15:09:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	146025	13.916 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	385156	20.343 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	366846	17.699 ng/ml
3) t n-Heptane	7.750	127854	6.460 ng/ml
4) t Benzene	7.887	185219	8.027 ng/ml
6) t Toluene	10.619	481122	21.976 ng/ml
7) t Ethylbenzene	13.056	155305	7.727 ng/ml
8) t m-Xylene	13.189	297266	14.751 ng/ml
9) t O-Xylene	13.916	288970	14.485 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	261533	13.126 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026712.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 8:20
Operator : AJ/MA
Sample : N1966-07MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MS

Integration File: Calibration.e
Quant Time: Mar 17 15:09:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

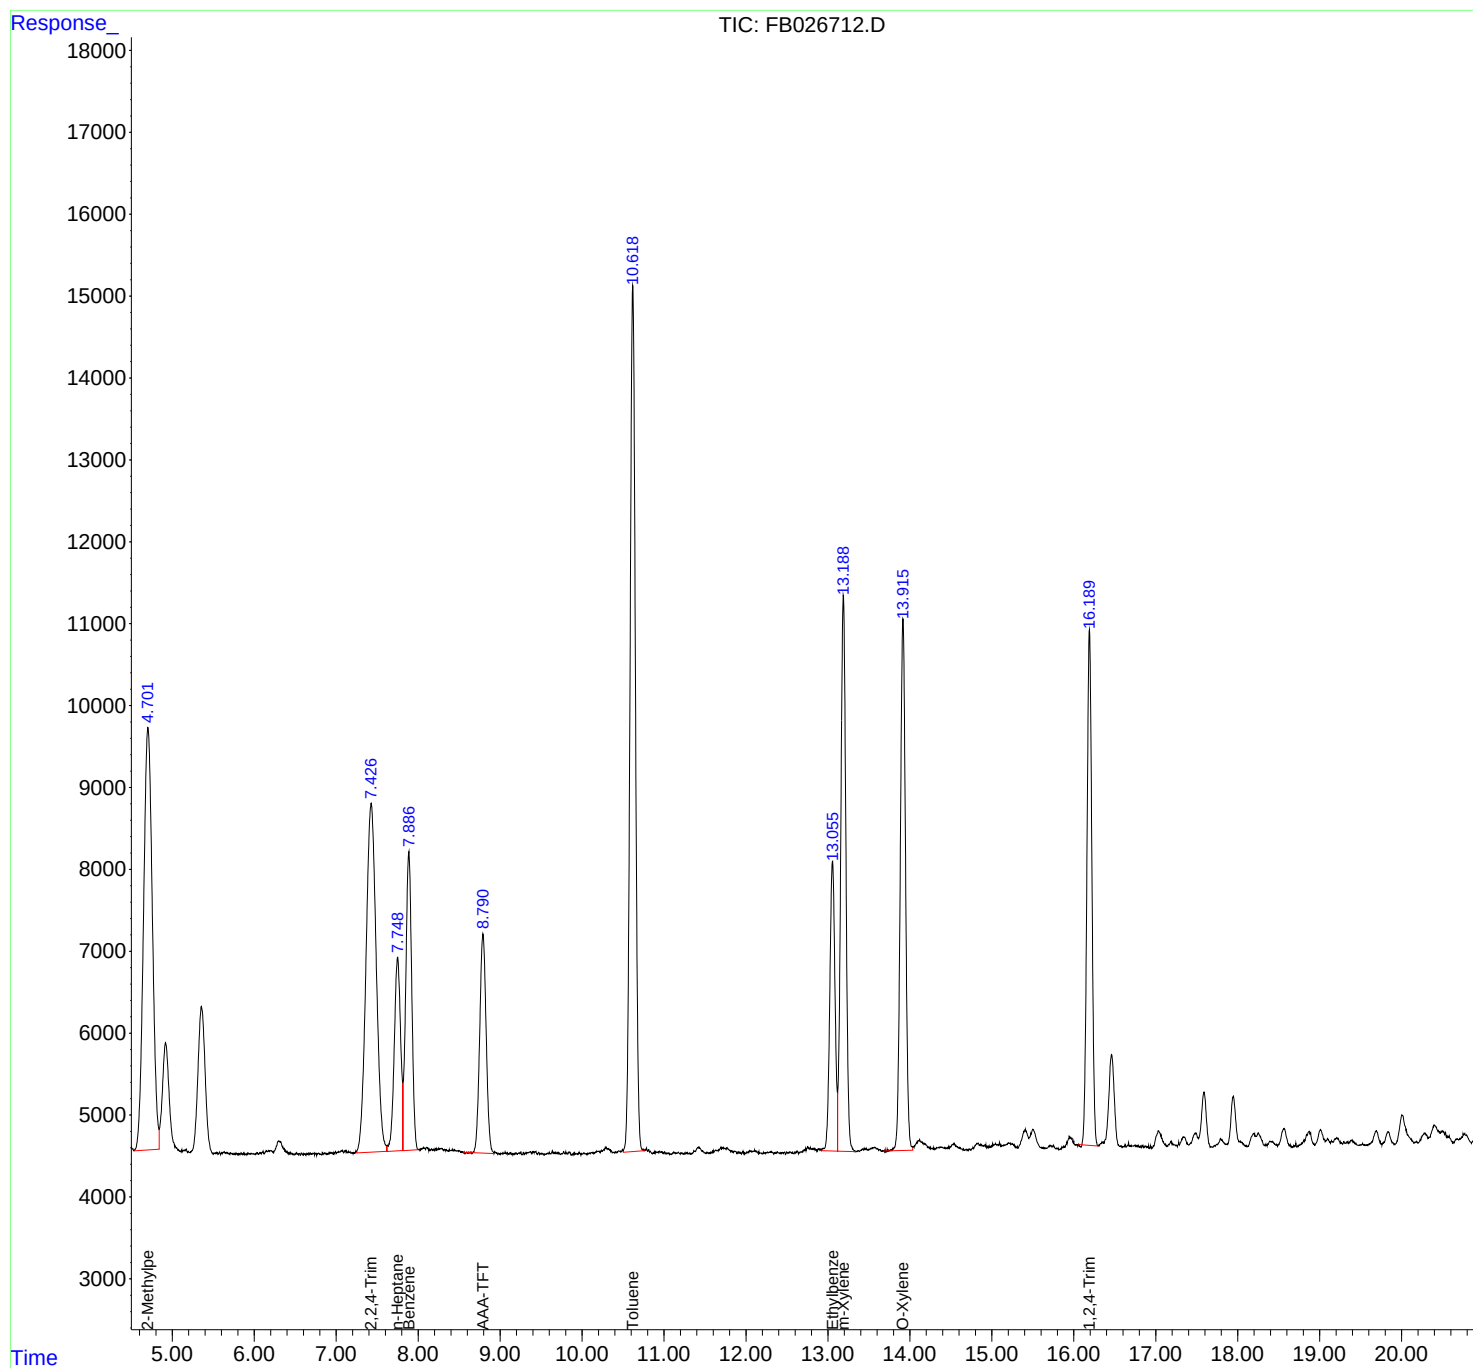


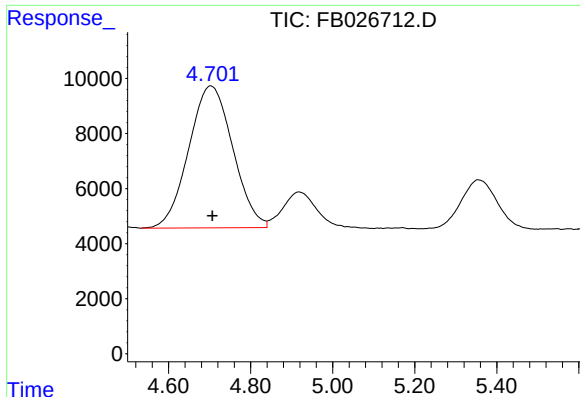

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.004 min
Response: 385156
Conc: 20.34 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MS

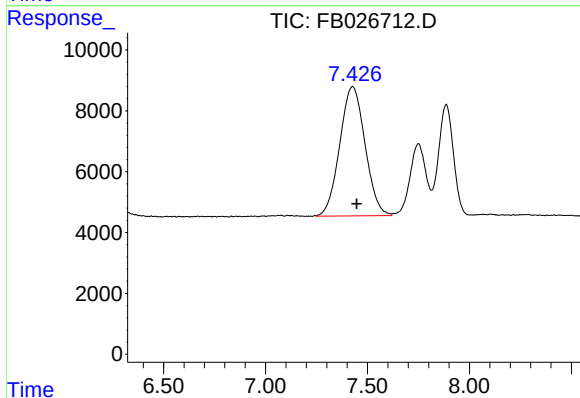


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.020 min
Response: 366846
Conc: 17.70 ng/ml

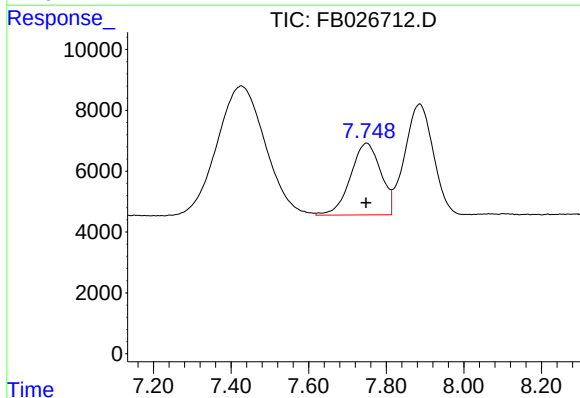


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 127854
Conc: 6.46 ng/ml

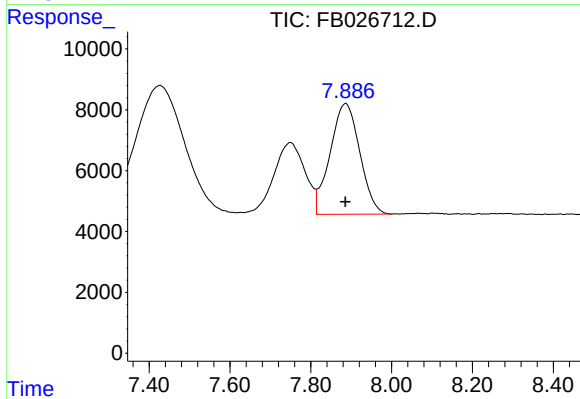

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.001 min
Response: 185219
Conc: 8.03 ng/ml

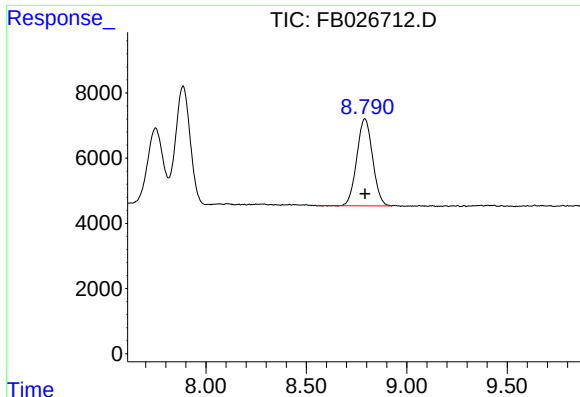

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 146025
Conc: 13.92 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MS

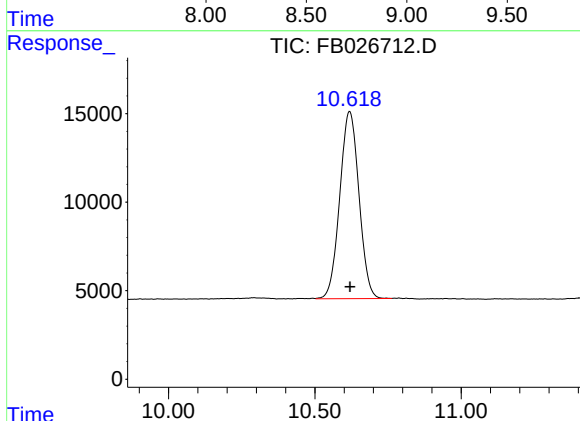


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 481122
Conc: 21.98 ng/ml

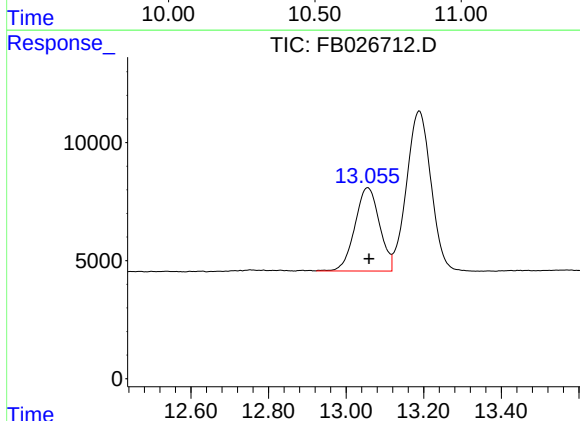


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 155305
Conc: 7.73 ng/ml

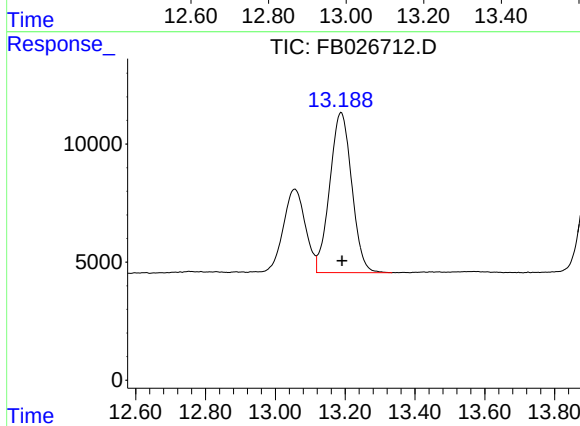

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.003 min
Response: 297266
Conc: 14.75 ng/ml

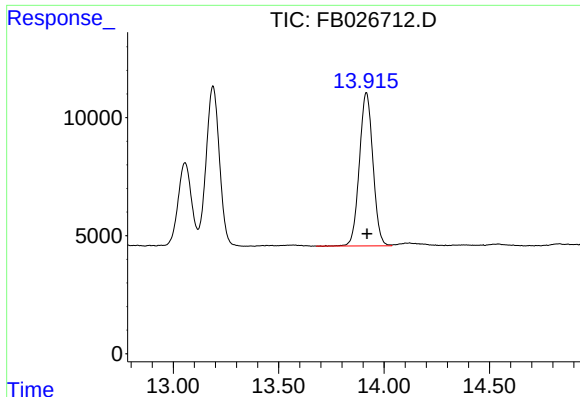

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 288970
Conc: 14.48 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MS

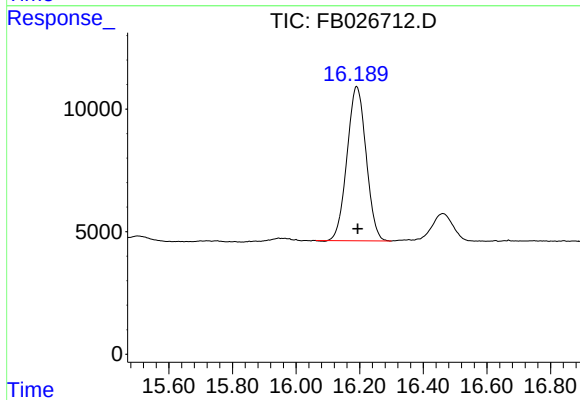

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.003 min
Response: 261533
Conc: 13.13 ng/ml