

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
 Data File : FB026713.D
 Signal(s) : FID2B.CH
 Acq On : 17 Mar 2022 8:58
 Operator : AJ/MA
 Sample : N1966-07MSD
 Misc : 5.09G/5.00 ML DI WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G-1-7-13-14MSD

Integration File: Calibration.e
 Quant Time: Mar 17 15:09:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	169424	16.146 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	513346	27.113 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	561312	27.081 ng/ml
3) t n-Heptane	7.749	182827	9.237 ng/ml
4) t Benzene	7.886	219356	9.506 ng/ml
6) t Toluene	10.619	623511	28.480 ng/ml
7) t Ethylbenzene	13.056	188365	9.372 ng/ml
8) t m-Xylene	13.188	370925	18.406 ng/ml
9) t O-Xylene	13.916	366126	18.352 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	353289	17.731 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026713.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 8:58
Operator : AJ/MA
Sample : N1966-07MSD
Misc : 5.09G/5.00 ML DI WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MSD

Integration File: Calibration.e
Quant Time: Mar 17 15:09:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

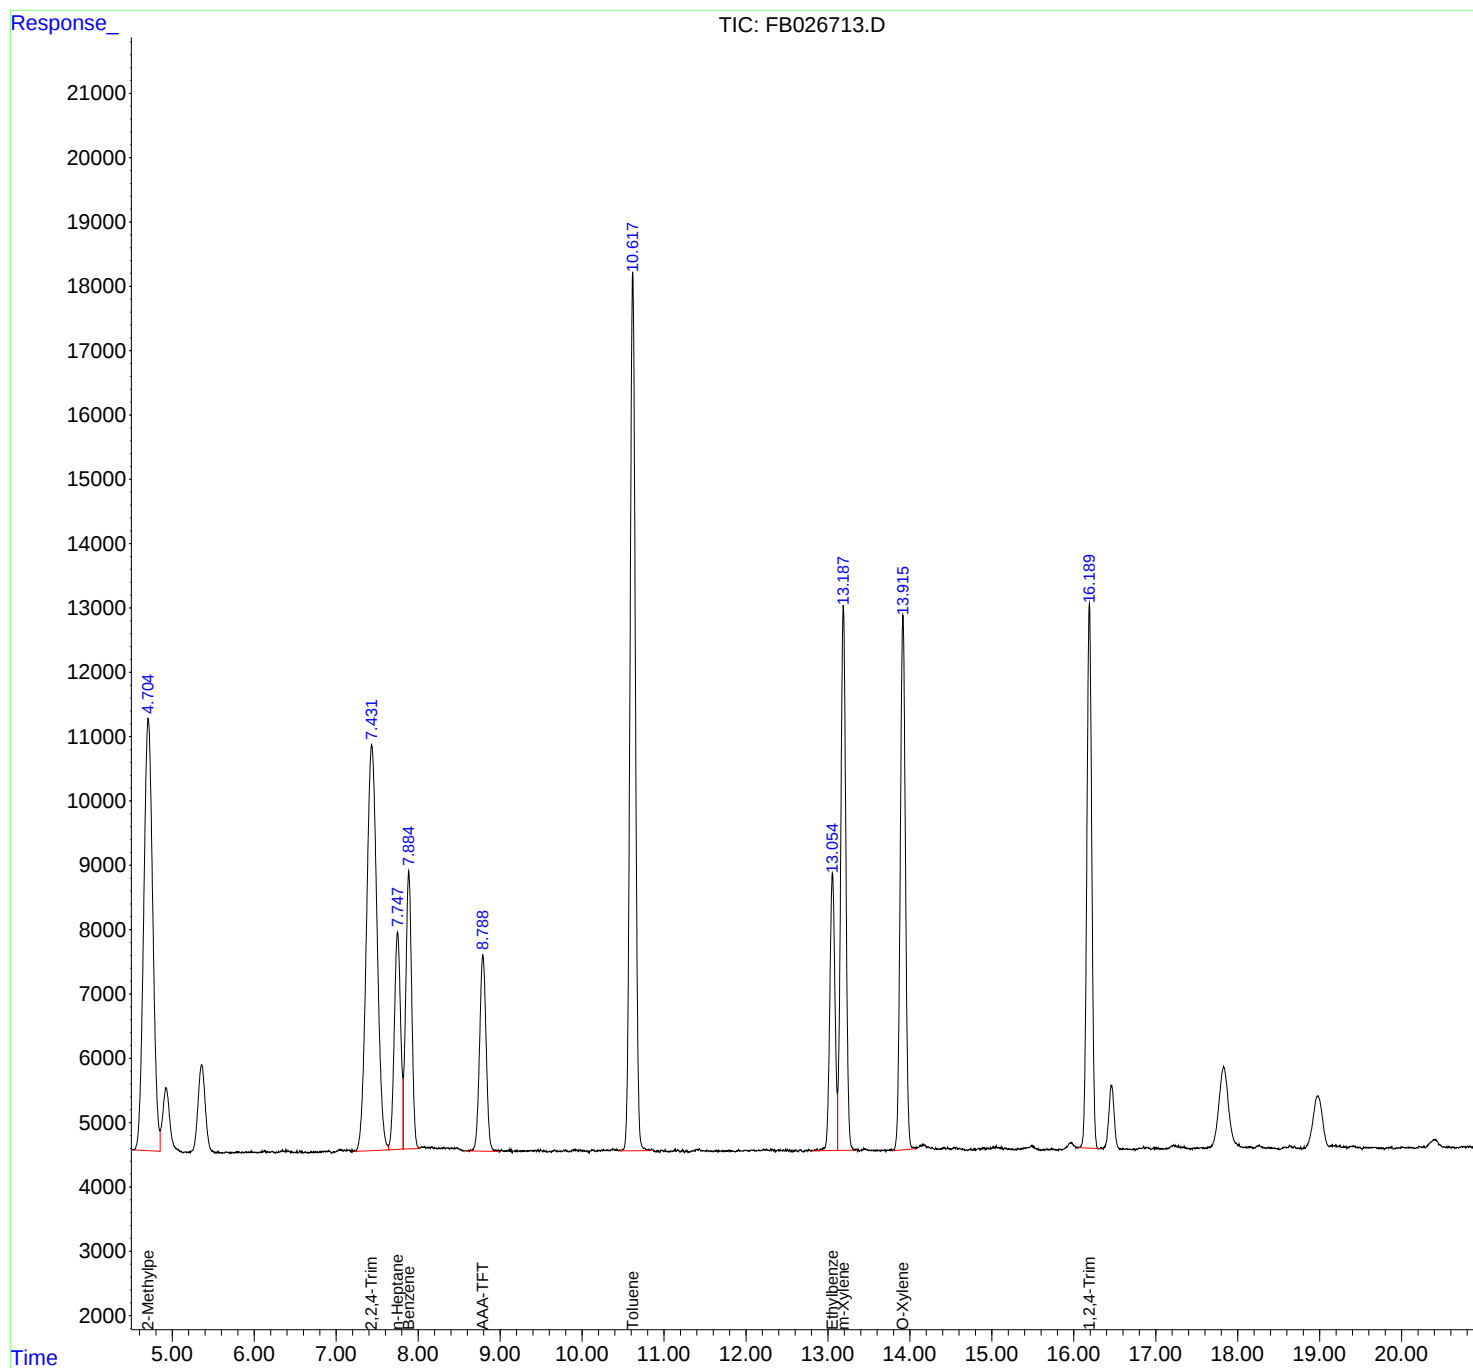


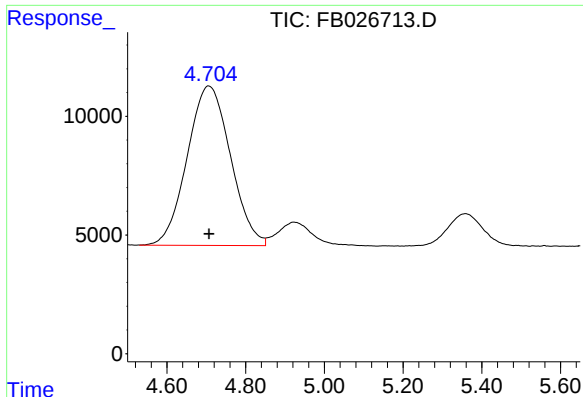

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 513346
Conc: 27.11 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MSD

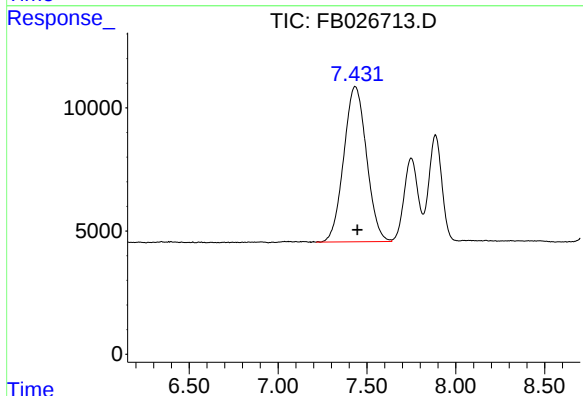


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: -0.015 min
Response: 561312
Conc: 27.08 ng/ml

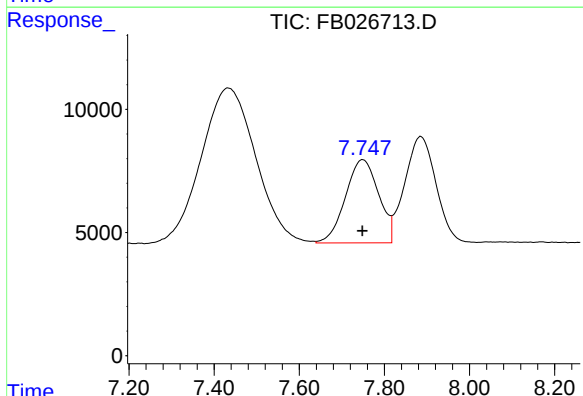


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 182827
Conc: 9.24 ng/ml

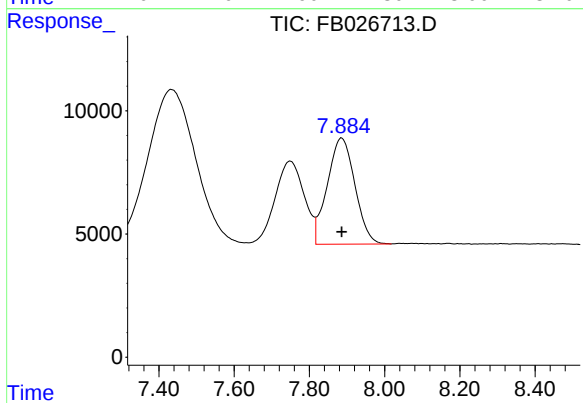

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 219356
Conc: 9.51 ng/ml

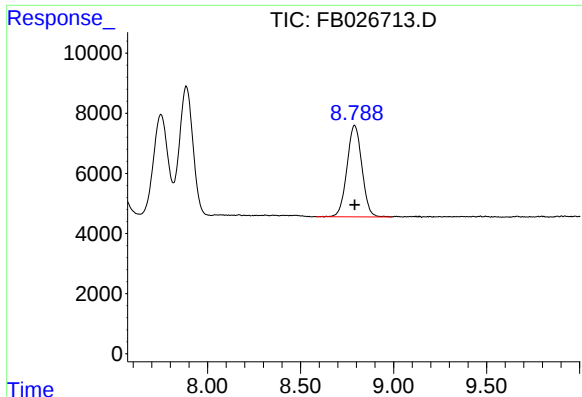

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 169424
Conc: 16.15 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MSD

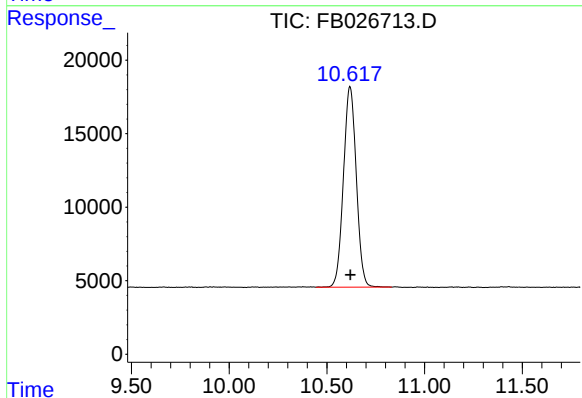


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 623511
Conc: 28.48 ng/ml

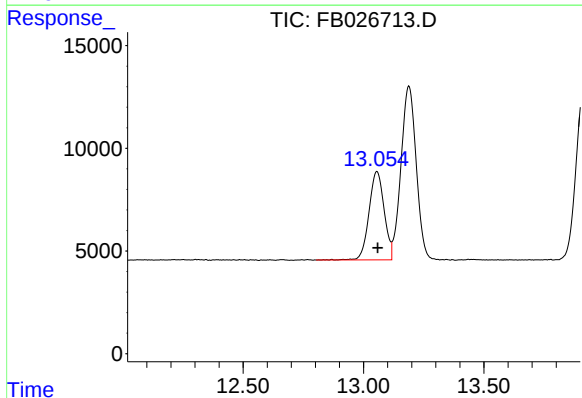


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 188365
Conc: 9.37 ng/ml

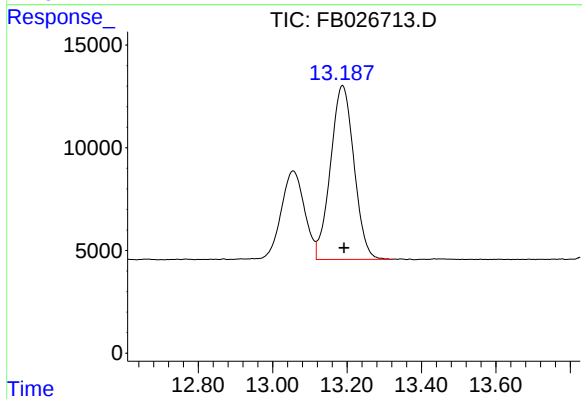

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 370925
Conc: 18.41 ng/ml

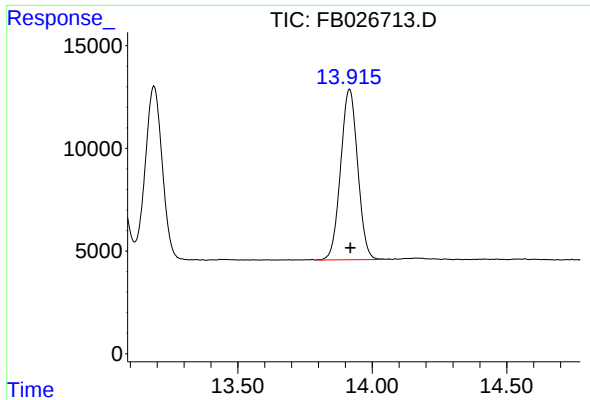

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 366126
Conc: 18.35 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14MSD

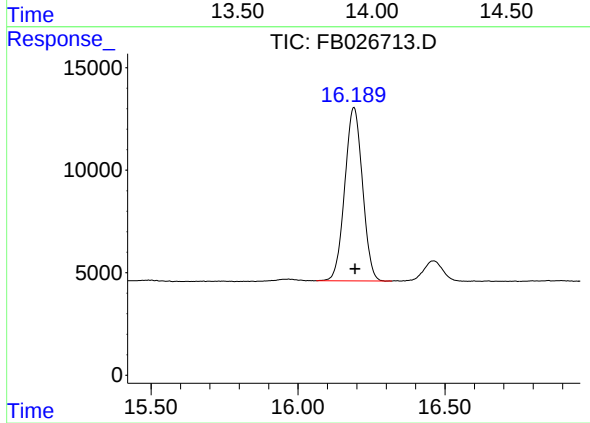

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 353289
Conc: 17.73 ng/ml