

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026714.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 9:36
Operator : AJ/MA
Sample : N1966-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14

Integration File: Calibration.e
Quant Time: Mar 17 15:09:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	189888	18.096 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031622\
Data File : FB026714.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2022 9:36
Operator : AJ/MA
Sample : N1966-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14

Integration File: Calibration.e
Quant Time: Mar 17 15:09:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

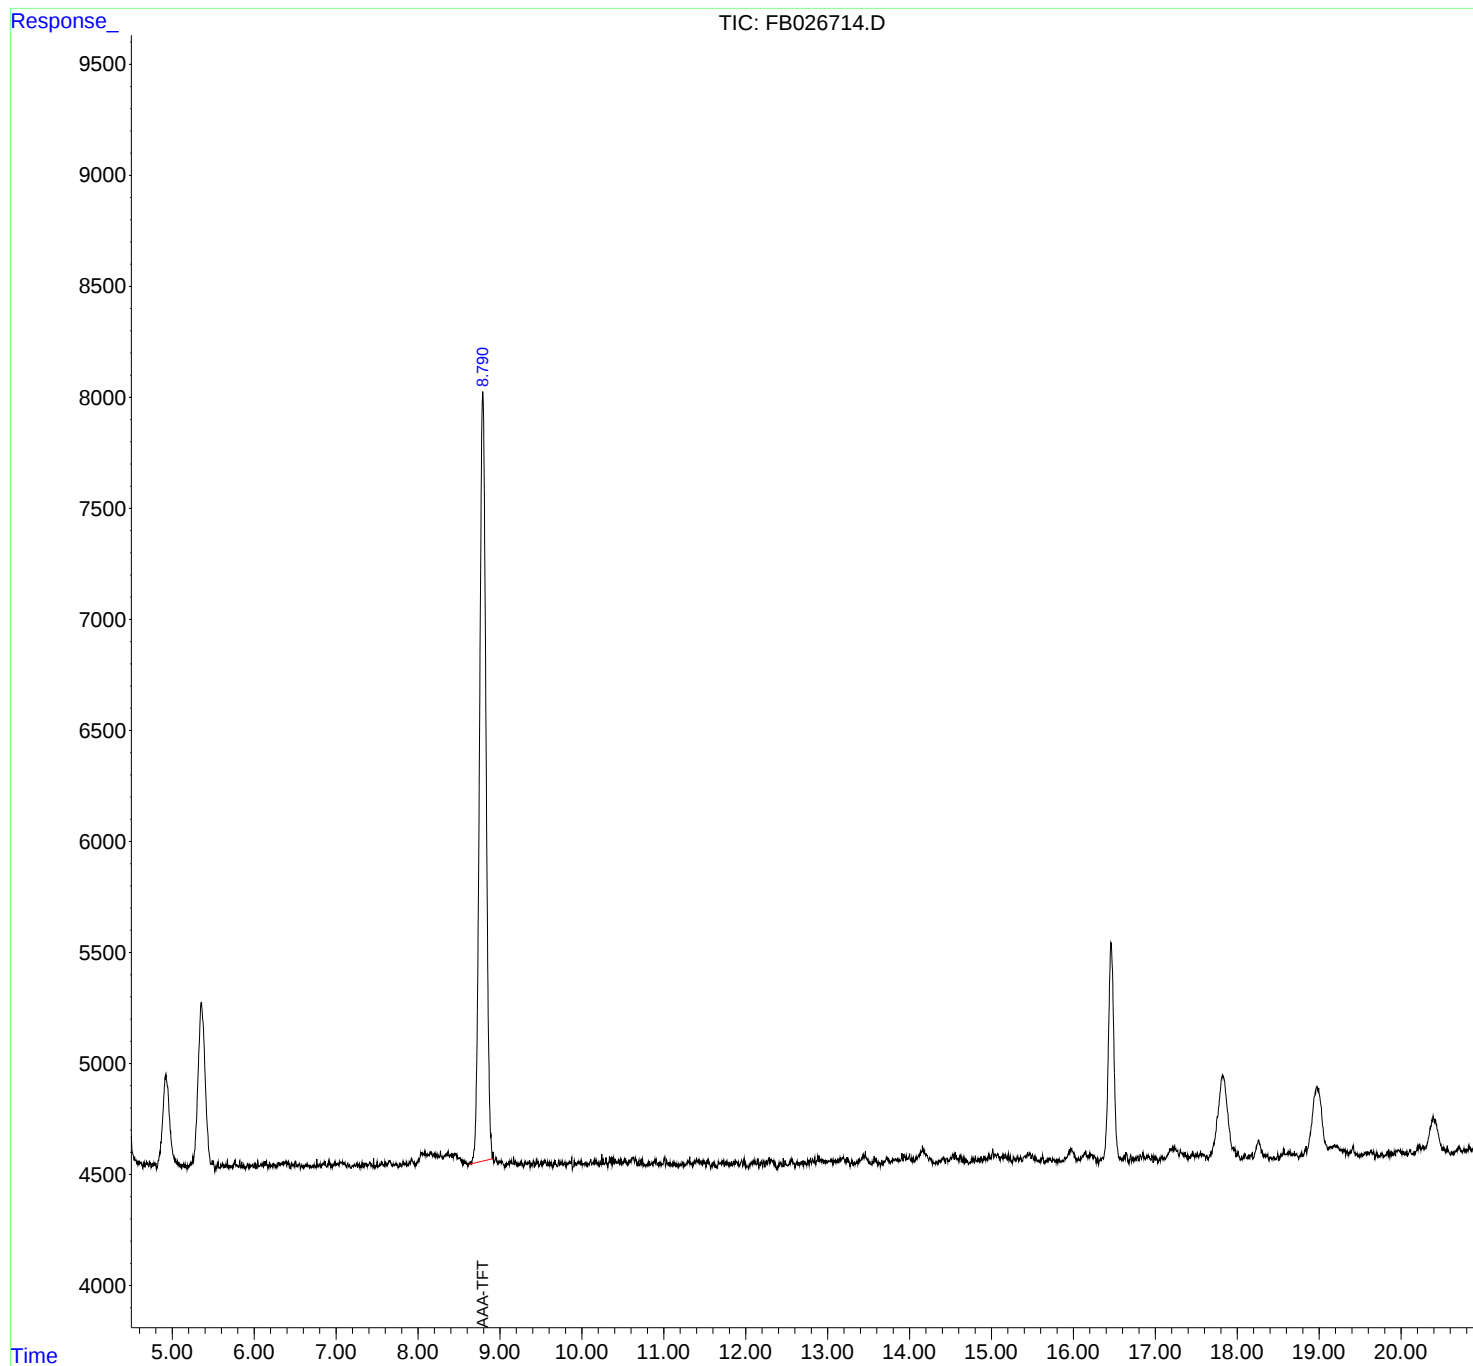

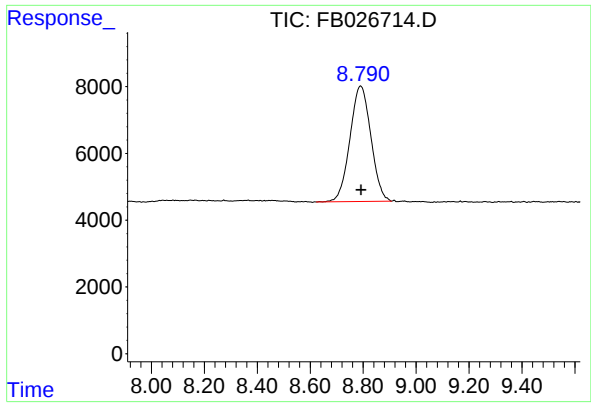

#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 189888
Conc: 18.10 ng/ml

Instrument :
FID_B
ClientSampleId :
G-1-7-13-14