

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031623\
 Data File : FB029512.D
 Signal(s) : FID2B.CH
 Acq On : 16 Mar 2023 14:27
 Operator : YP/AJ
 Sample : BSF0316S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 16 16:19:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	194695	16.070 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	352776	22.991 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	402964	23.922 ng/ml
3) t n-Heptane	7.753	139084	8.041 ng/ml
4) t Benzene	7.890	166003	8.178 ng/ml
6) t Toluene	10.623	502480	25.456 ng/ml
7) t Ethylbenzene	13.060	157252	8.447 ng/ml
8) t m-Xylene	13.193	312341	16.789 ng/ml
9) t O-Xylene	13.920	298377	16.205 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	282268	15.155 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031623\
Data File : FB029512.D
Signal(s) : FID2B.CH
Acq On : 16 Mar 2023 14:27
Operator : YP/AJ
Sample : BSF0316S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 16 16:19:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

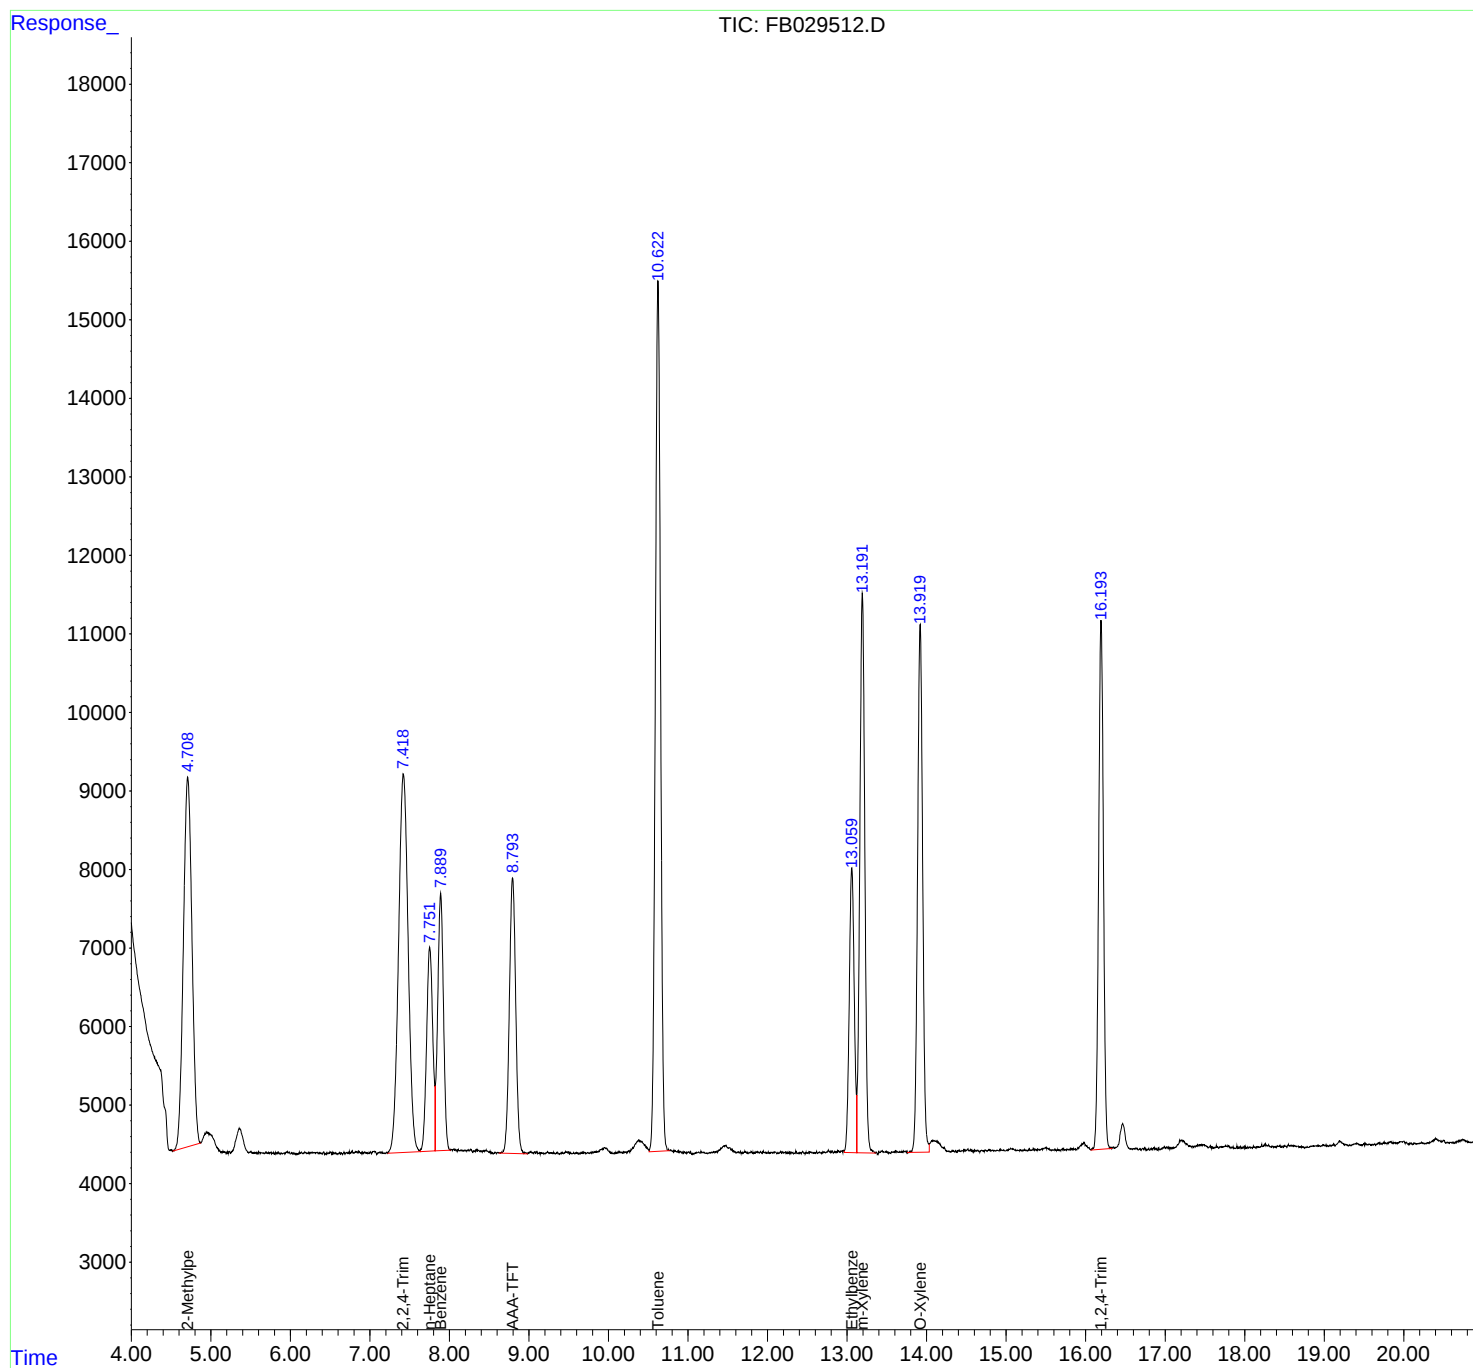

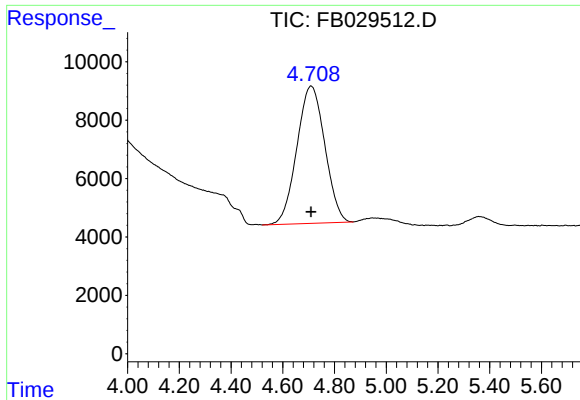


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 352776
Conc: 22.99 ng/ml

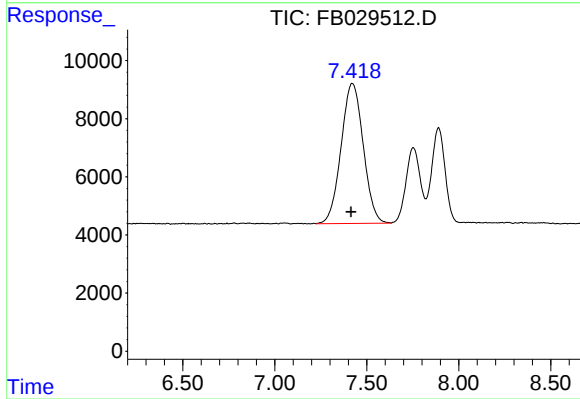


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.004 min
Response: 402964
Conc: 23.92 ng/ml

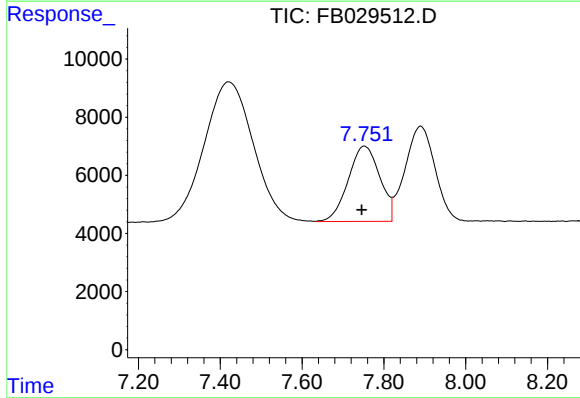


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.007 min
Response: 139084
Conc: 8.04 ng/ml

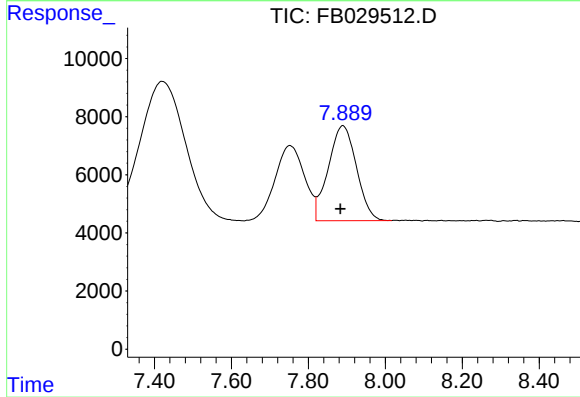


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.007 min
Response: 166003
Conc: 8.18 ng/ml

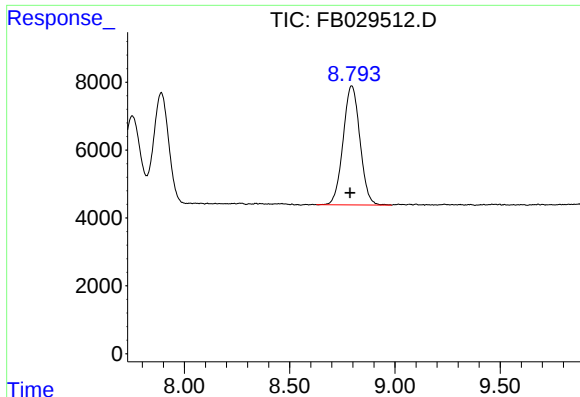


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.007 min
Response: 194695
Conc: 16.07 ng/ml

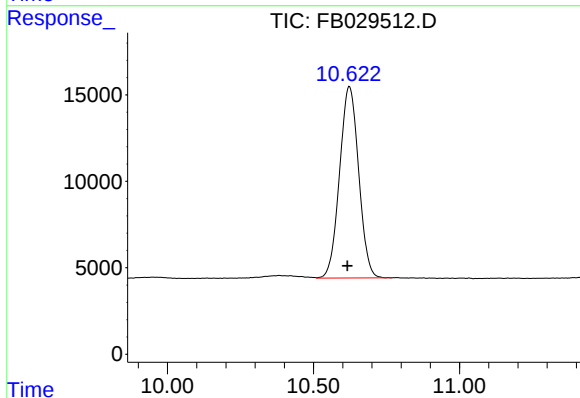


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.007 min
Response: 502480
Conc: 25.46 ng/ml

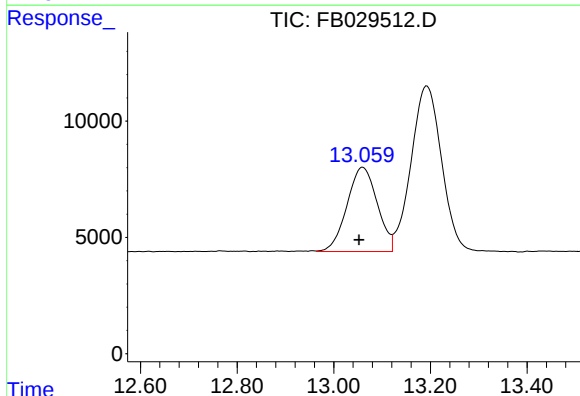


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.007 min
Response: 157252
Conc: 8.45 ng/ml

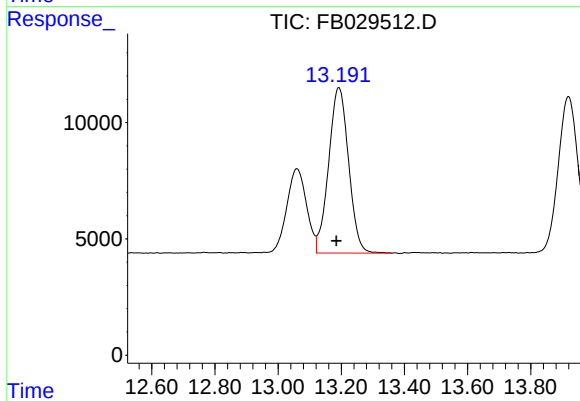


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.008 min
Response: 312341
Conc: 16.79 ng/ml

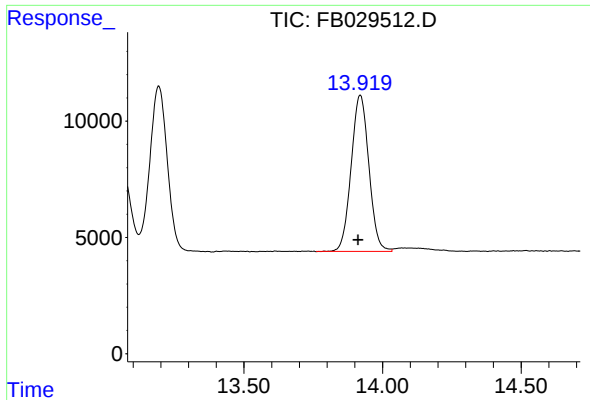

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.008 min
Response: 298377
Conc: 16.20 ng/ml

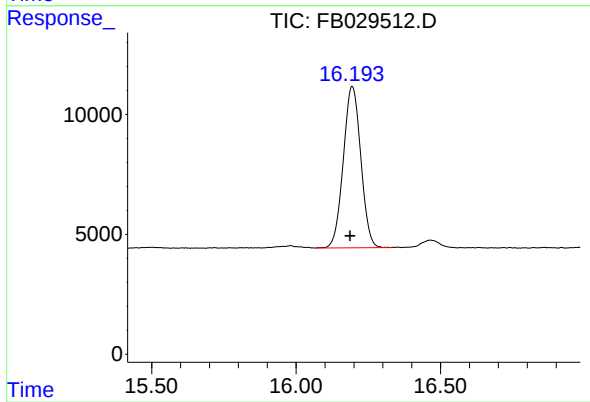

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.008 min
Response: 282268
Conc: 15.15 ng/ml