

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031819\
 Data File : FB020256.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2019 9:35
 Operator : MJ/SJ
 Sample : BSF0318S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 19 02:30:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.036	519593	19.792 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.894	1087854	32.249 ng/ml
2) t 2,2,4-Trimethylpentane	7.656	1018333	31.052 ng/ml
3) t n-Heptane	7.990	435618	10.467 ng/ml
4) t Benzene	8.127	463748	9.961 ng/ml
6) t Toluene	10.882	1054428	28.534 ng/ml
7) t Ethylbenzene	13.334	233174	9.910 ng/ml
8) t m-Xylene	13.468	461740	21.646 ng/ml
9) t O-Xylene	14.200	446933	23.593 ng/ml
10) t 1,2,4-Trimethylbenzene	16.486	459182	23.154 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031819\
Data File : FB020256.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2019 9:35
Operator : MJ/SJ
Sample : BSF0318S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 19 02:30:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

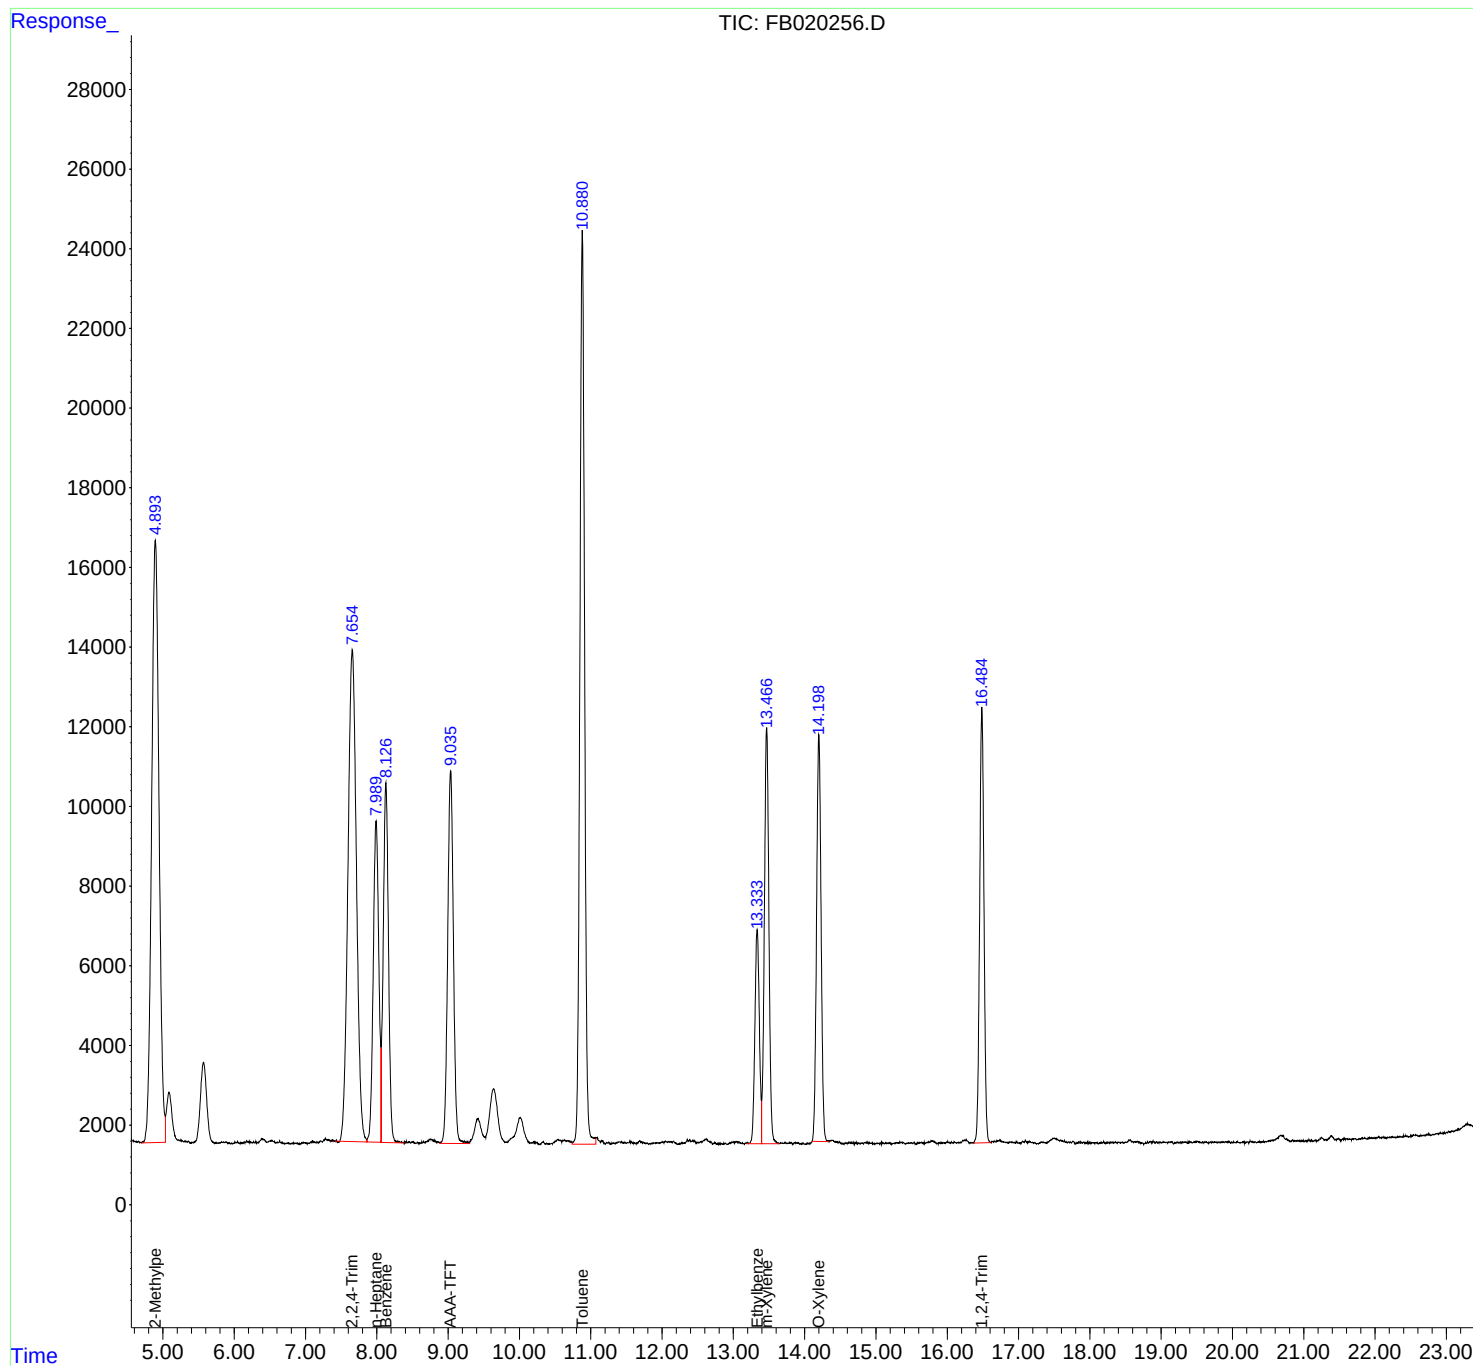

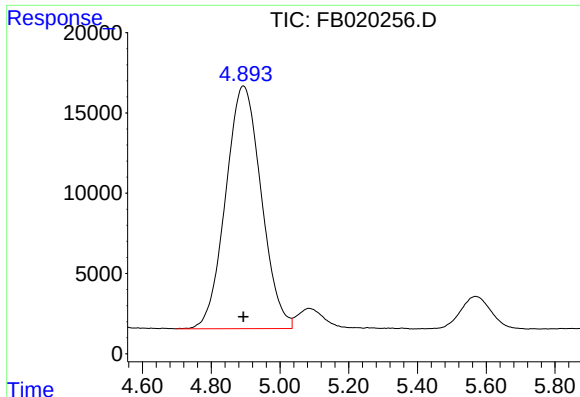


#1 2-Methylpentane

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 1087854
Conc: 32.25 ng/ml

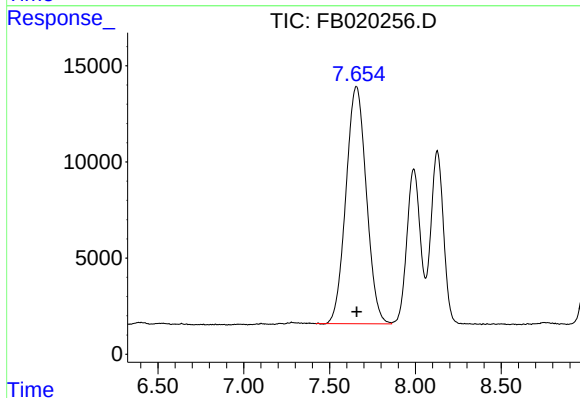


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 1018333
Conc: 31.05 ng/ml

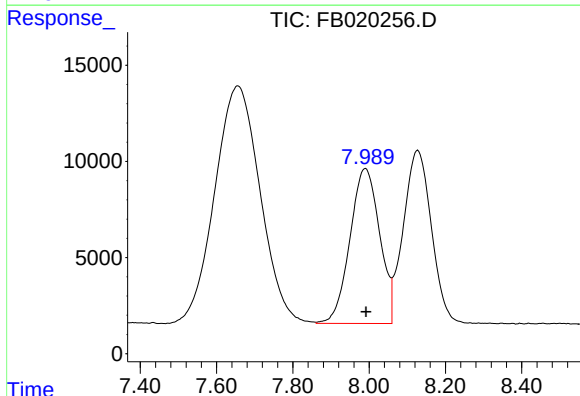


#3 n-Heptane

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 435618
Conc: 10.47 ng/ml

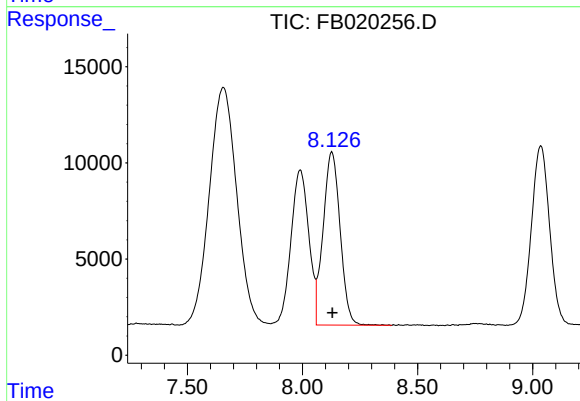


#4 Benzene

R.T.: 8.127 min
Delta R.T.: -0.003 min
Response: 463748
Conc: 9.96 ng/ml

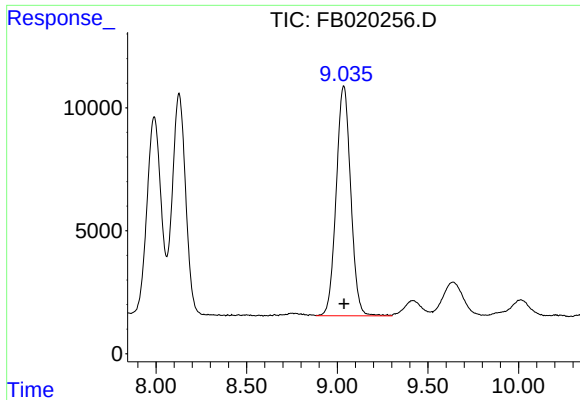


#5 AAA-TFT

R.T.: 9.036 min
Delta R.T.: -0.002 min
Response: 519593
Conc: 19.79 ng/ml

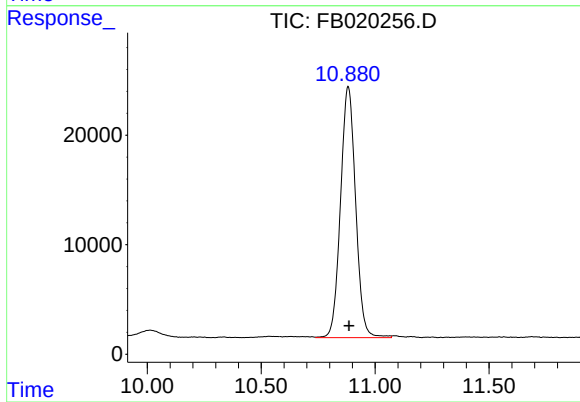


#6 Toluene

R.T.: 10.882 min
Delta R.T.: -0.003 min
Response: 1054428
Conc: 28.53 ng/ml

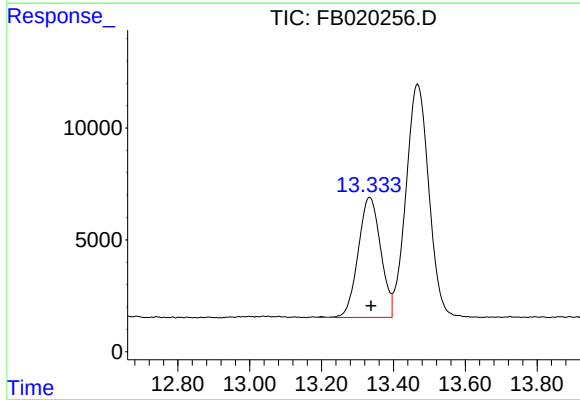


#7 Ethylbenzene

R.T.: 13.334 min
Delta R.T.: -0.003 min
Response: 233174
Conc: 9.91 ng/ml

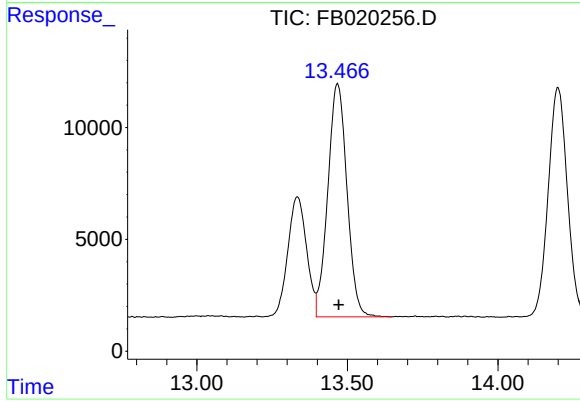

#8 m-Xylene

R.T.: 13.468 min
Delta R.T.: -0.004 min
Response: 461740
Conc: 21.65 ng/ml

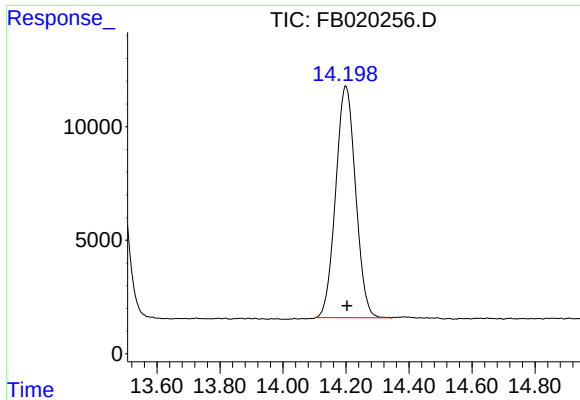


#9 O-Xylene

R.T.: 14.200 min

Delta R.T.: -0.003 min

Response: 446933

Conc: 23.59 ng/ml

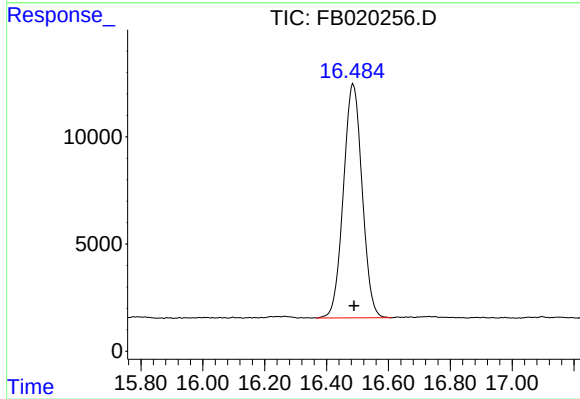

#10 1,2,4-Trimethylbenzene

R.T.: 16.486 min

Delta R.T.: -0.003 min

Response: 459182

Conc: 23.15 ng/ml