

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031819\
 Data File : FB020263.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2019 14:15
 Operator : MJ/SJ
 Sample : K1697-09MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 19 02:31:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	464944	17.710 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	849350	25.178 ng/ml
2) t 2,2,4-Trimethylpentane	7.660	701677	21.396 ng/ml
3) t n-Heptane	7.994	303957	7.304 ng/ml
4) t Benzene	8.132	434960	9.342 ng/ml
6) t Toluene	10.886	940598	25.454 ng/ml
7) t Ethylbenzene	13.339	205968	8.754 ng/ml
8) t m-Xylene	13.472	390107	18.288 ng/ml
9) t O-Xylene	14.204	374269	19.758 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	391589	19.745 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031819\
Data File : FB020263.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2019 14:15
Operator : MJ/SJ
Sample : K1697-09MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 19 02:31:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

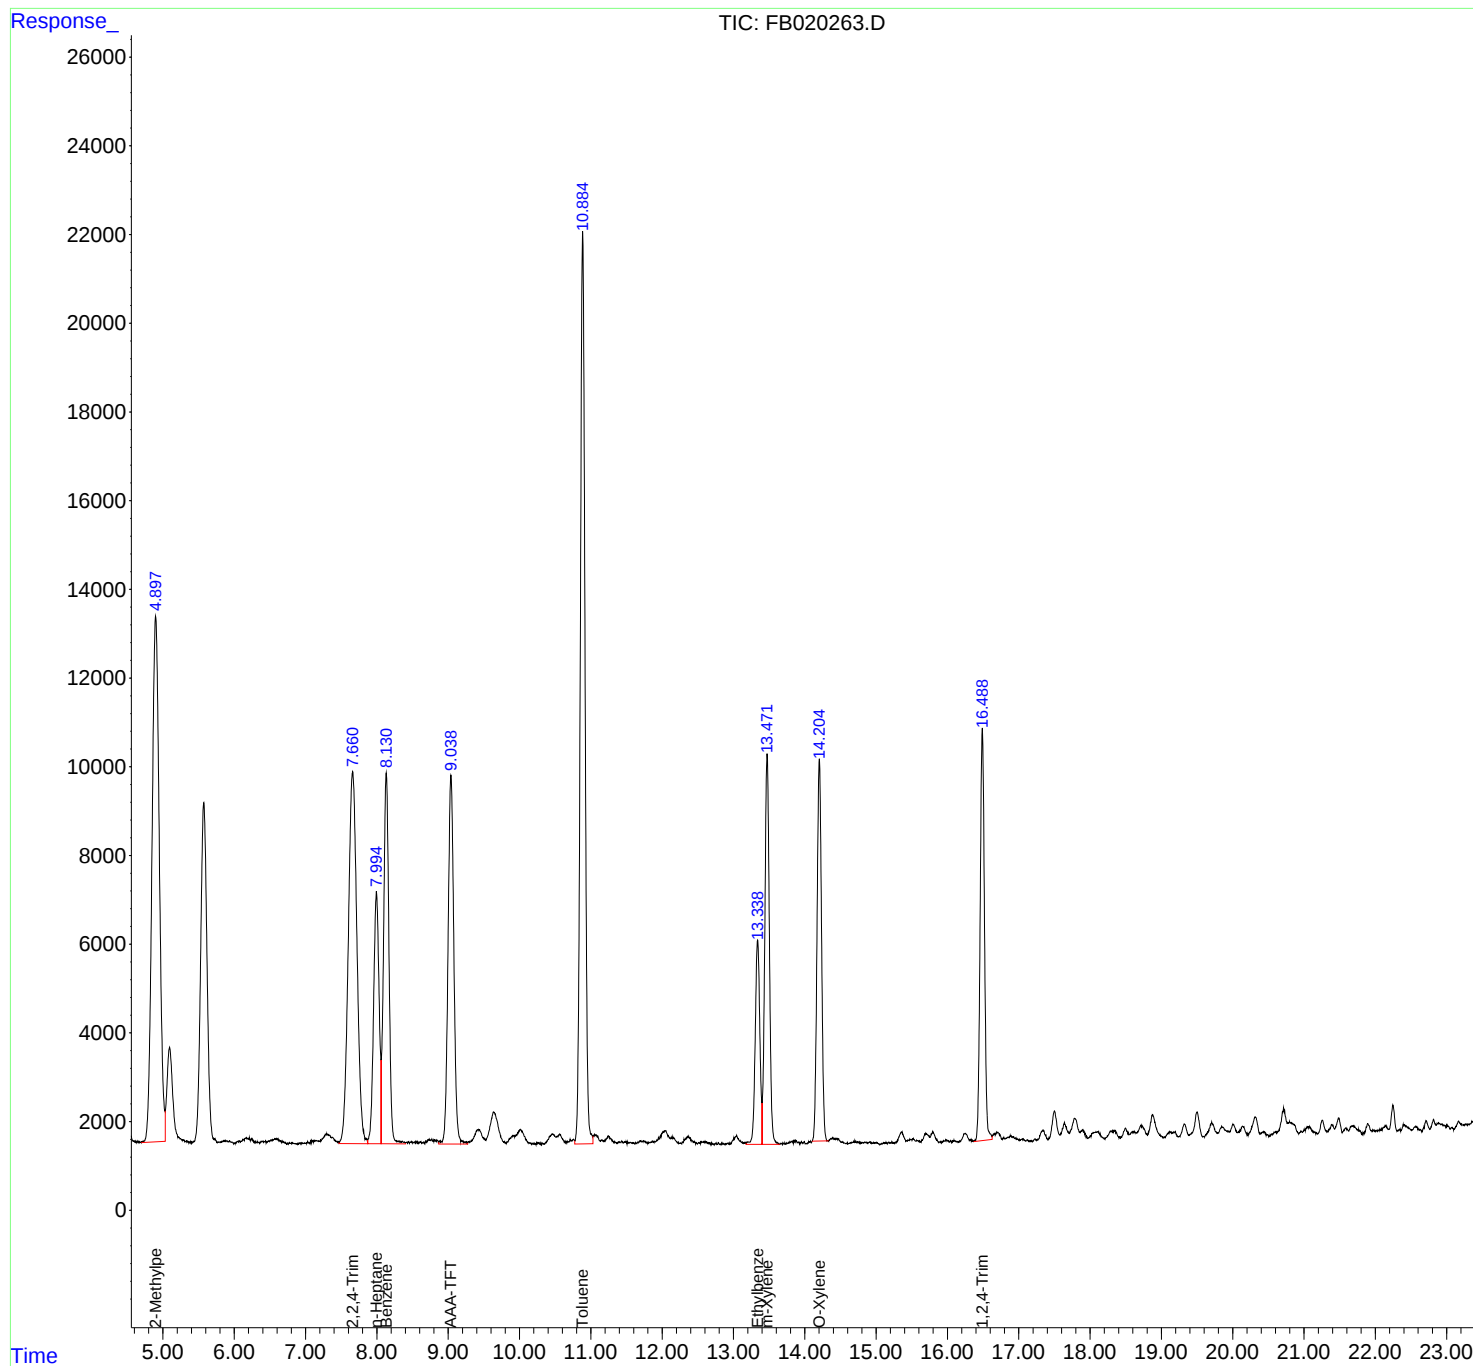

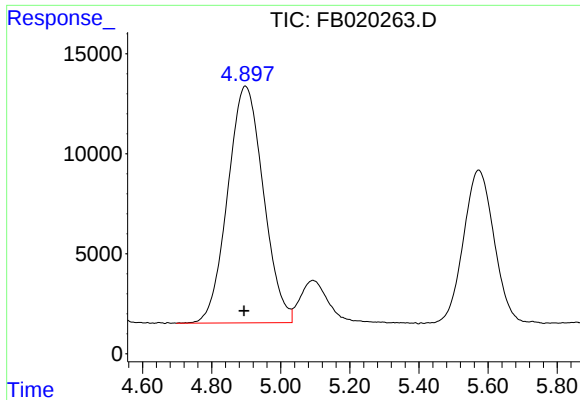


#1 2-Methylpentane

R.T.: 4.898 min

Delta R.T.: 0.004 min

Response: 849350

Conc: 25.18 ng/ml

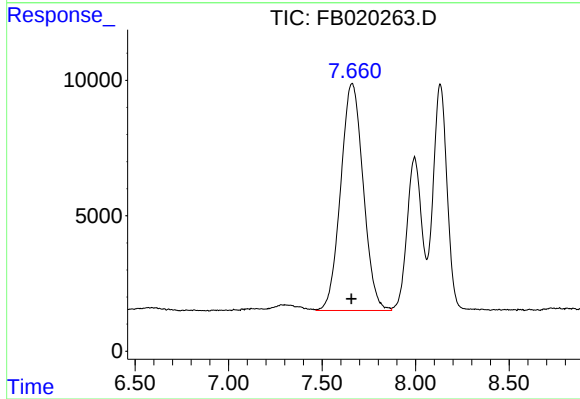


#2 2,2,4-Trimethylpentane

R.T.: 7.660 min

Delta R.T.: 0.003 min

Response: 701677

Conc: 21.40 ng/ml

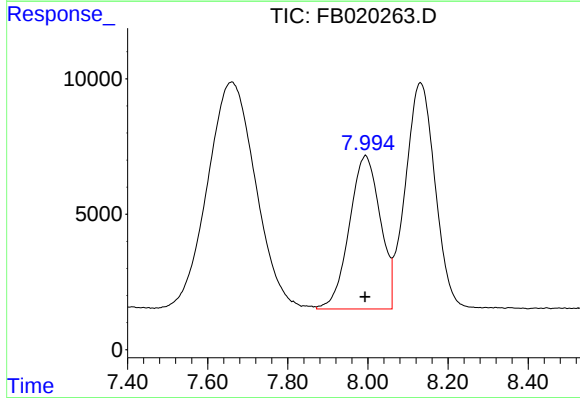


#3 n-Heptane

R.T.: 7.994 min

Delta R.T.: 0.002 min

Response: 303957

Conc: 7.30 ng/ml

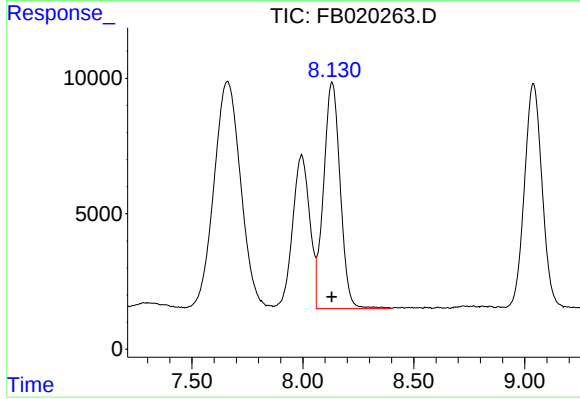


#4 Benzene

R.T.: 8.132 min

Delta R.T.: 0.002 min


Response: 434960

Conc: 9.34 ng/ml

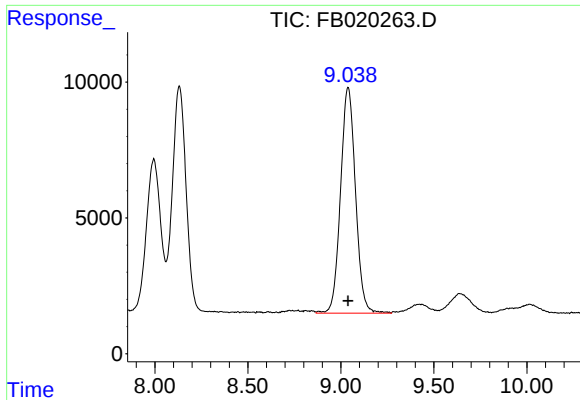


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.001 min
Response: 464944
Conc: 17.71 ng/ml

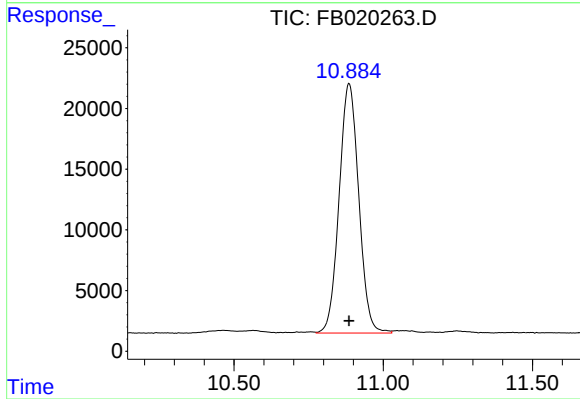


#6 Toluene

R.T.: 10.886 min
Delta R.T.: 0.000 min
Response: 940598
Conc: 25.45 ng/ml

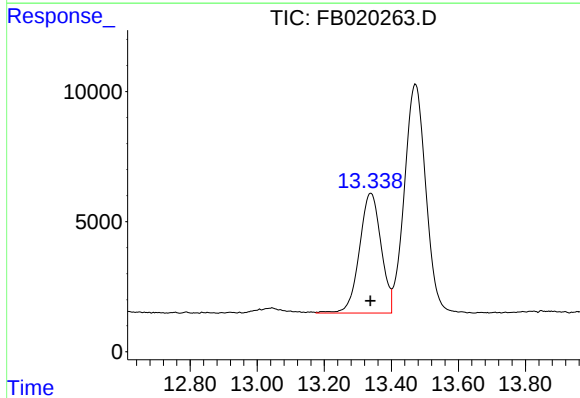


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: 0.001 min
Response: 205968
Conc: 8.75 ng/ml

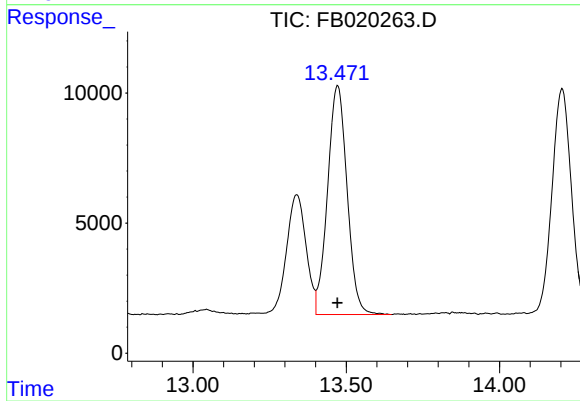


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: 0.000 min
Response: 390107
Conc: 18.29 ng/ml

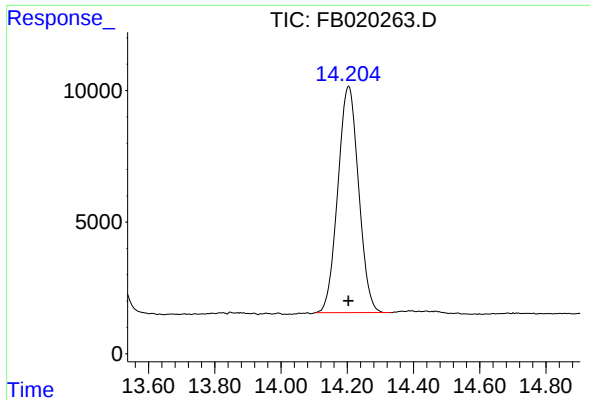

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.001 min
Response: 374269
Conc: 19.76 ng/ml

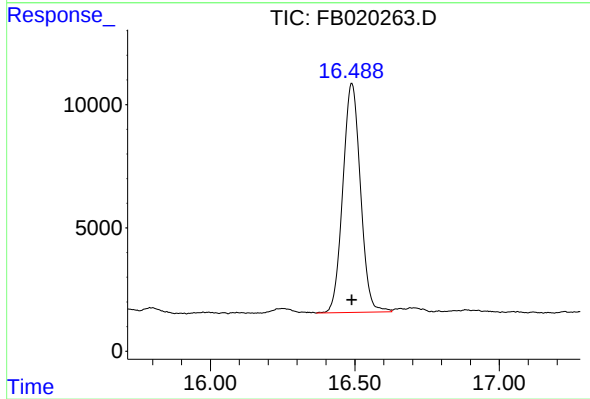

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: 0.000 min
Response: 391589
Conc: 19.75 ng/ml