

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031820\
 Data File : FB023984.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2020 13:47
 Operator : DD/AJ
 Sample : L1954-02MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 18 15:03:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	434569	20.644 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	829018	26.825 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	824168	24.441 ng/ml
3) t n-Heptane	7.755	267091	8.062 ng/ml
4) t Benzene	7.889	419234	10.012 ng/ml
6) t Toluene	10.626	1212608	29.740 ng/ml
7) t Ethylbenzene	13.067	368535	9.646 ng/ml
8) t m-Xylene	13.199	711131	19.315 ng/ml
9) t O-Xylene	13.927	687542	19.332 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	574780	18.973 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031820\
Data File : FB023984.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2020 13:47
Operator : DD/AJ
Sample : L1954-02MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 18 15:03:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

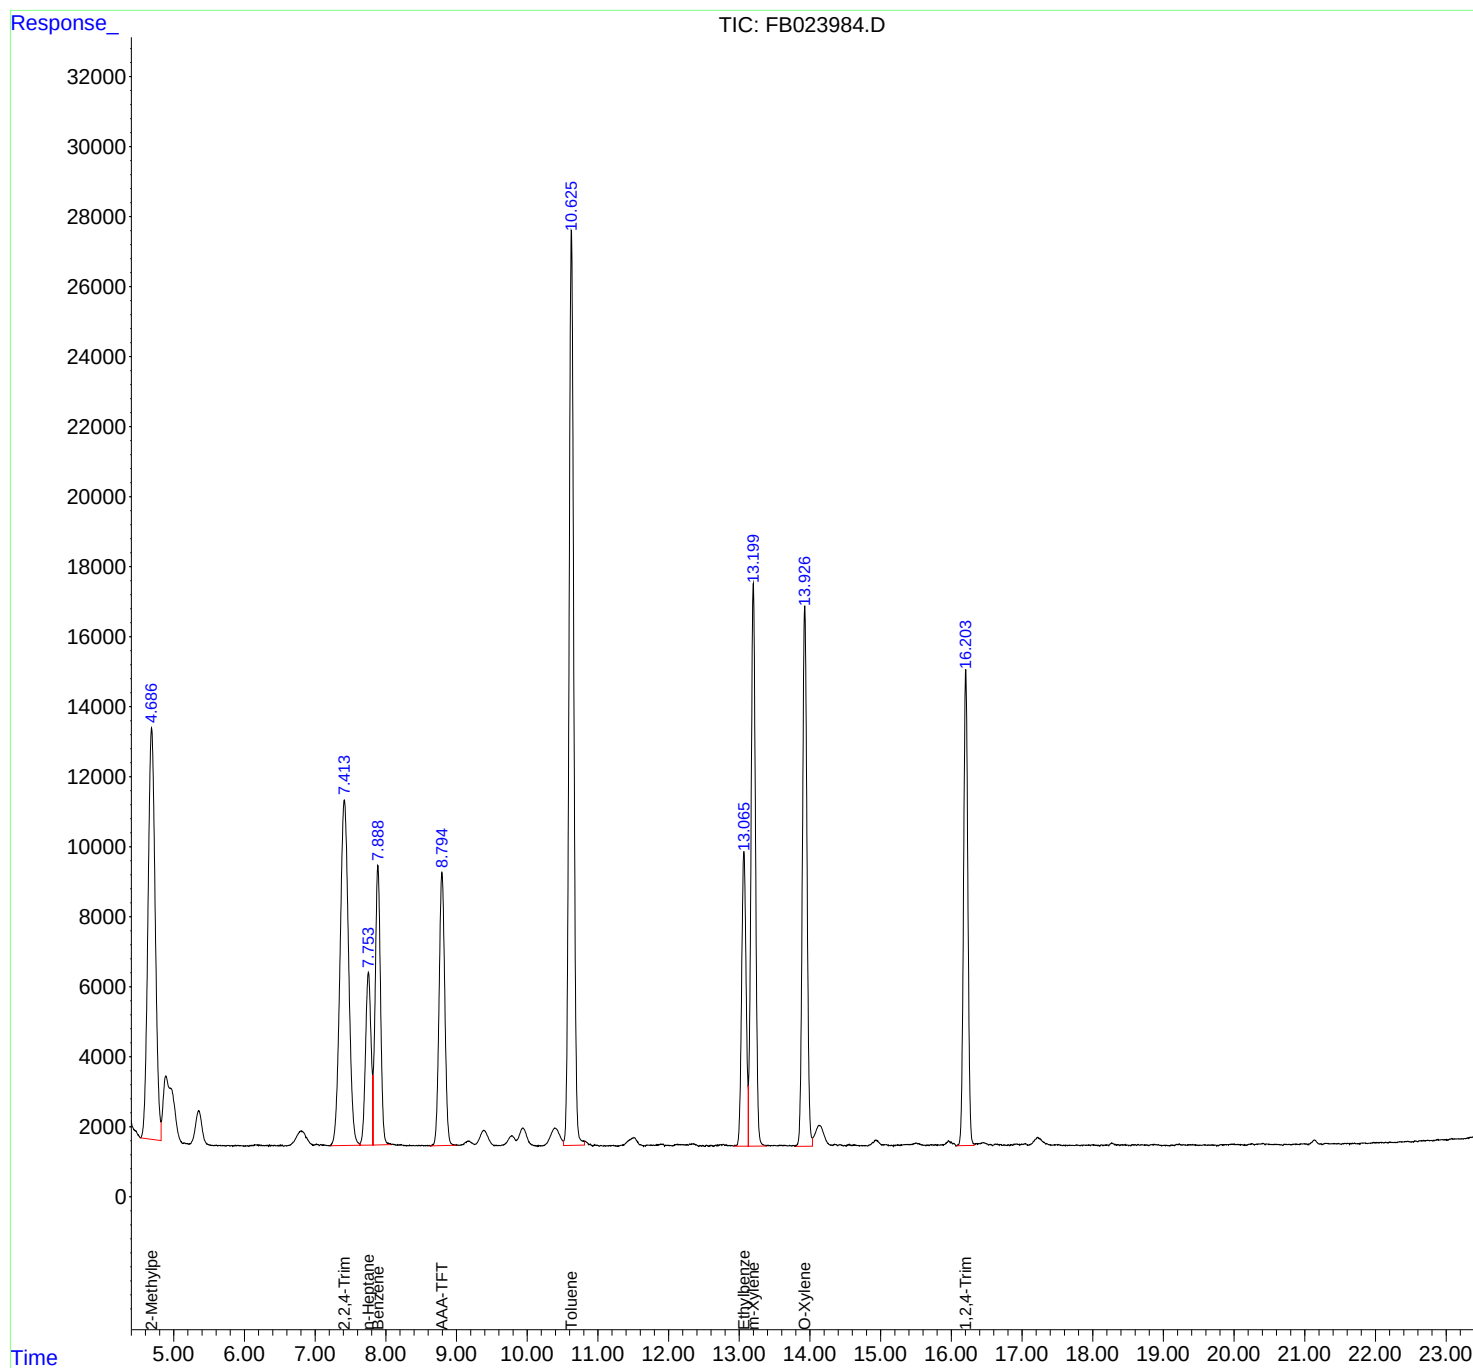

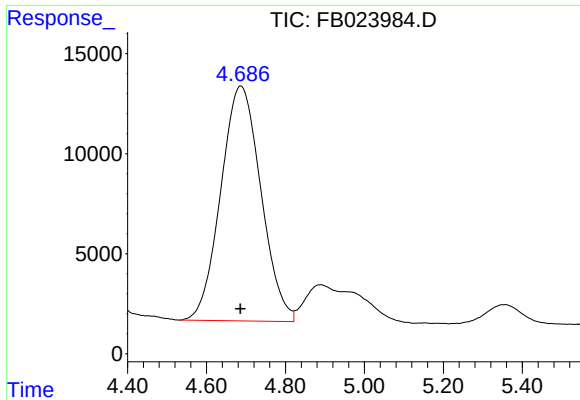


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.001 min
Response: 829018
Conc: 26.82 ng/ml

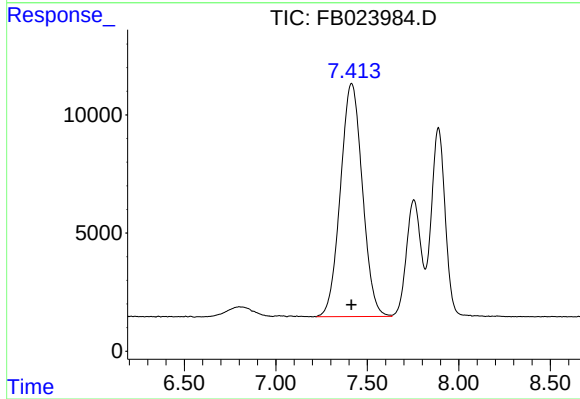


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.001 min
Response: 824168
Conc: 24.44 ng/ml

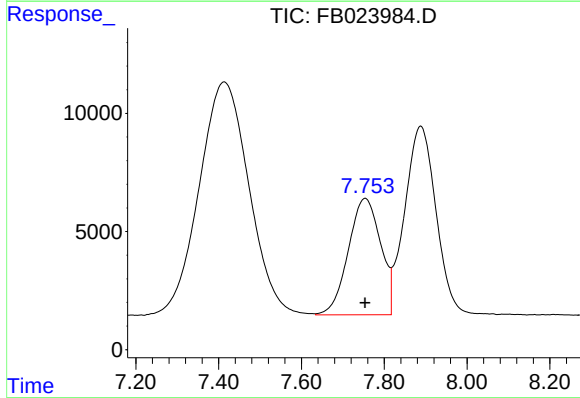


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.001 min
Response: 267091
Conc: 8.06 ng/ml

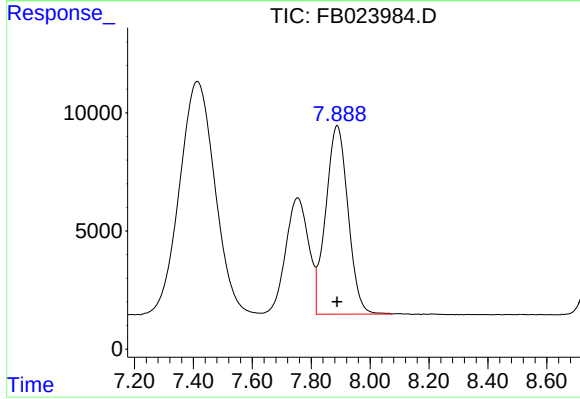


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 419234
Conc: 10.01 ng/ml

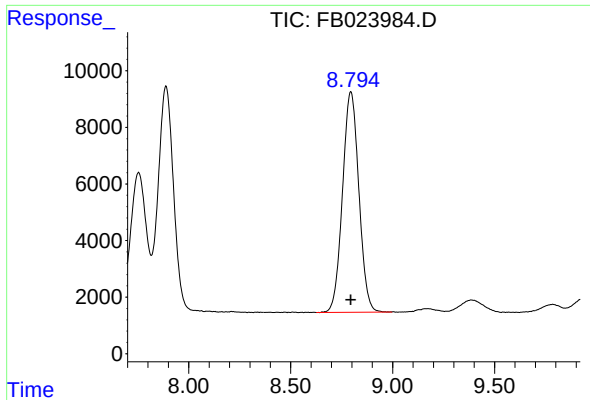


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 434569
Conc: 20.64 ng/ml

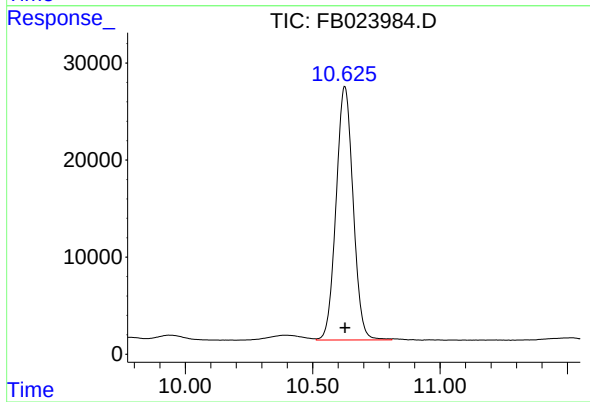


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.000 min
Response: 1212608
Conc: 29.74 ng/ml

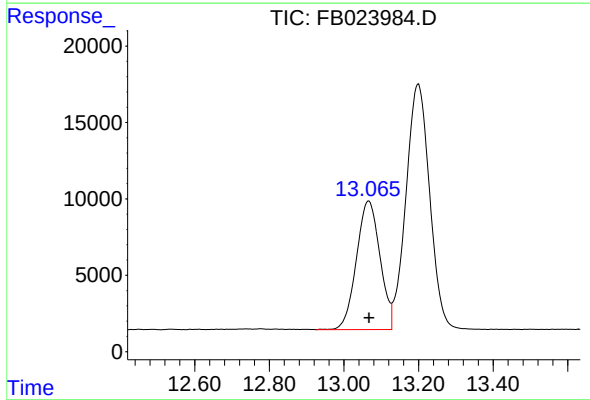


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 368535
Conc: 9.65 ng/ml

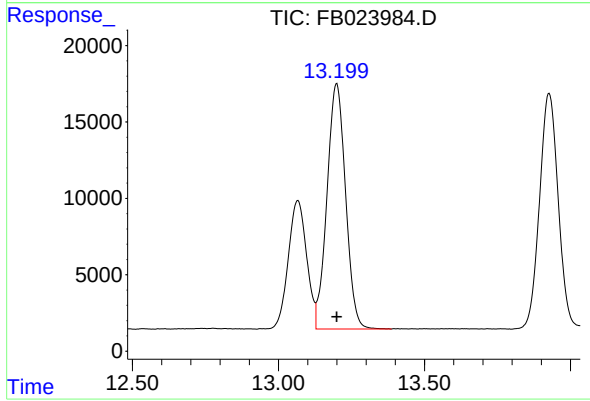


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: 0.000 min
Response: 711131
Conc: 19.32 ng/ml

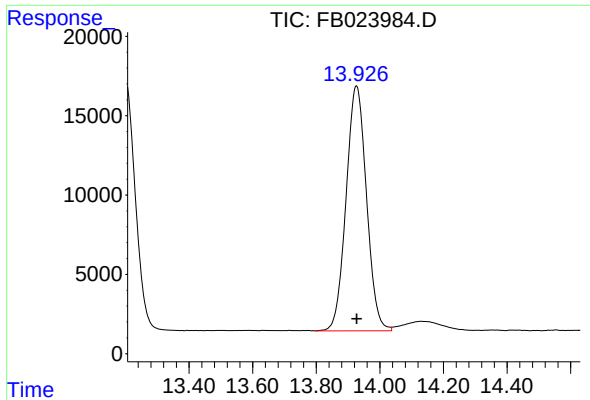

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.000 min
Response: 687542
Conc: 19.33 ng/ml

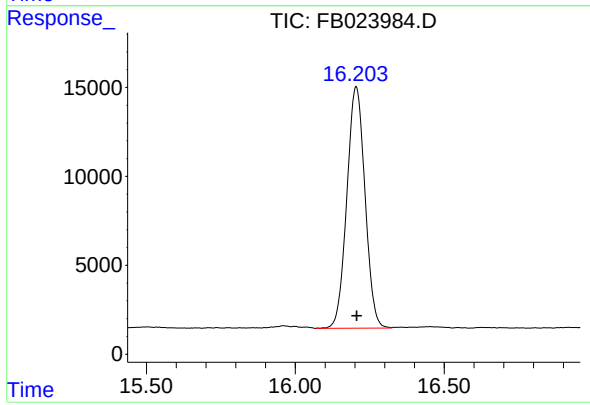

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.001 min
Response: 574780
Conc: 18.97 ng/ml