

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB031820\  
Data File : FB023986.D  
Signal(s) : FID2B.CH  
Acq On : 18 Mar 2020 15:39  
Operator : DD/AJ  
Sample : L1964-02  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Mar 18 16:02:04 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030520.M  
Quant Title :  
QLast Update : Thu Mar 05 11:03:12 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.794  | 432750   | 20.558 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.679  | 6540     | 0.212 ng/ml  |
| 6) t Toluene                 | 10.641 | 2942     | 0.072 ng/ml  |
| 8) t m-Xylene                | 13.174 | 1567     | 0.043 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.208 | 1604     | 0.053 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB031820\  
Data File : FB023986.D  
Signal(s) : FID2B.CH  
Acq On : 18 Mar 2020 15:39  
Operator : DD/AJ  
Sample : L1964-02  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Mar 18 16:02:04 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030520.M  
Quant Title :  
QLast Update : Thu Mar 05 11:03:12 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

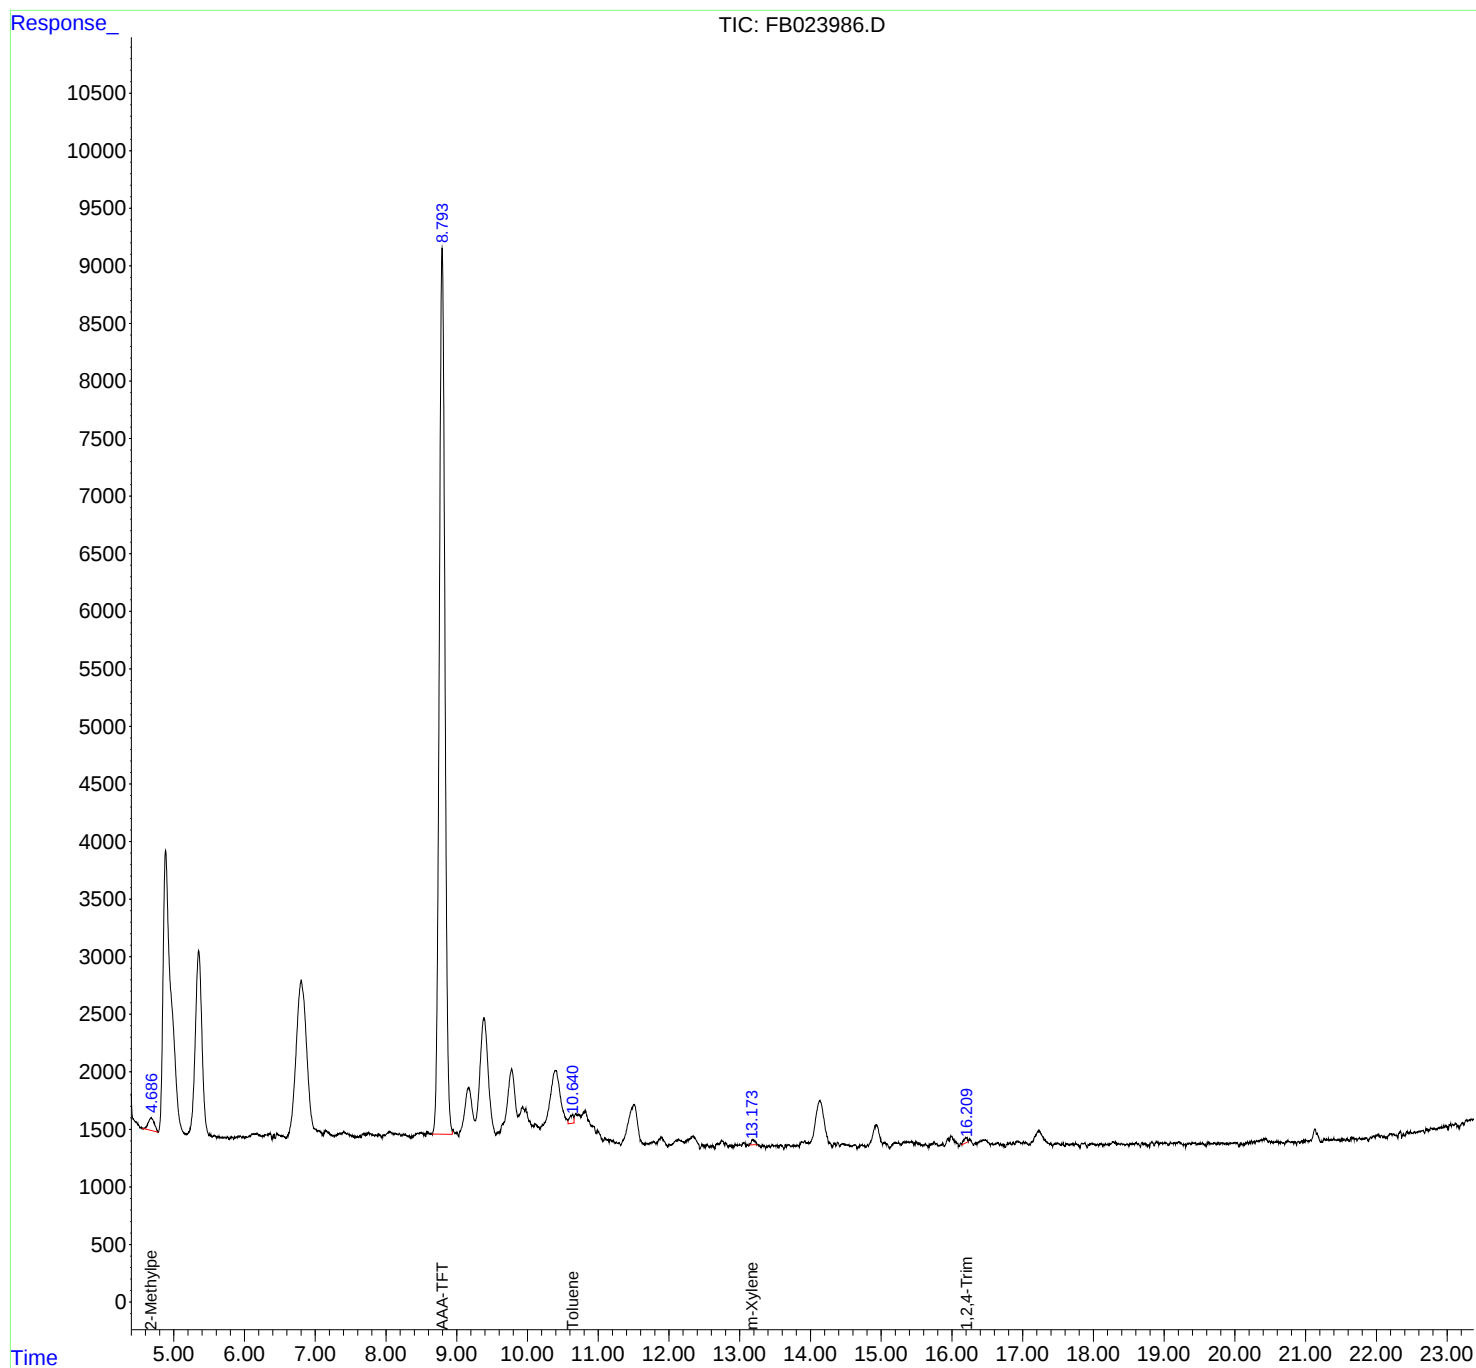

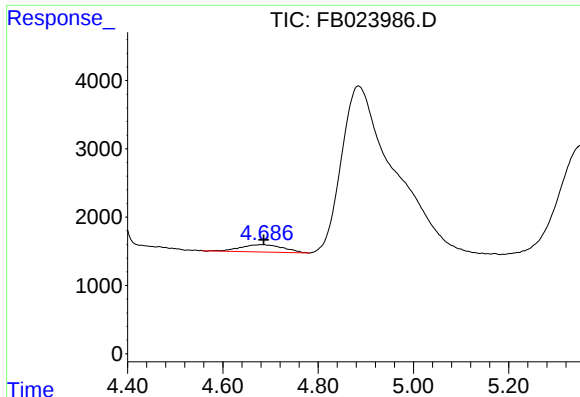


#1 2-Methylpentane

R.T.: 4.679 min  
Delta R.T.: -0.007 min  
Response: 6540  
Conc: 0.21 ng/ml

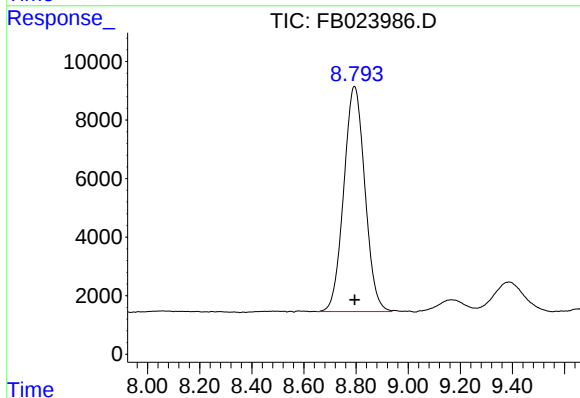


#5 AAA-TFT

R.T.: 8.794 min  
Delta R.T.: 0.000 min  
Response: 432750  
Conc: 20.56 ng/ml

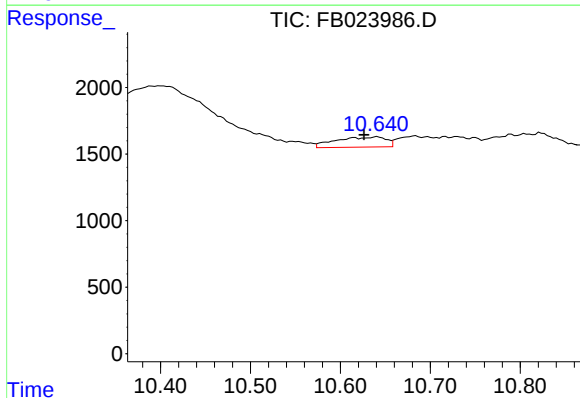


#6 Toluene

R.T.: 10.641 min  
Delta R.T.: 0.015 min  
Response: 2942  
Conc: 0.07 ng/ml

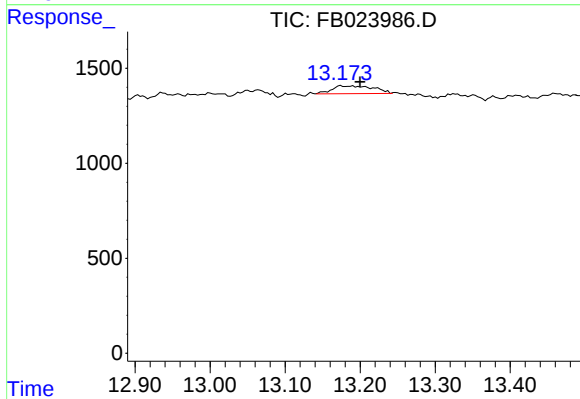

#8 m-Xylene

R.T.: 13.174 min  
Delta R.T.: -0.025 min  
Response: 1567  
Conc: 0.04 ng/ml

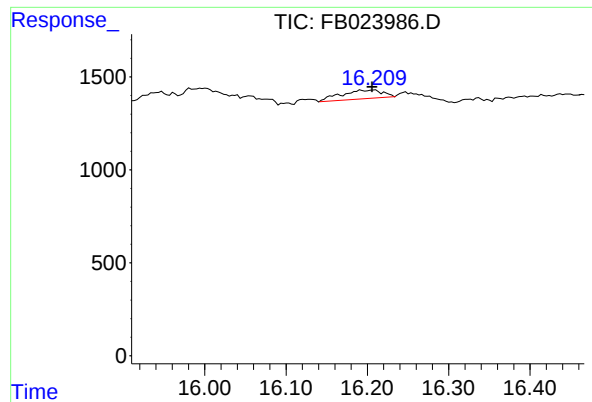

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min  
Delta R.T.: 0.003 min  
Response: 1604  
Conc: 0.05 ng/ml