

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031820\
 Data File : FB023979.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2020 9:45
 Operator : DD/AJ
 Sample : BSF0318S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 18 15:03:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	422065	20.050 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	929306	30.070 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1056947	31.344 ng/ml
3) t n-Heptane	7.753	337676	10.193 ng/ml
4) t Benzene	7.888	417253	9.965 ng/ml
6) t Toluene	10.625	1220163	29.925 ng/ml
7) t Ethylbenzene	13.065	385190	10.082 ng/ml
8) t m-Xylene	13.198	746199	20.268 ng/ml
9) t O-Xylene	13.926	711904	20.017 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	609693	20.125 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031820\
Data File : FB023979.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2020 9:45
Operator : DD/AJ
Sample : BSF0318S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 18 15:03:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

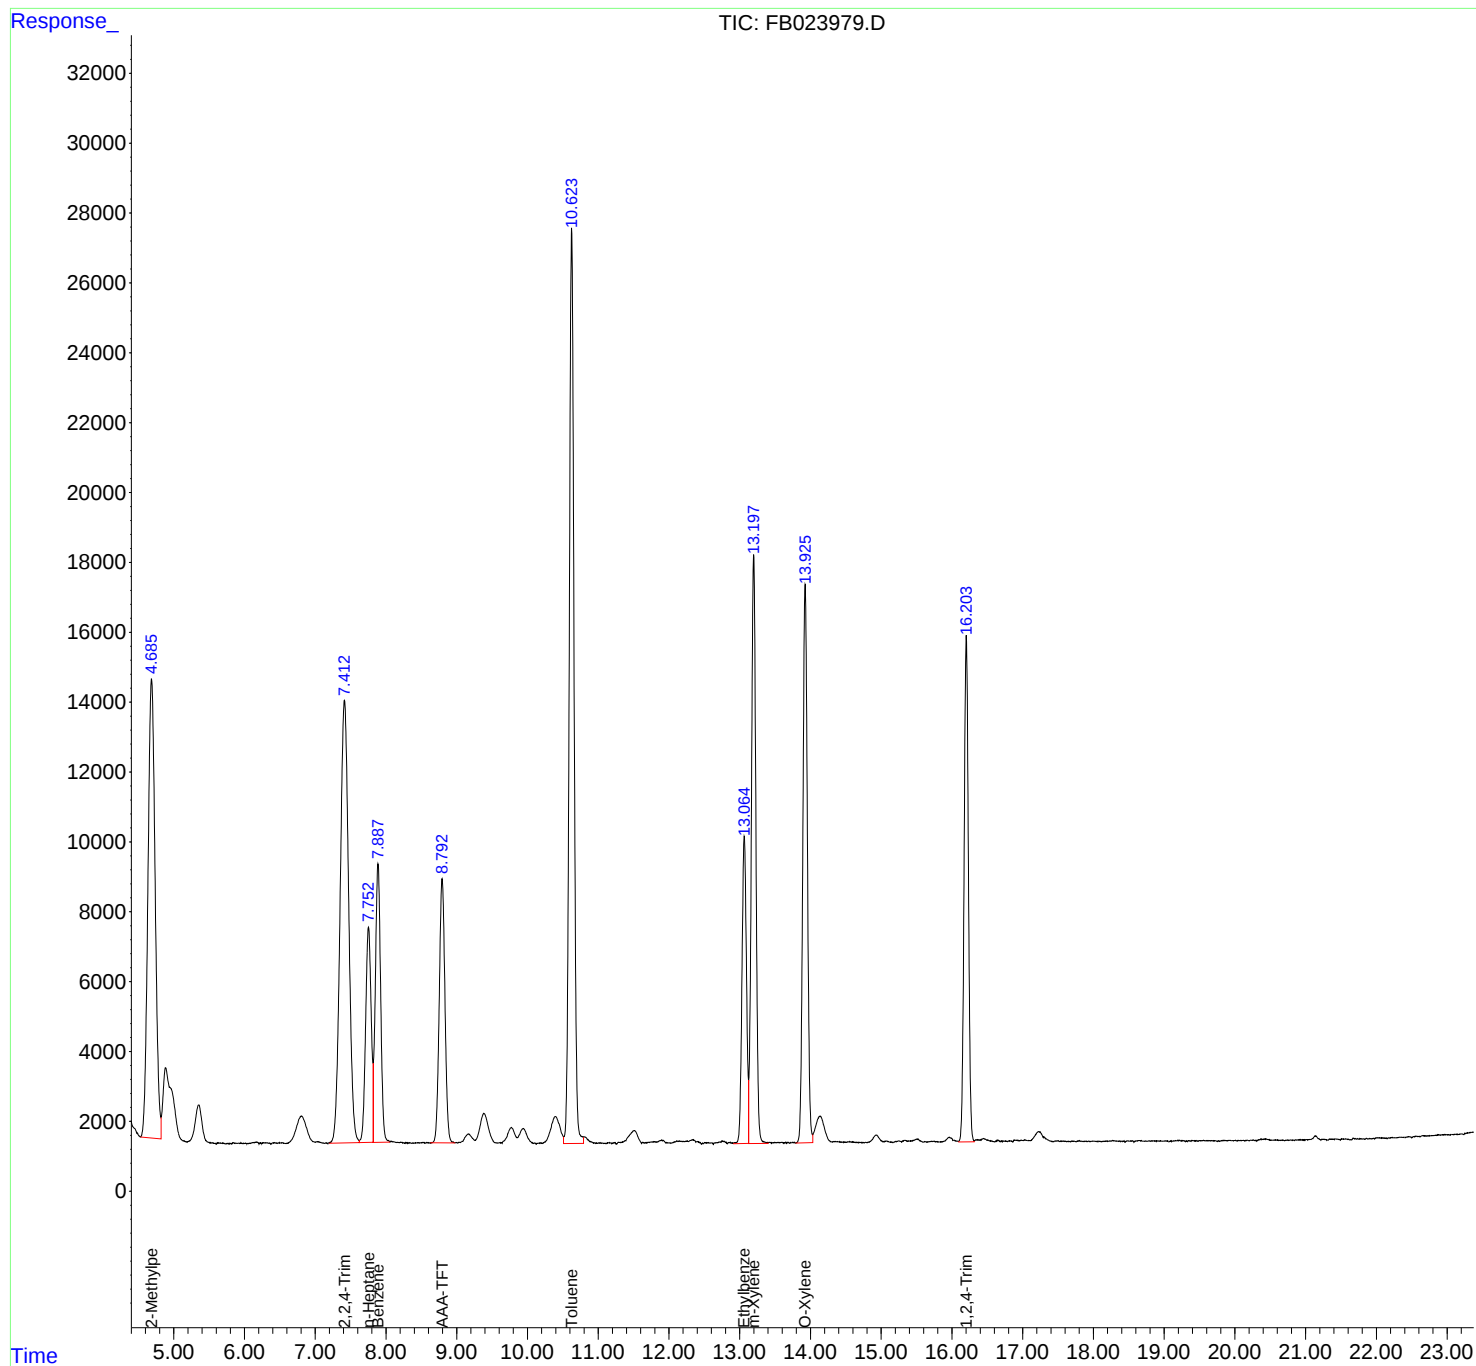

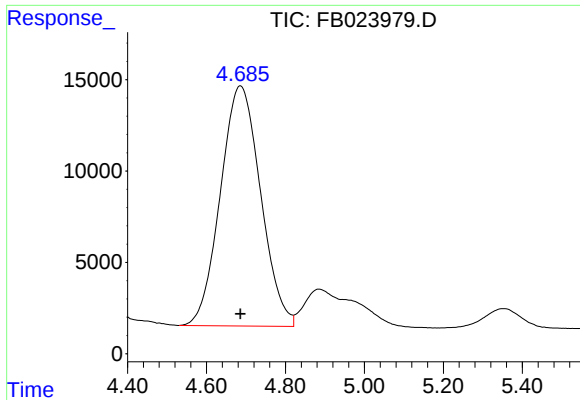


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 929306
Conc: 30.07 ng/ml

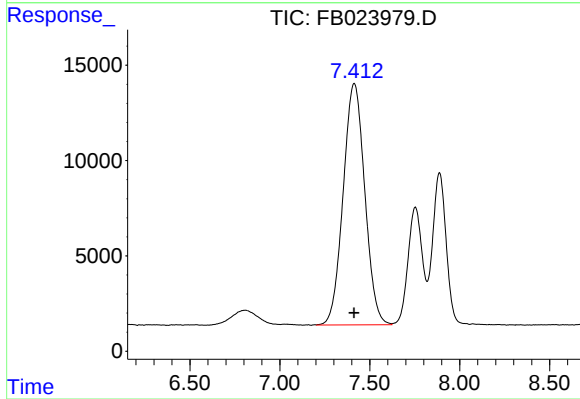


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.000 min
Response: 1056947
Conc: 31.34 ng/ml

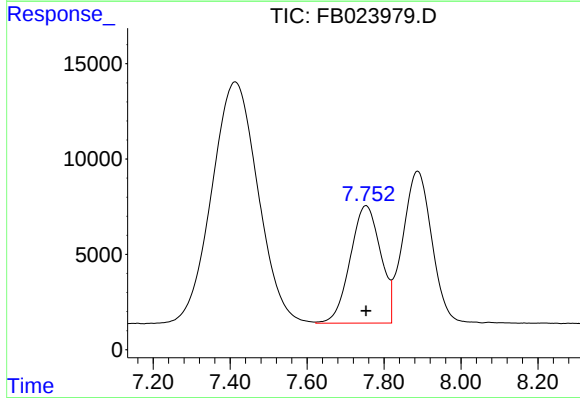


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 337676
Conc: 10.19 ng/ml

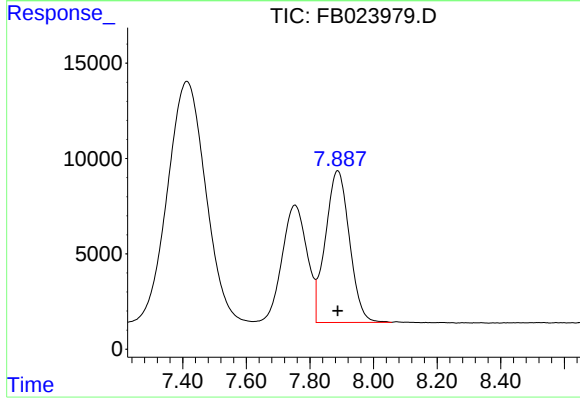


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 417253
Conc: 9.96 ng/ml

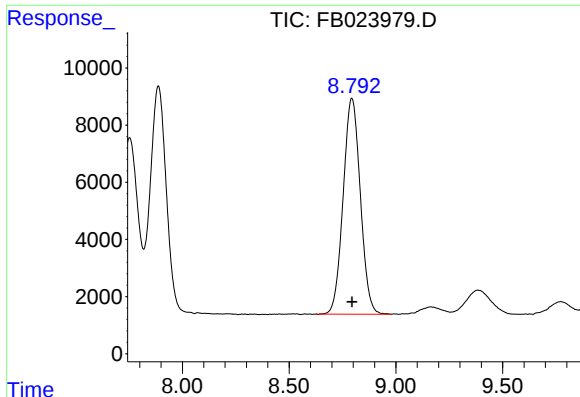


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 422065
Conc: 20.05 ng/ml

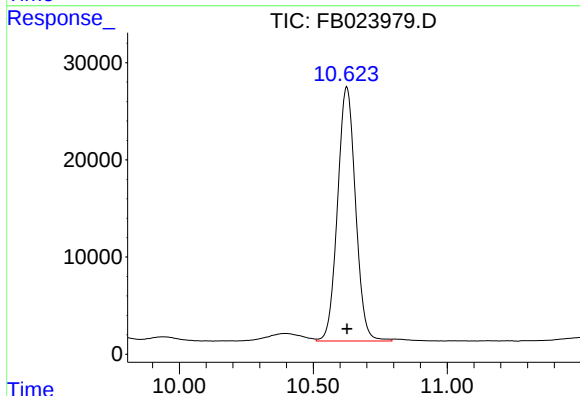


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.001 min
Response: 1220163
Conc: 29.93 ng/ml

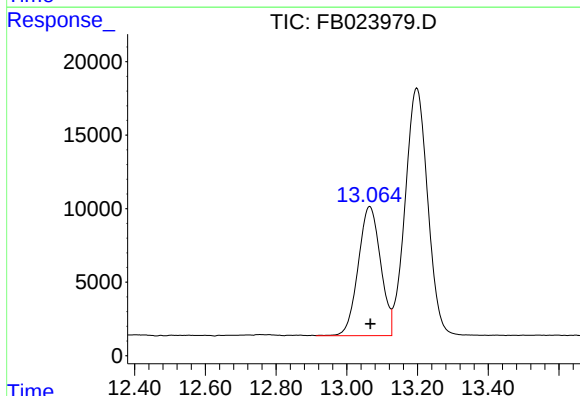


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.002 min
Response: 385190
Conc: 10.08 ng/ml

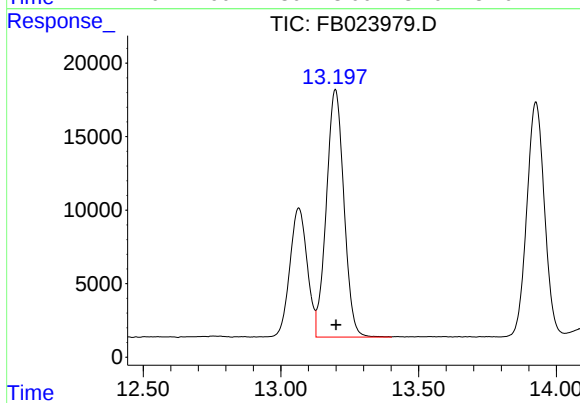


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.002 min
Response: 746199
Conc: 20.27 ng/ml

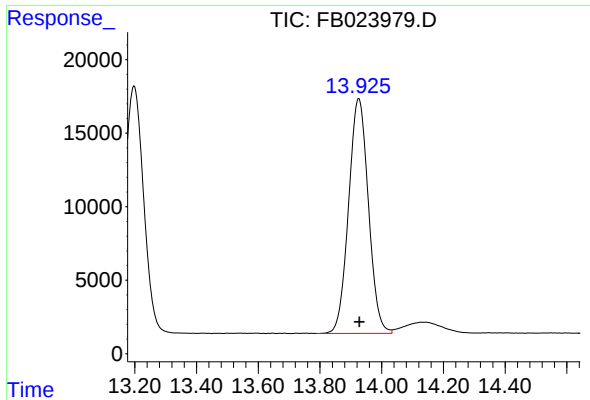

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.002 min
Response: 711904
Conc: 20.02 ng/ml

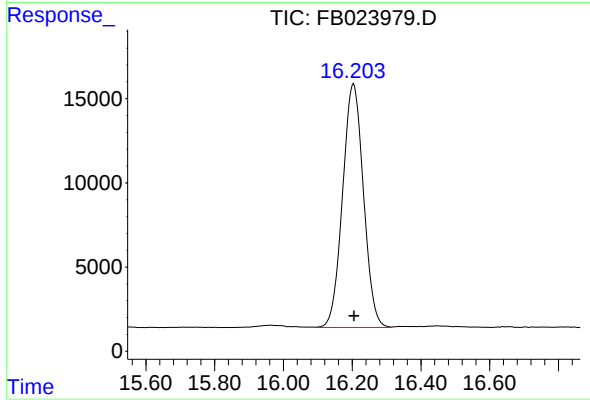

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.002 min
Response: 609693
Conc: 20.13 ng/ml