

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031821\
 Data File : FB025544.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2021 13:34
 Operator : DD/AJ
 Sample : BSF0318S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 19 01:06:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
 Quant Title :
 QLast Update : Wed Mar 17 08:44:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	467975	22.356 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	1029363	34.546 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1134950	35.781 ng/ml
3) t n-Heptane	7.761	369286	11.897 ng/ml
4) t Benzene	7.896	445745	11.471 ng/ml
6) t Toluene	10.634	1289539	34.151 ng/ml
7) t Ethylbenzene	13.074	398673	11.540 ng/ml
8) t m-Xylene	13.207	791144	23.064 ng/ml
9) t O-Xylene	13.934	757524	22.875 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	670498	23.234 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031821\
Data File : FB025544.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2021 13:34
Operator : DD/AJ
Sample : BSF0318S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 19 01:06:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
Quant Title :
QLast Update : Wed Mar 17 08:44:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

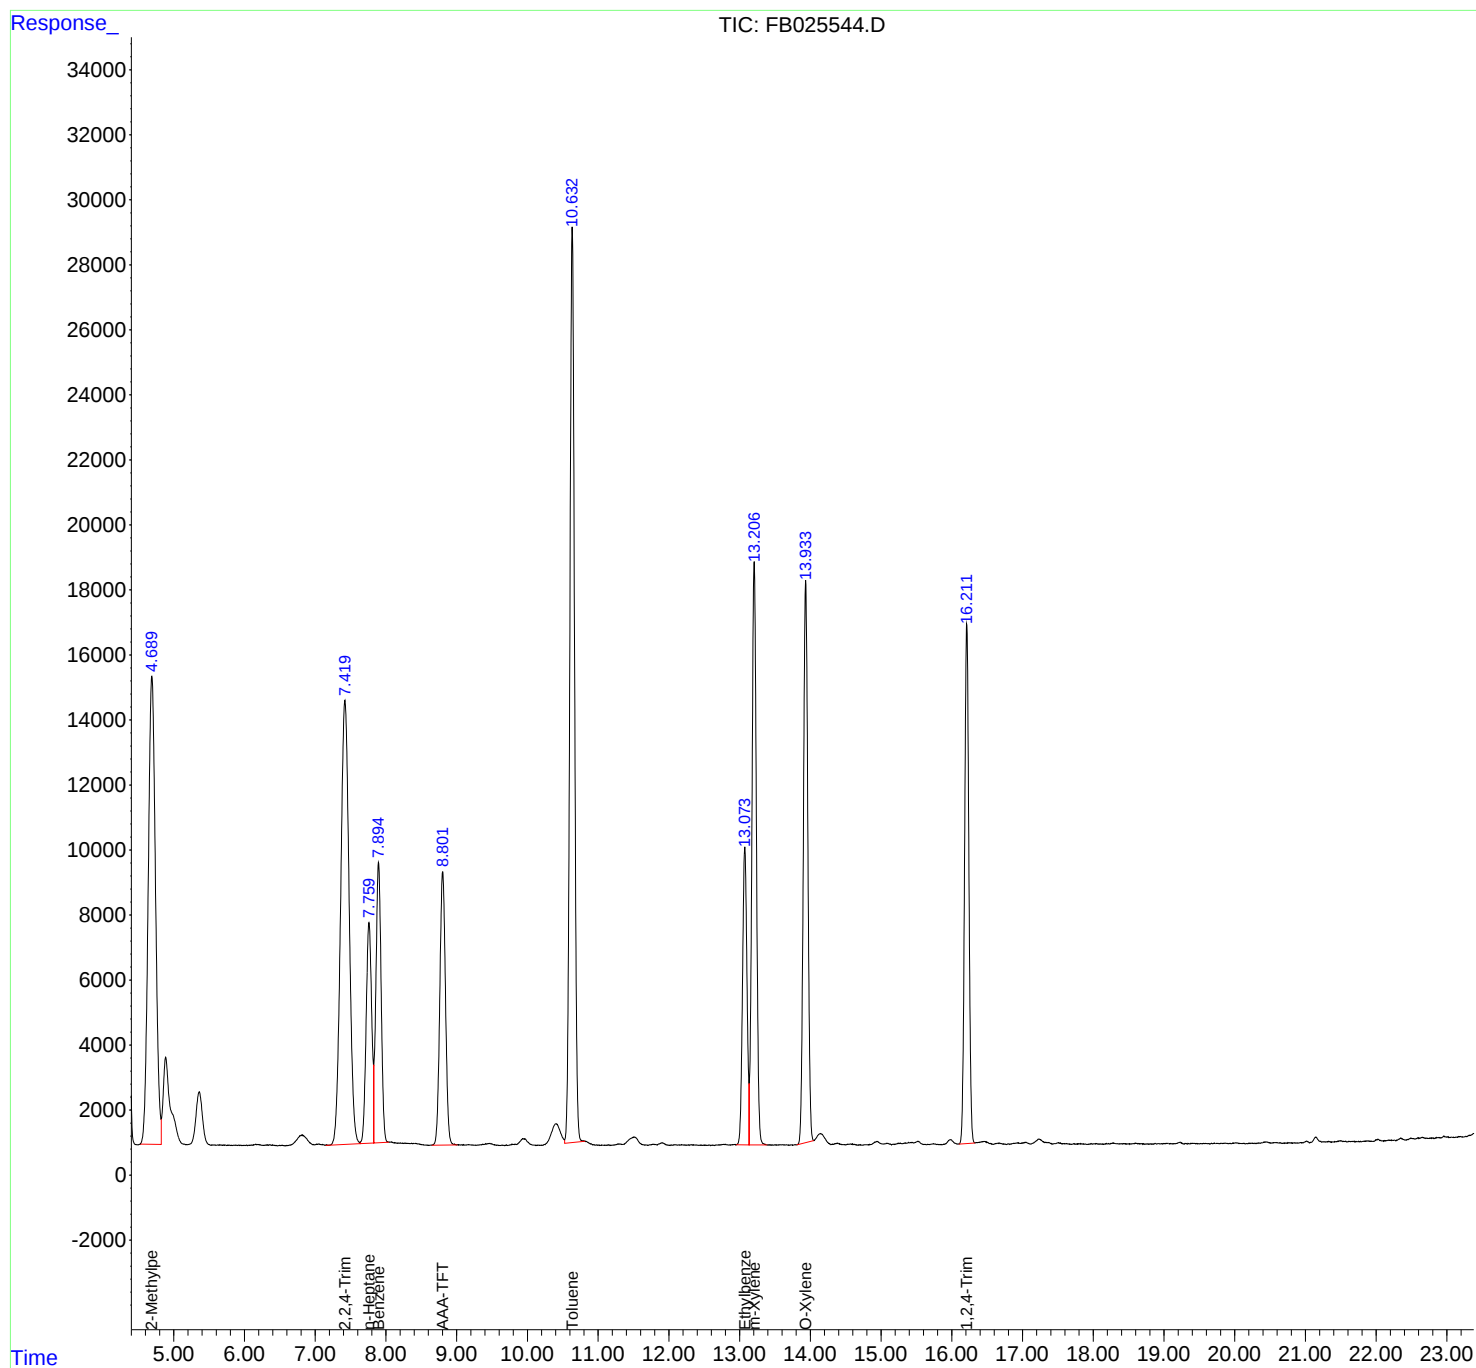

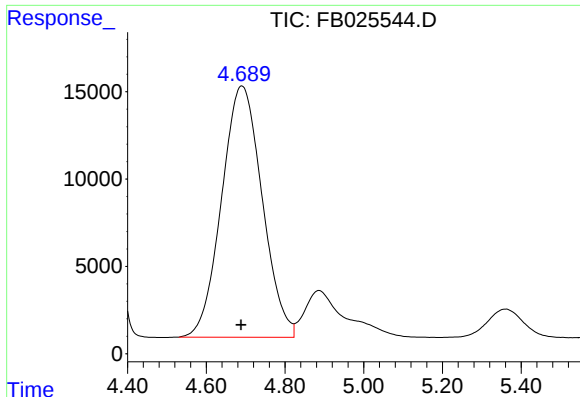


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.003 min
Response: 1029363
Conc: 34.55 ng/ml

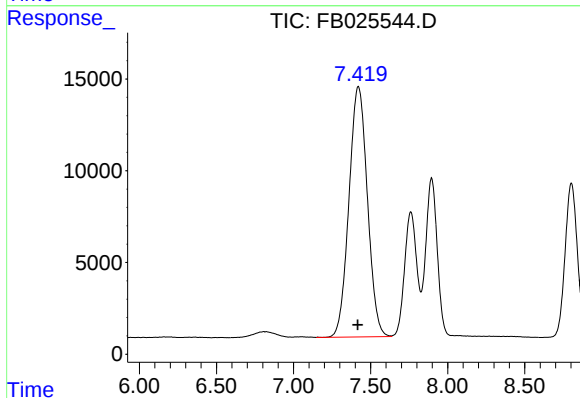


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.003 min
Response: 1134950
Conc: 35.78 ng/ml

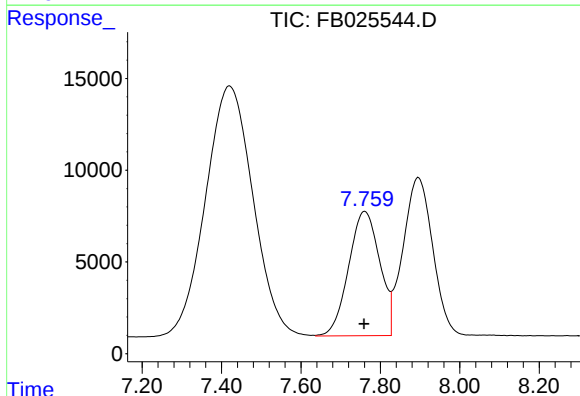


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 369286
Conc: 11.90 ng/ml

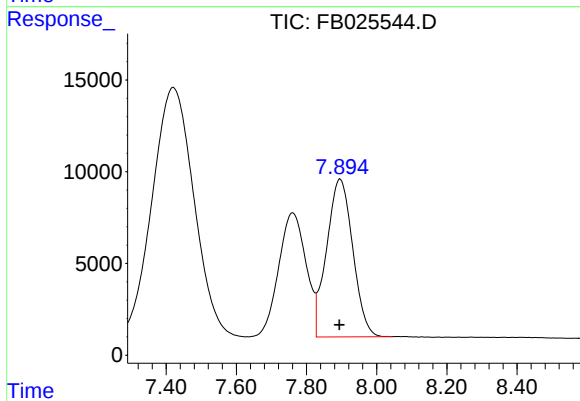


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.002 min
Response: 445745
Conc: 11.47 ng/ml

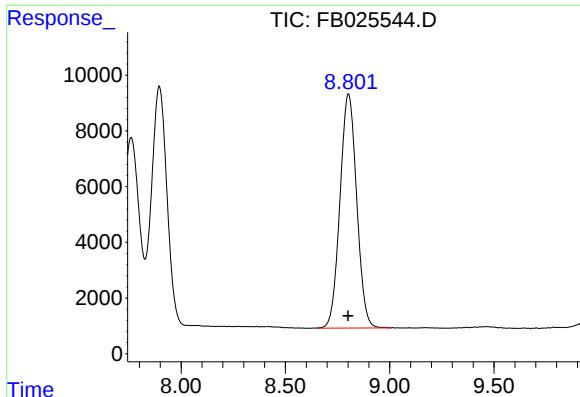


#5 AAA-TFT

R.T.: 8.803 min
Delta R.T.: 0.002 min
Response: 467975
Conc: 22.36 ng/ml

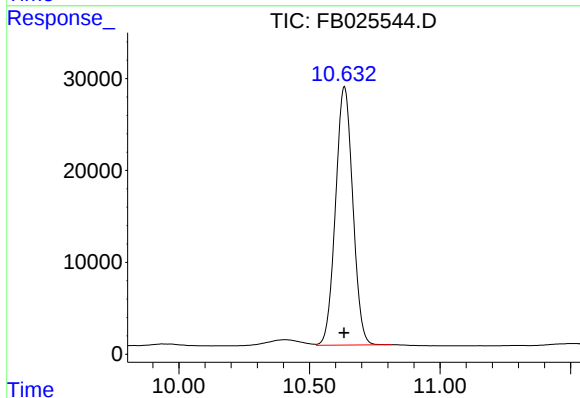


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.002 min
Response: 1289539
Conc: 34.15 ng/ml

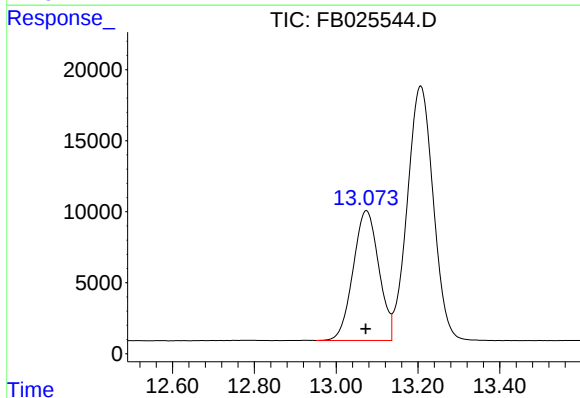


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.002 min
Response: 398673
Conc: 11.54 ng/ml

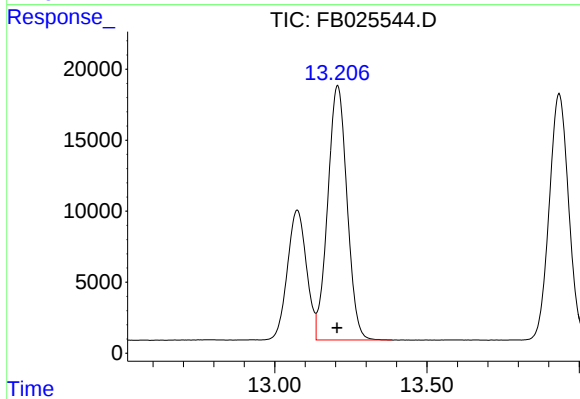


#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.002 min
Response: 791144
Conc: 23.06 ng/ml

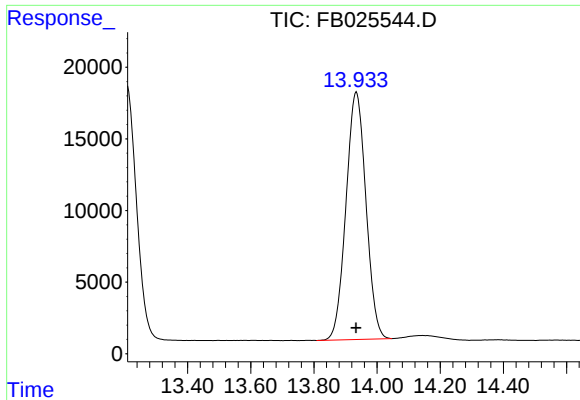

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 757524
Conc: 22.87 ng/ml

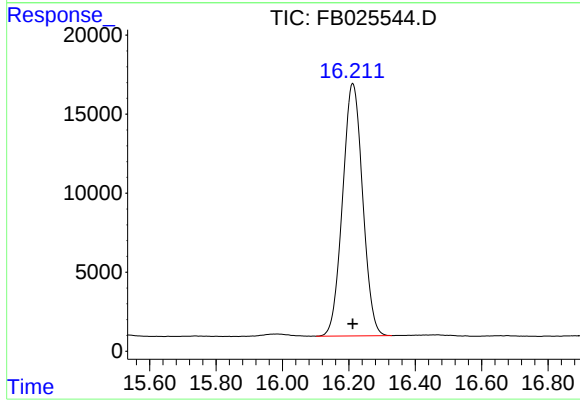

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.001 min
Response: 670498
Conc: 23.23 ng/ml