

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
 Data File : FB026734.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2022 9:18
 Operator : AJ/MA
 Sample : N2007-01
 Misc : 5.81G/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 18 22:43:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	150051	14.299 ng/ml
Target Compounds			
8) t m-Xylene	13.186	4090	0.203 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	4754	0.239 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
Data File : FB026734.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2022 9:18
Operator : AJ/MA
Sample : N2007-01
Misc : 5.81G/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 18 22:43:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

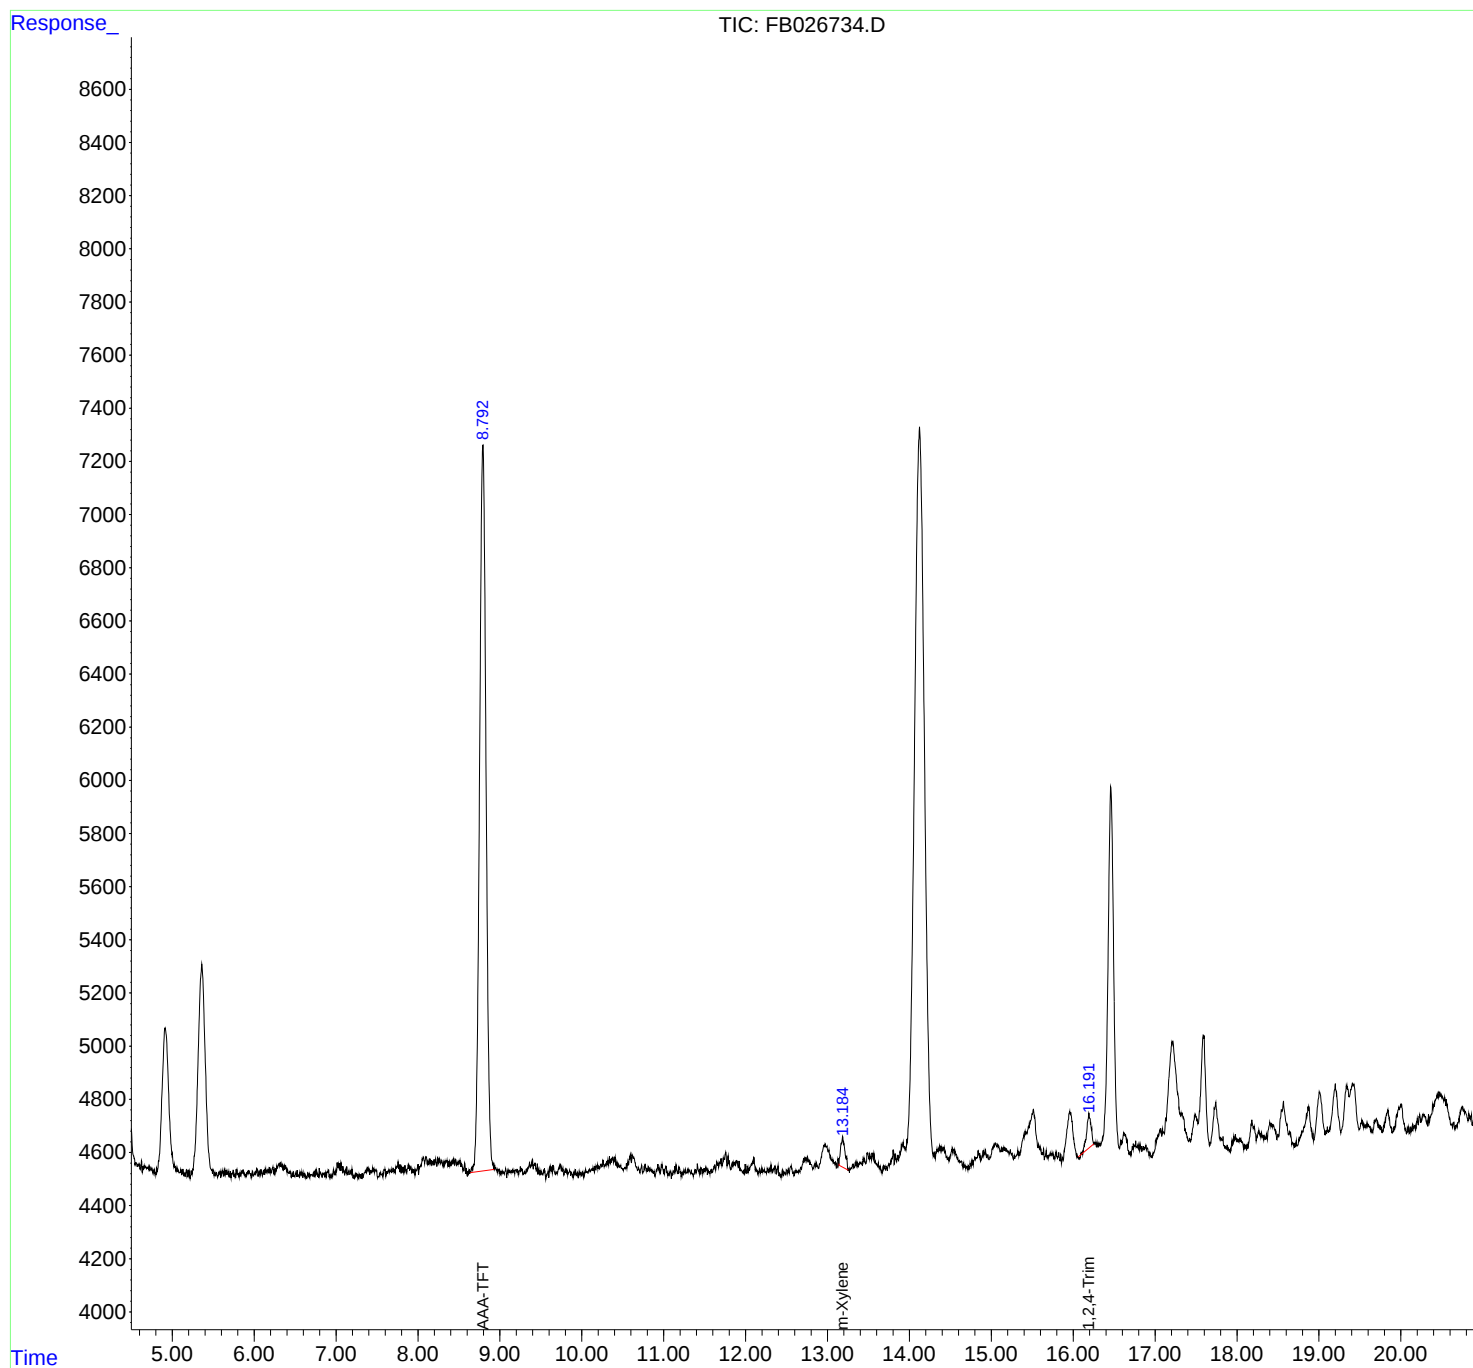


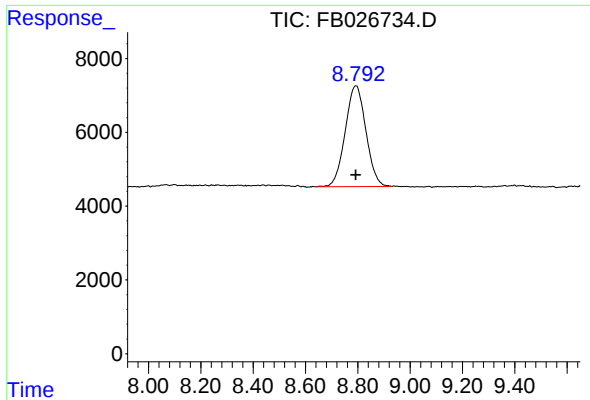

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 150051
Conc: 14.30 ng/ml

Instrument :
FID_B
ClientSampleId :

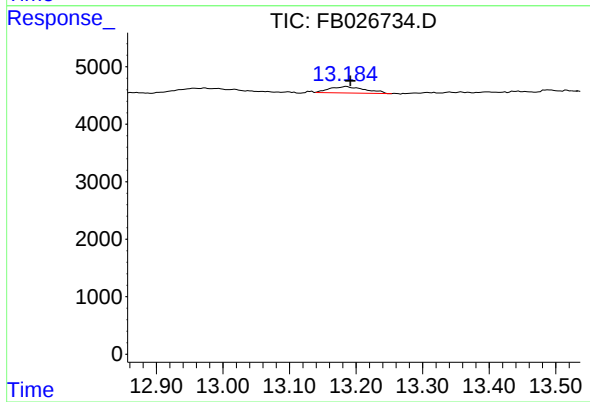

#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.006 min
Response: 4090
Conc: 0.20 ng/ml

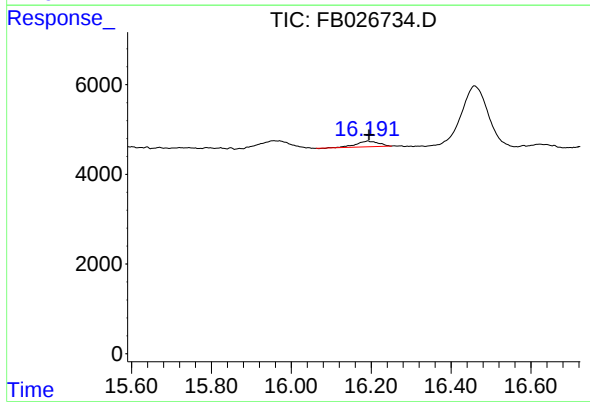

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.002 min
Response: 4754
Conc: 0.24 ng/ml