

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
 Data File : FB026740.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2022 14:18
 Operator : AJ/MA
 Sample : N1970-02MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 18 22:44:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	153412	14.620 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	352253	18.605 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	413236	19.937 ng/ml
3) t n-Heptane	7.753	129104	6.523 ng/ml
4) t Benzene	7.890	182624	7.915 ng/ml
6) t Toluene	10.622	520229	23.763 ng/ml
7) t Ethylbenzene	13.058	153617	7.644 ng/ml
8) t m-Xylene	13.191	309225	15.344 ng/ml
9) t O-Xylene	13.918	311831	15.631 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	297520	14.932 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
Data File : FB026740.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2022 14:18
Operator : AJ/MA
Sample : N1970-02MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 18 22:44:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

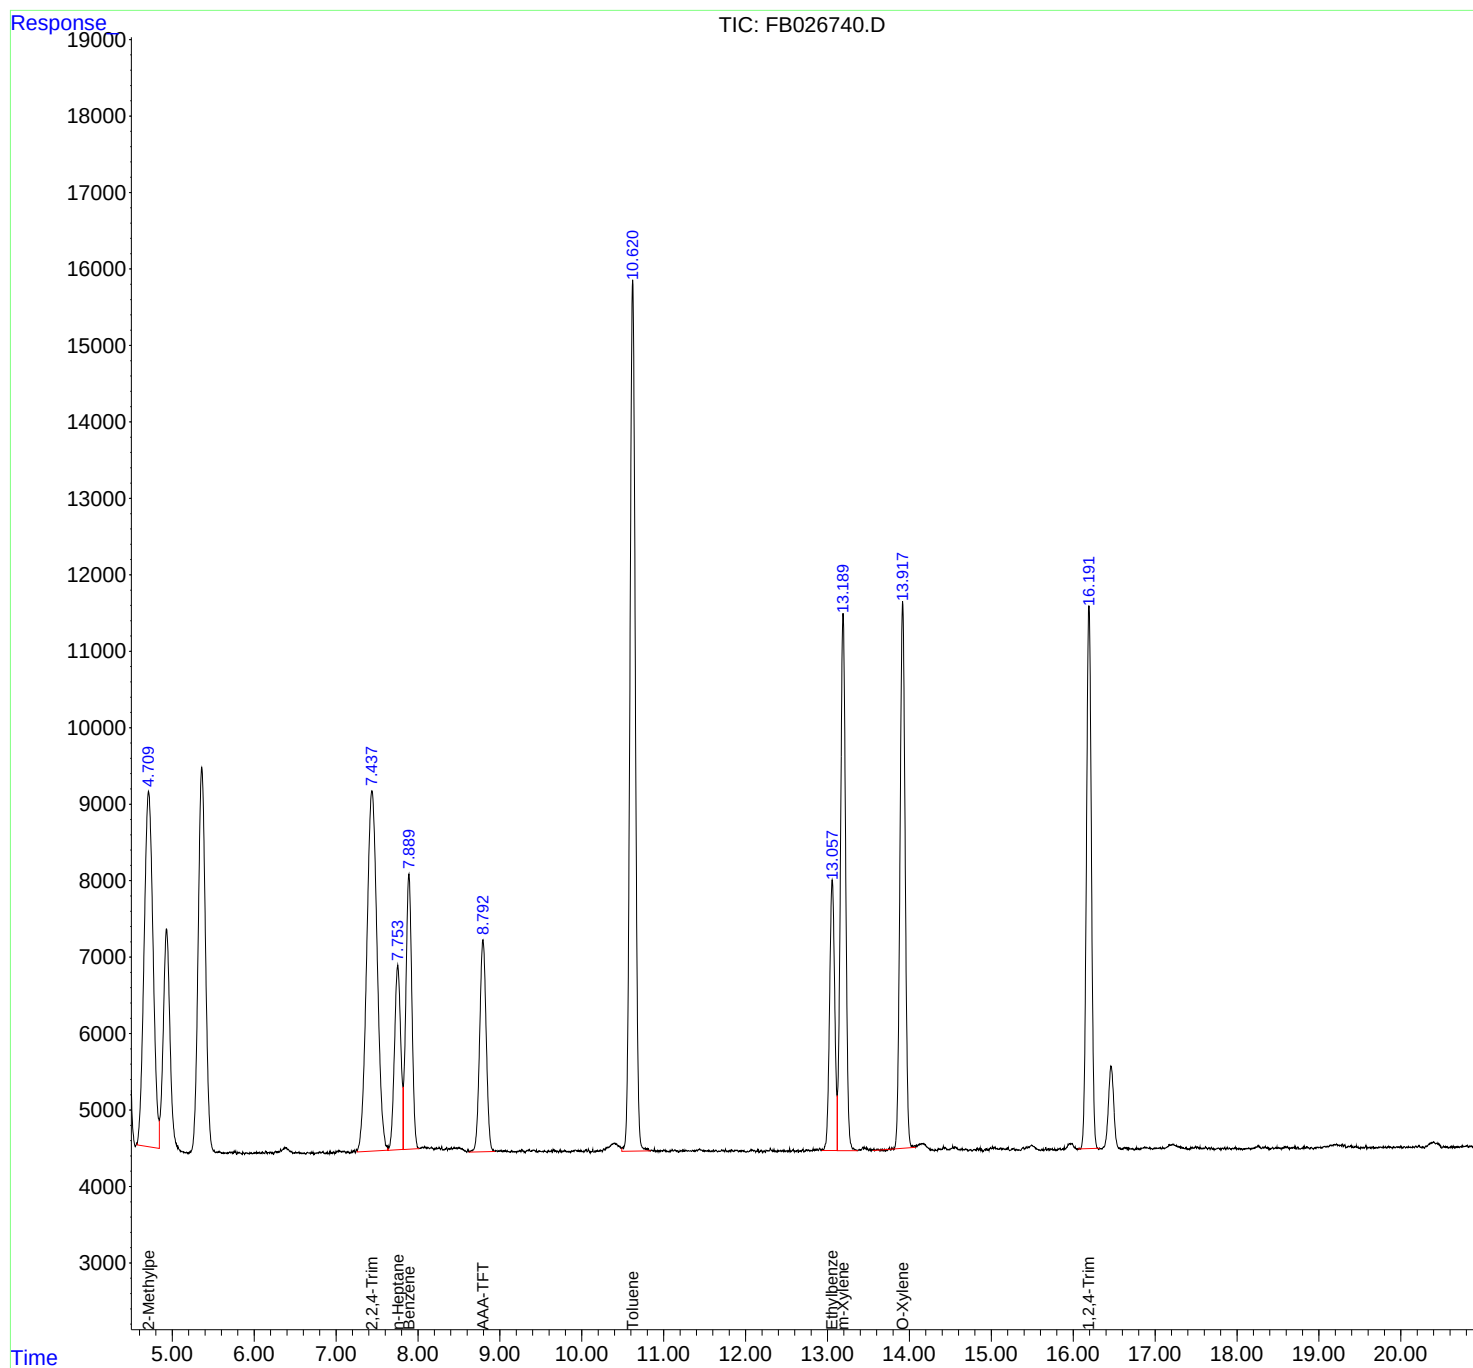


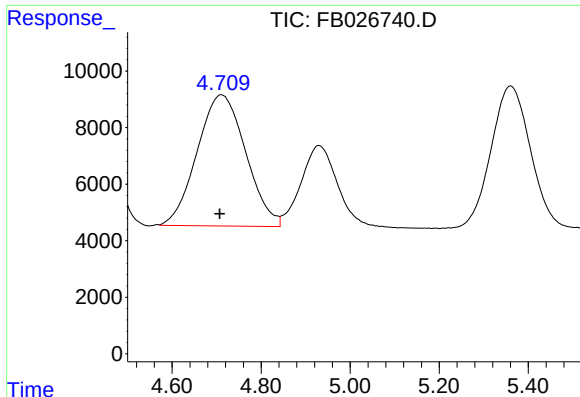

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 352253
Conc: 18.60 ng/ml

Instrument :
FID_B
ClientSampleId :

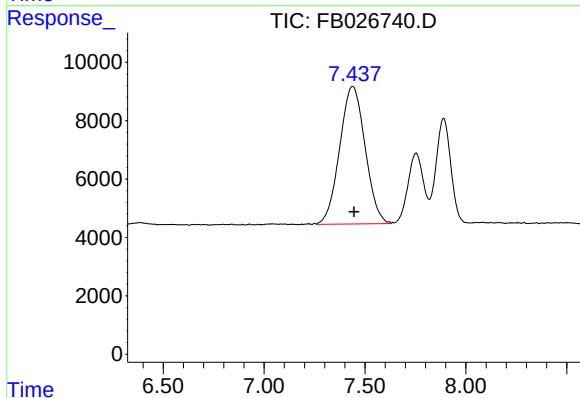


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: -0.009 min
Response: 413236
Conc: 19.94 ng/ml

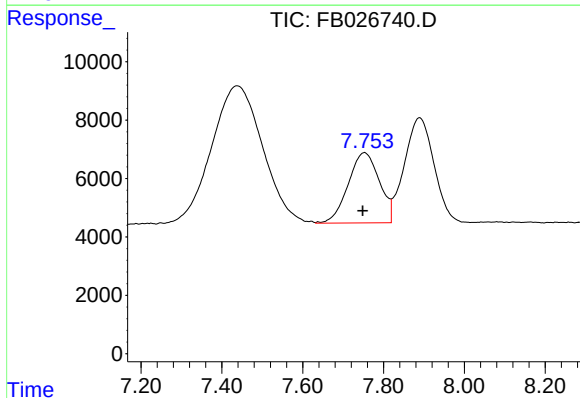


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.005 min
Response: 129104
Conc: 6.52 ng/ml

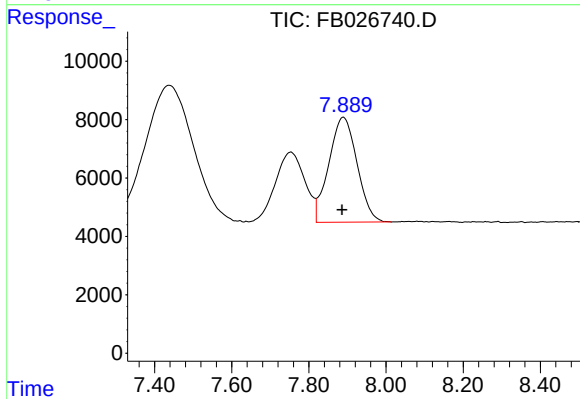

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.004 min
Response: 182624
Conc: 7.91 ng/ml

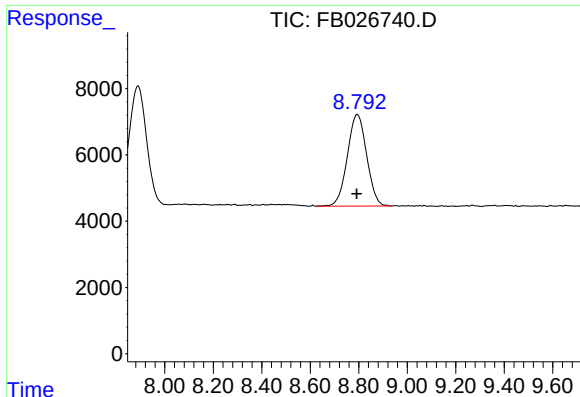

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 153412
Conc: 14.62 ng/ml

Instrument :
FID_B
ClientSampleId :

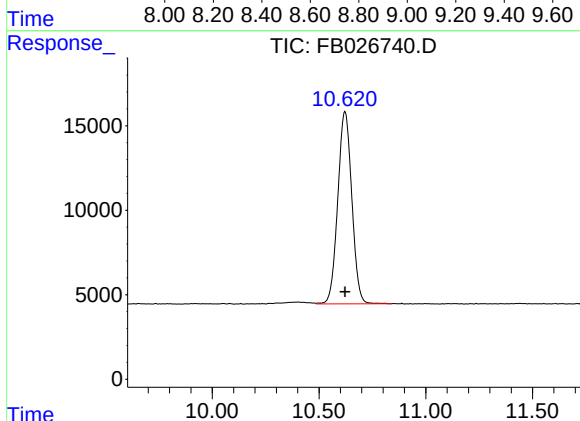


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 520229
Conc: 23.76 ng/ml

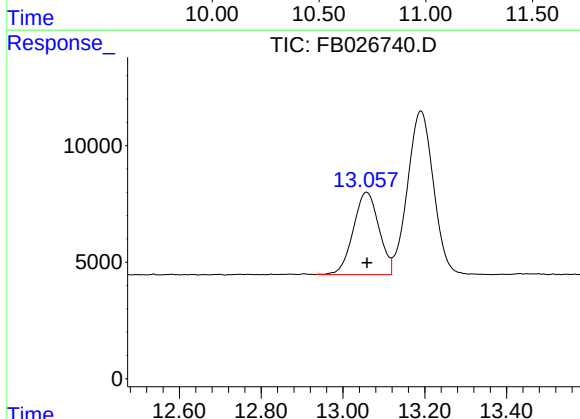


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 153617
Conc: 7.64 ng/ml

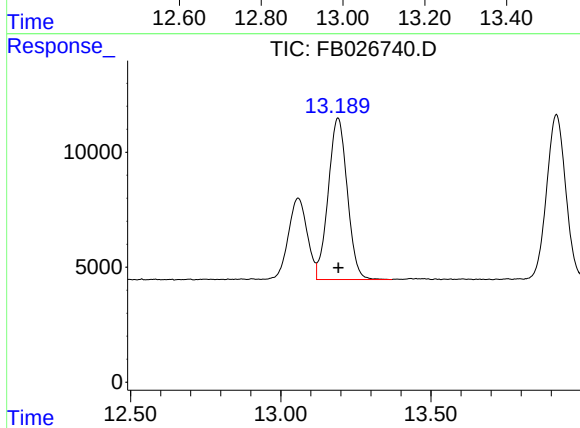

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 309225
Conc: 15.34 ng/ml

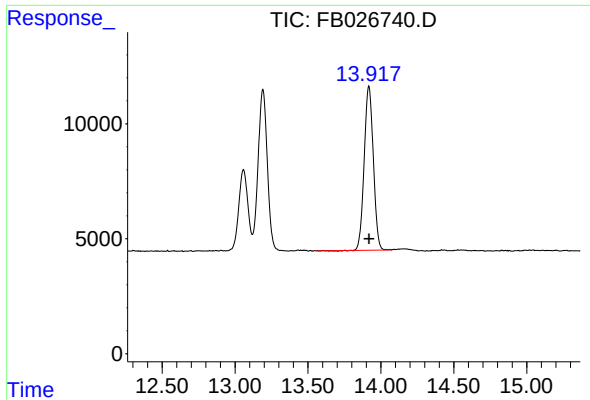

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 311831
Conc: 15.63 ng/ml

Instrument :
FID_B
ClientSampleId :

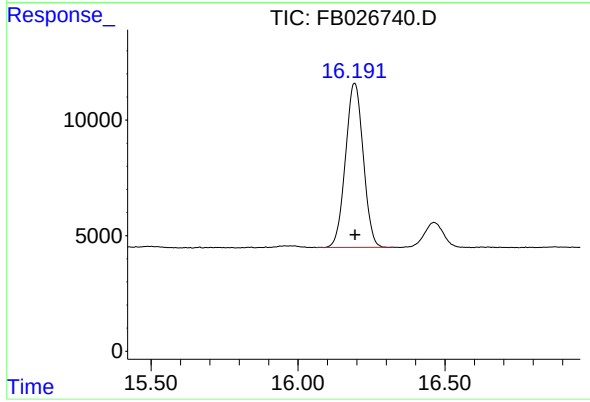

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.002 min
Response: 297520
Conc: 14.93 ng/ml