

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
 Data File : FB026733.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2022 8:25
 Operator : AJ/MA
 Sample : BSF0317S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0317S1

Integration File: SAMPLE.e
 Quant Time: Mar 18 22:43:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	178635	17.024 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	504050	26.622 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	572604	27.626 ng/ml
3) t n-Heptane	7.750	170699	8.624 ng/ml
4) t Benzene	7.886	207779	9.005 ng/ml
6) t Toluene	10.619	586637	26.796 ng/ml
7) t Ethylbenzene	13.056	183973	9.154 ng/ml
8) t m-Xylene	13.188	366761	18.199 ng/ml
9) t O-Xylene	13.915	371698	18.631 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	375570	18.850 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
Data File : FB026733.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2022 8:25
Operator : AJ/MA
Sample : BSF0317S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0317S1

Integration File: SAMPLE.e
Quant Time: Mar 18 22:43:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

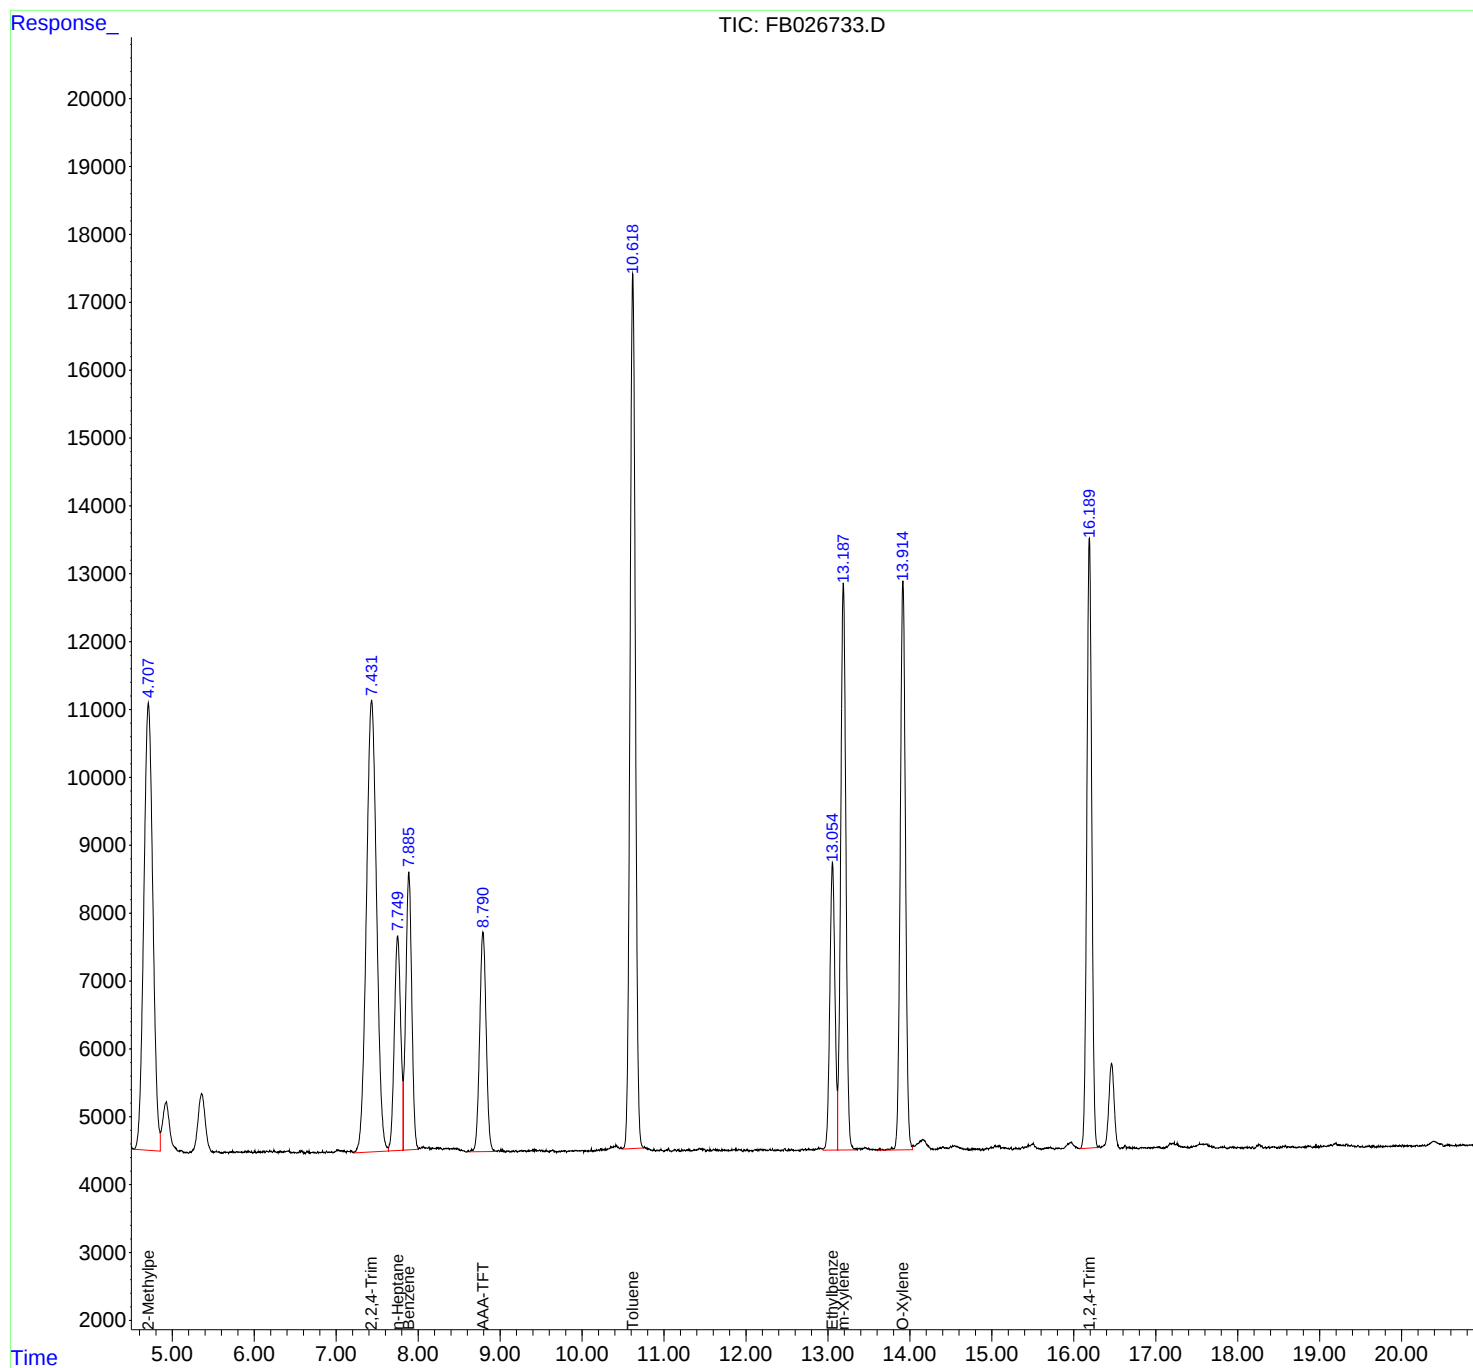


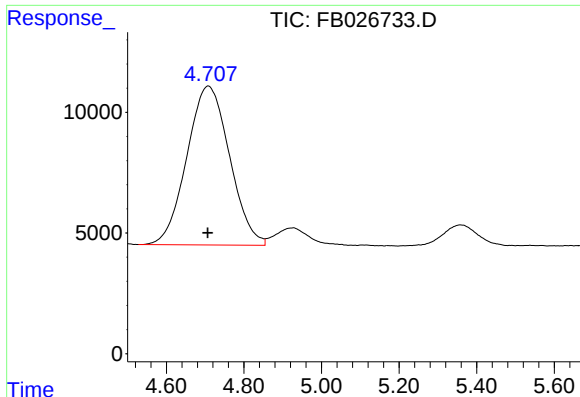

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 504050
Conc: 26.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0317S1

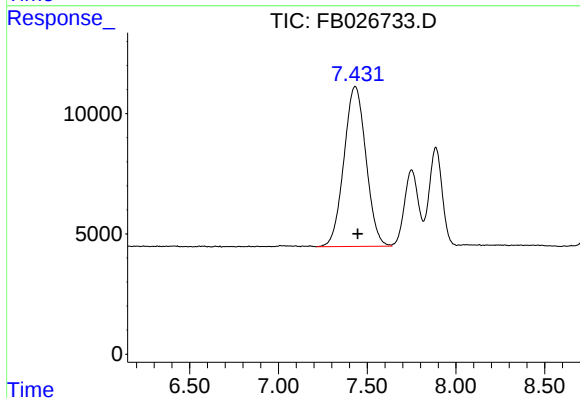


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.014 min
Response: 572604
Conc: 27.63 ng/ml

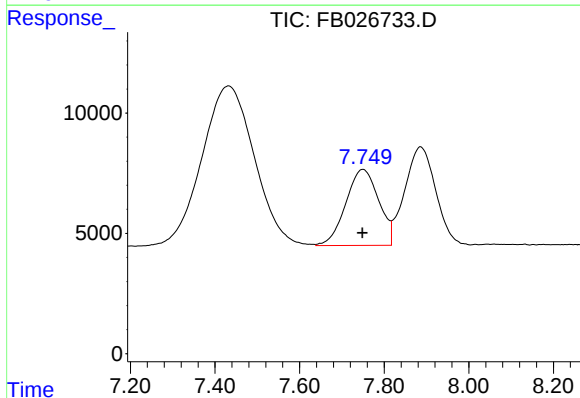


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 170699
Conc: 8.62 ng/ml

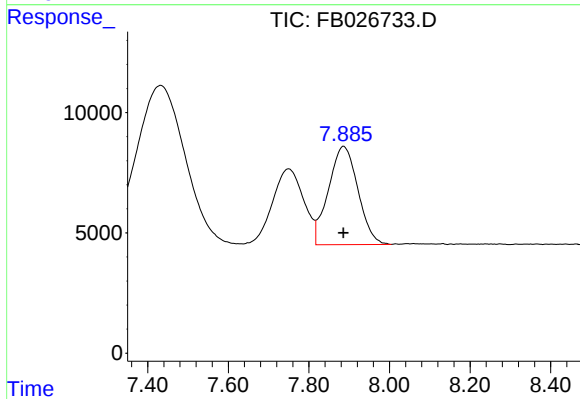

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 207779
Conc: 9.00 ng/ml

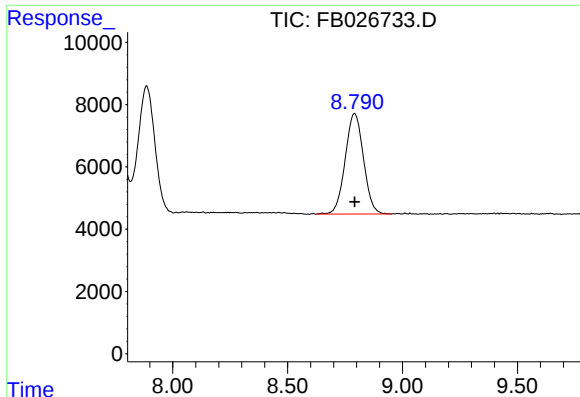

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 178635
Conc: 17.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0317S1

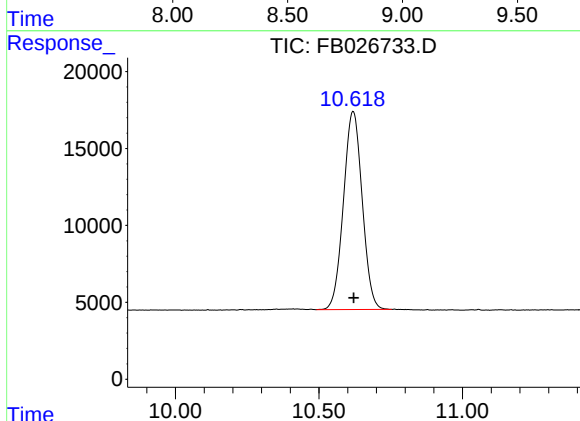


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 586637
Conc: 26.80 ng/ml

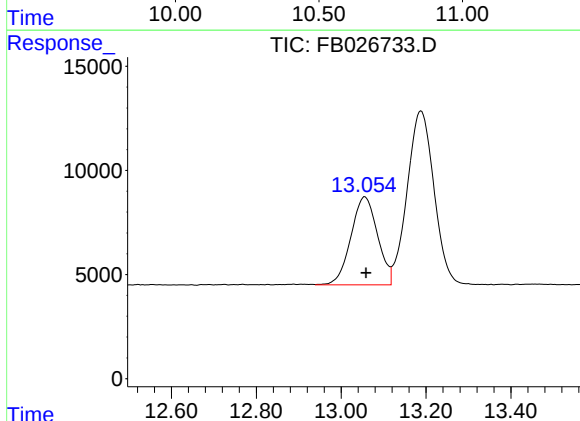


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 183973
Conc: 9.15 ng/ml

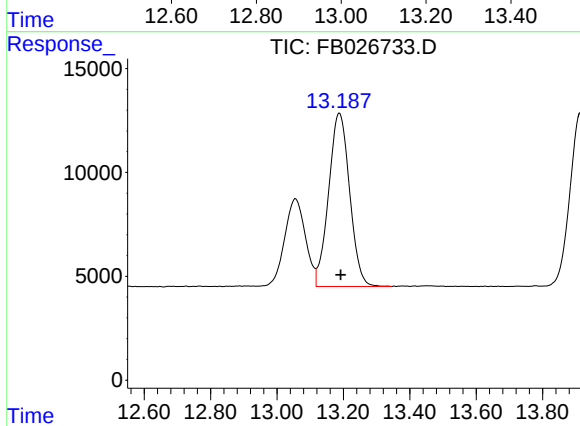

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 366761
Conc: 18.20 ng/ml

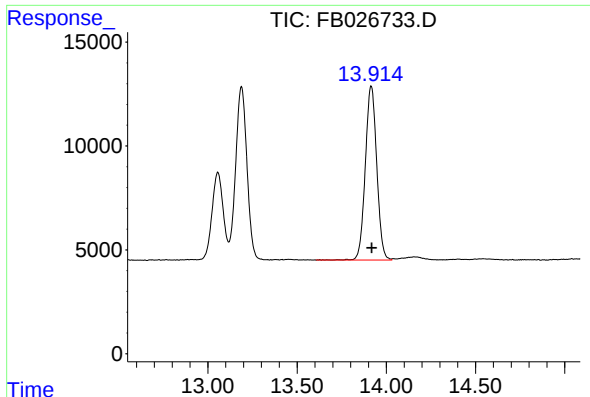

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.003 min
Response: 371698
Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0317S1

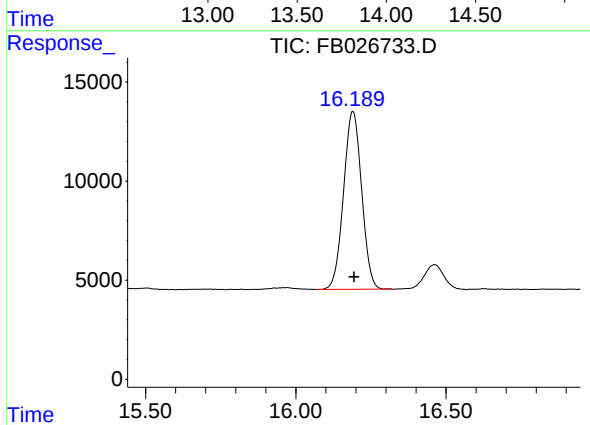

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 375570
Conc: 18.85 ng/ml