

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
 Data File : FB026741.D
 Signal(s) : FID2B.CH
 Acq On : 18 Mar 2022 14:59
 Operator : AJ/MA
 Sample : N1970-02MSD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G-3-5-8-9MSD

Integration File: SAMPLE.e
 Quant Time: Mar 18 22:44:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	134448	12.813 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	404376	21.358 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	459932	22.190 ng/ml
3) t n-Heptane	7.752	147891	7.472 ng/ml
4) t Benzene	7.889	200488	8.689 ng/ml
6) t Toluene	10.621	561105	25.630 ng/ml
7) t Ethylbenzene	13.058	167779	8.348 ng/ml
8) t m-Xylene	13.191	331255	16.437 ng/ml
9) t O-Xylene	13.918	331457	16.614 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	306545	15.385 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031822\
Data File : FB026741.D
Signal(s) : FID2B.CH
Acq On : 18 Mar 2022 14:59
Operator : AJ/MA
Sample : N1970-02MSD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-3-5-8-9MSD

Integration File: SAMPLE.e
Quant Time: Mar 18 22:44:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

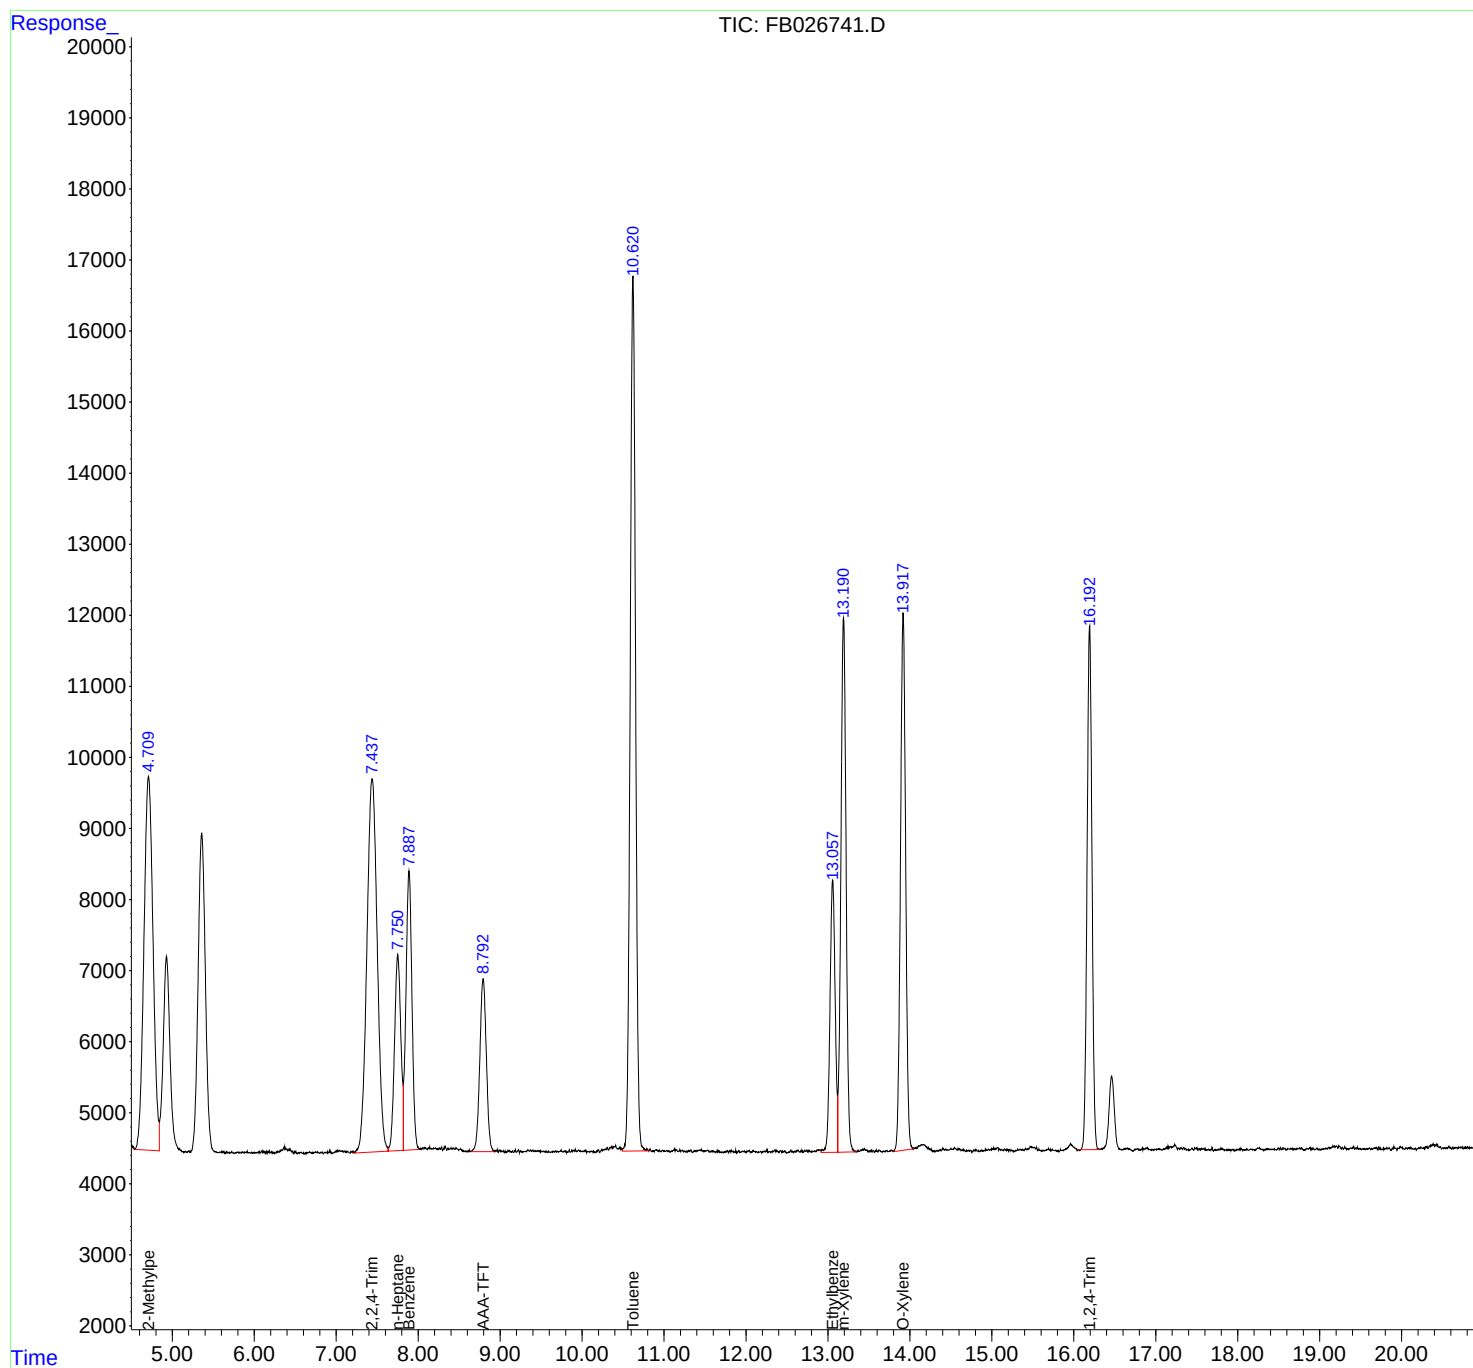


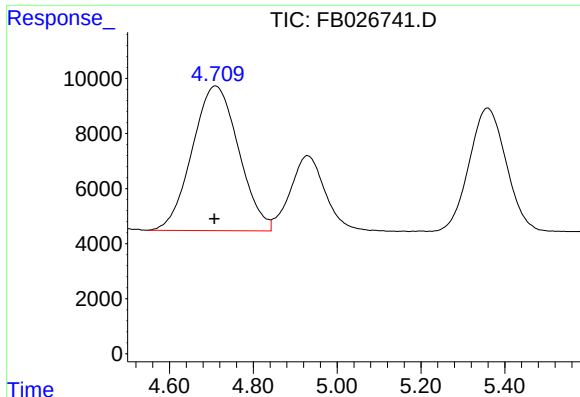

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.003 min
Response: 404376
Conc: 21.36 ng/ml

Instrument :
FID_B
ClientSampleId :
G-3-5-8-9MSD

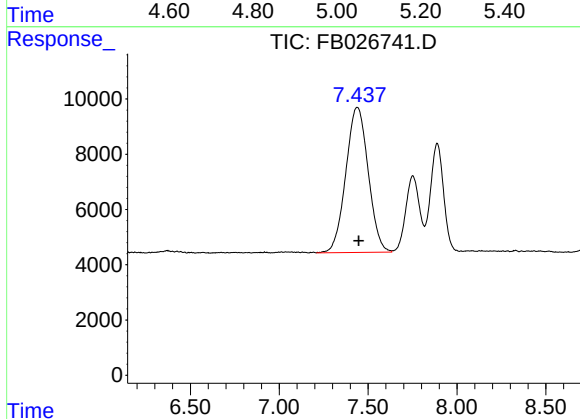


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: -0.008 min
Response: 459932
Conc: 22.19 ng/ml

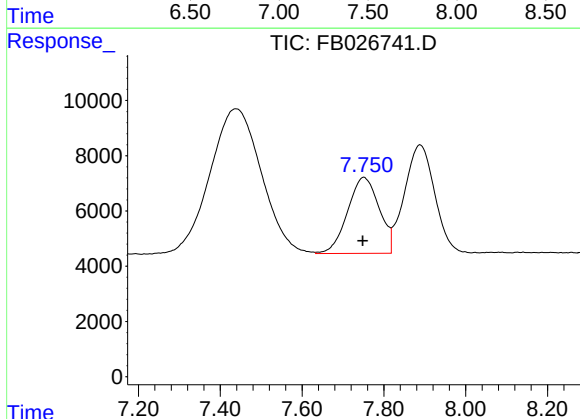


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.003 min
Response: 147891
Conc: 7.47 ng/ml

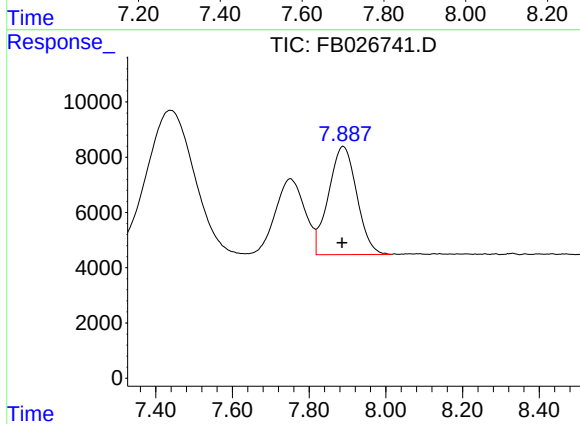

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 200488
Conc: 8.69 ng/ml

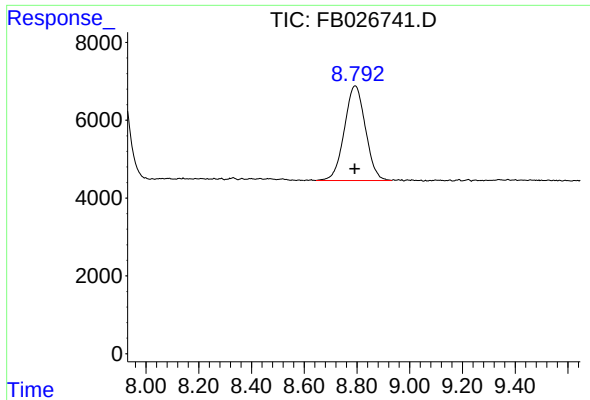

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 134448
Conc: 12.81 ng/ml

Instrument :
FID_B
ClientSampleId :
G-3-5-8-9MSD

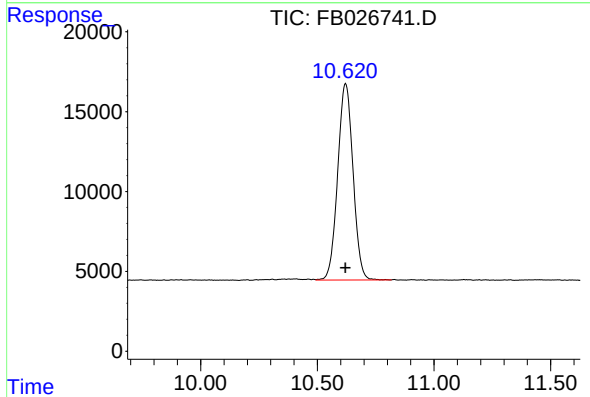


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 561105
Conc: 25.63 ng/ml

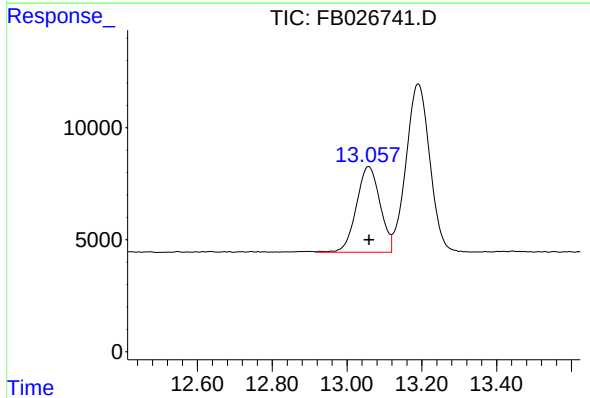


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 167779
Conc: 8.35 ng/ml

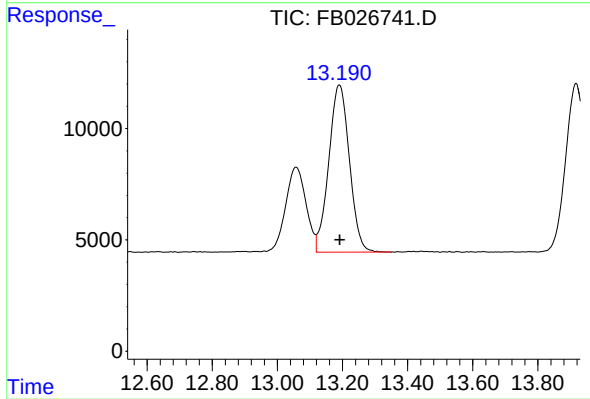

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 331255
Conc: 16.44 ng/ml

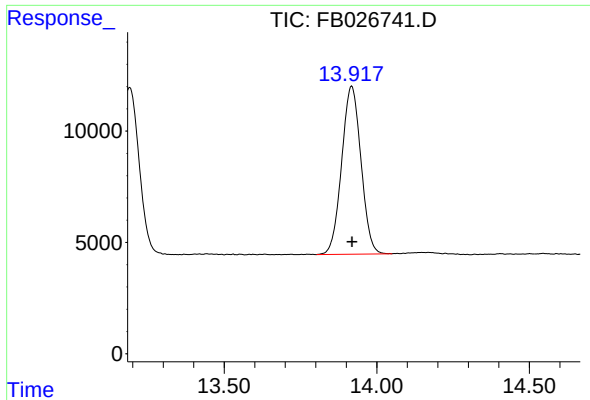

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 331457
Conc: 16.61 ng/ml

Instrument :
FID_B
ClientSampleId :
G-3-5-8-9MSD

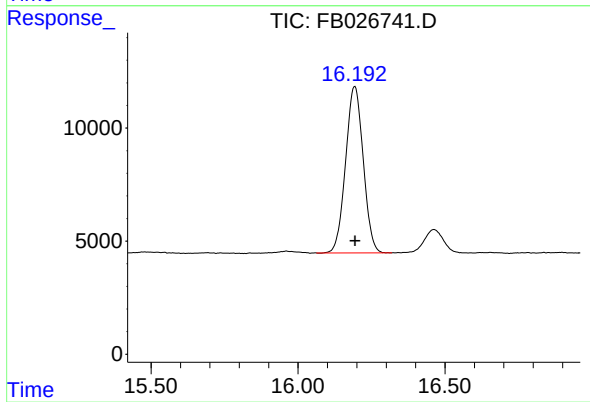

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.001 min
Response: 306545
Conc: 15.39 ng/ml