

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB031822\  
 Data File : FB026746.D  
 Signal(s) : FID2B.CH  
 Acq On : 18 Mar 2022 18:27  
 Operator : AJ/MA  
 Sample : N1995-02  
 Misc : 5.06G/5.00 ML DI WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 SB-06-COMP

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 03/21/2022  
 Supervised By :mohammad ahmed 03/23/2022

Integration File: SAMPLE.e  
 Quant Time: Mar 18 22:45:12 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030822.M  
 Quant Title :  
 QLast Update : Fri Mar 11 13:08:49 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.797 | 7869     | 0.750 ng/mlm |
| Target Compounds            |       |          |              |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB031822\  
Data File : FB026746.D  
Signal(s) : FID2B.CH  
Acq On : 18 Mar 2022 18:27  
Operator : AJ/MA  
Sample : N1995-02  
Misc : 5.06G/5.00 ML DI WATER  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
FID\_B  
ClientSampleId :  
SB-06-COMP


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/21/2022  
Supervised By :mohammad ahmed 03/23/2022

Integration File: SAMPLE.e  
Quant Time: Mar 18 22:45:12 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030822.M  
Quant Title :  
QLast Update : Fri Mar 11 13:08:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

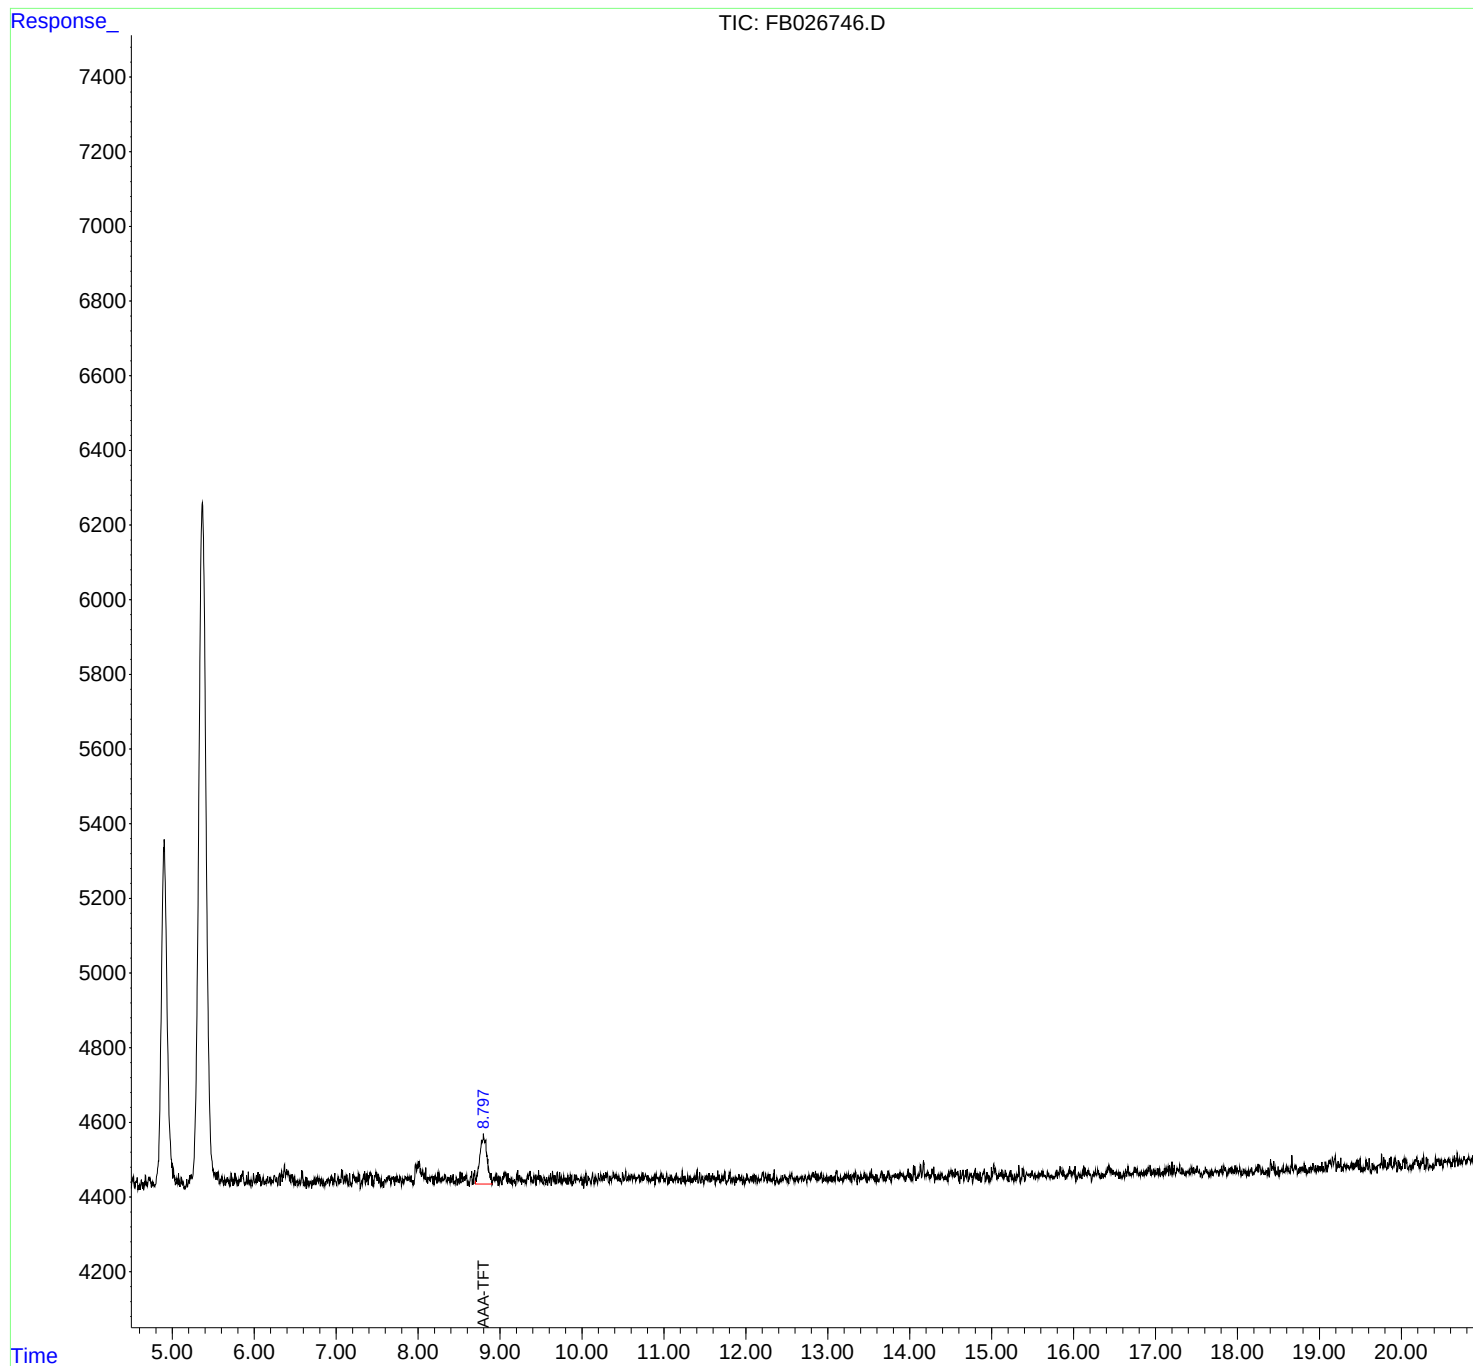

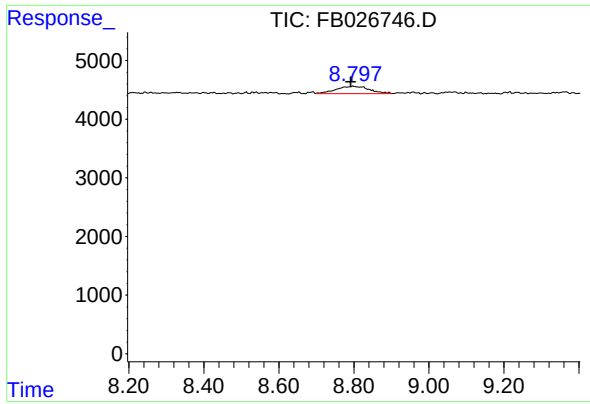

#5 AAA-TFT

R.T.: 8.797 min  
Delta R.T.: 0.005 min  
Response: 7869  
Conc: 0.75 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
SB-06-COMP

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/21/2022  
Supervised By :mohammad ahmed 03/23/2022