

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
 Data File : FB020286.D
 Signal(s) : FID2B.CH
 Acq On : 19 Mar 2019 14:28
 Operator : MJ/SJ
 Sample : K1692-03MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-02-031819MS

Integration File: Calibration.e
 Quant Time: Mar 20 00:14:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.041	477372	18.184 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	835124	24.757 ng/ml
2) t 2,2,4-Trimethylpentane	7.666	676451	20.627 ng/ml
3) t n-Heptane	7.997	310112	7.452 ng/ml
4) t Benzene	8.134	418734	8.994 ng/ml
6) t Toluene	10.888	954793	25.838 ng/ml
7) t Ethylbenzene	13.341	204102	8.675 ng/ml
8) t m-Xylene	13.474	386317	18.110 ng/ml
9) t O-Xylene	14.206	370791	19.574 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	377905	19.055 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


```
Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\  
Data File : FB020286.D  
Signal(s) : FID2B.CH  
Acq On    : 19 Mar 2019  14:28  
Operator  : MJ/SJ  
Sample    : K1692-03MS  
Misc      : 5.02g/5.00ml DI WATER  
ALS Vial  : 12    Sample Multiplier: 1
```

Instrument :
FID_B
ClientSampleId :
OK-02-031819MS

Integration File: Calibration.e
Quant Time: Mar 20 00:14:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

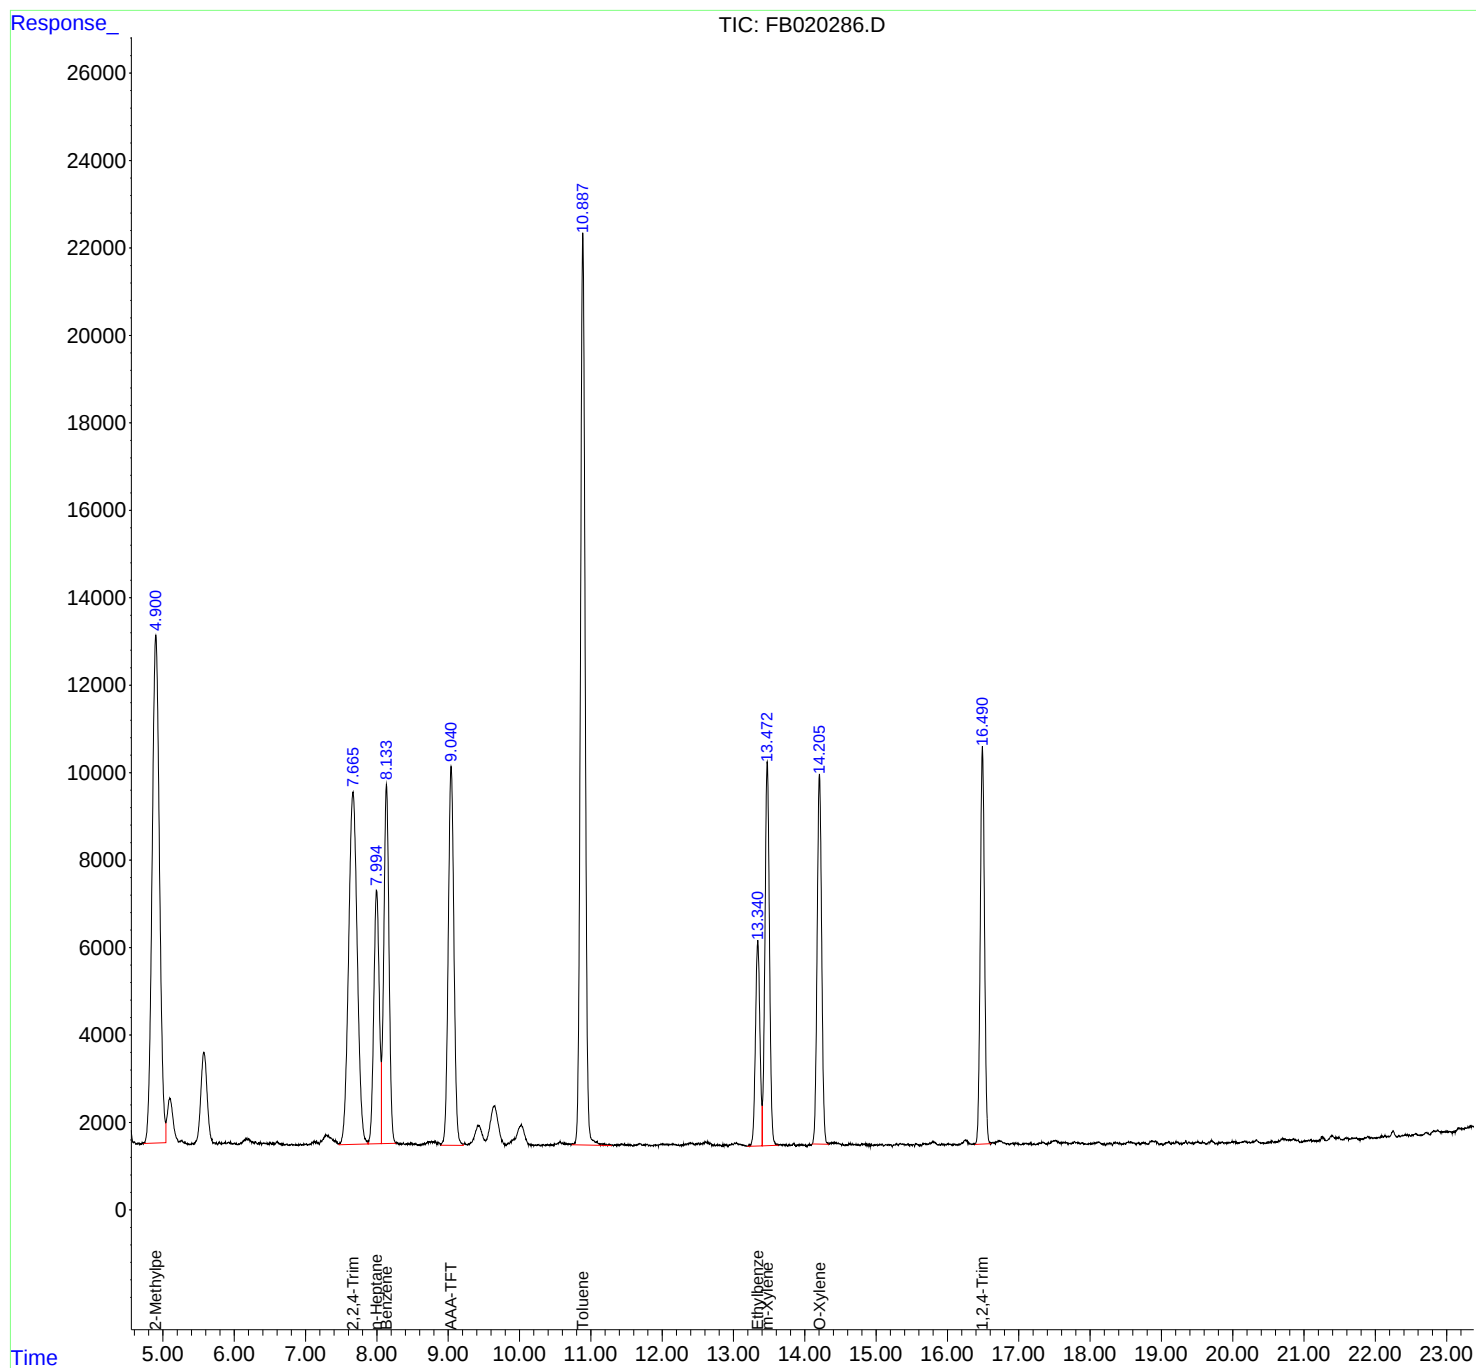


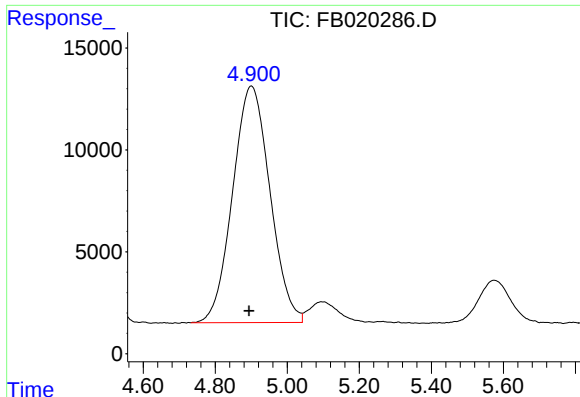

#1 2-Methylpentane


R.T.: 4.901 min
Delta R.T.: 0.007 min
Response: 835124
Conc: 24.76 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-031819MS

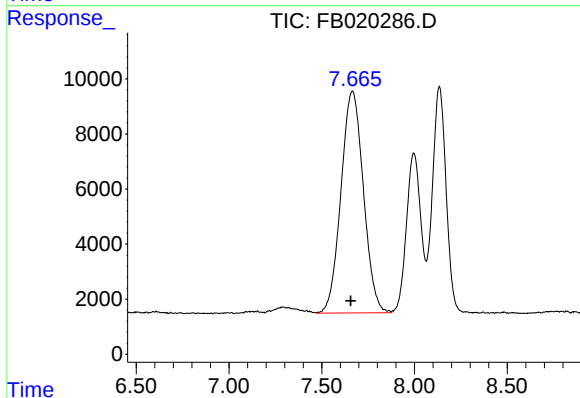


#2 2,2,4-Trimethylpentane

R.T.: 7.666 min
Delta R.T.: 0.008 min
Response: 676451
Conc: 20.63 ng/ml

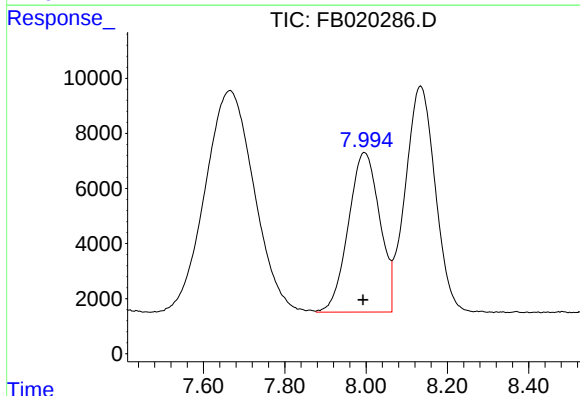


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: 0.004 min
Response: 310112
Conc: 7.45 ng/ml

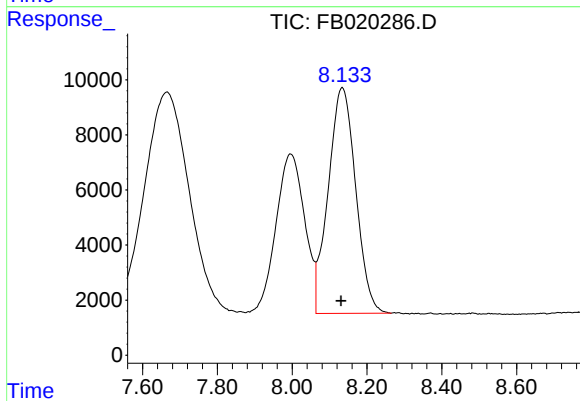

#4 Benzene


R.T.: 8.134 min
Delta R.T.: 0.004 min
Response: 418734
Conc: 8.99 ng/ml

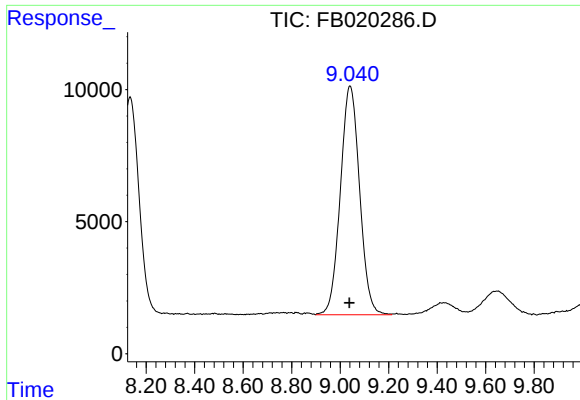

#5 AAA-TFT


R.T.: 9.041 min
Delta R.T.: 0.003 min
Response: 477372
Conc: 18.18 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-031819MS

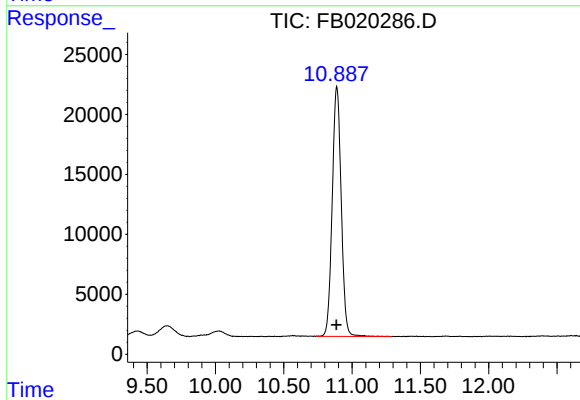


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.003 min
Response: 954793
Conc: 25.84 ng/ml

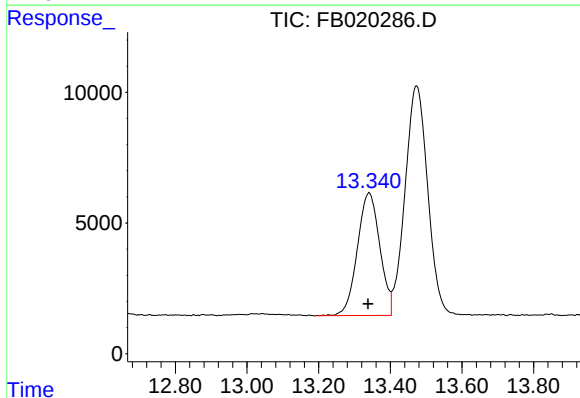


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: 0.003 min
Response: 204102
Conc: 8.67 ng/ml

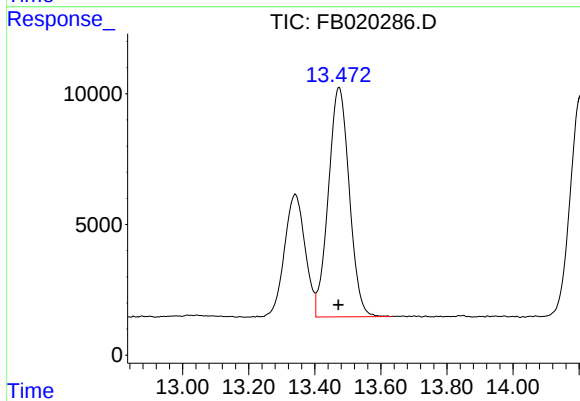

#8 m-Xylene


R.T.: 13.474 min
Delta R.T.: 0.003 min
Response: 386317
Conc: 18.11 ng/ml

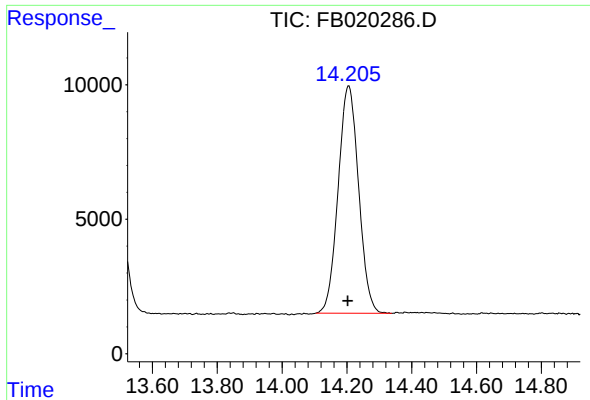

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: 0.003 min
Response: 370791
Conc: 19.57 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-031819MS

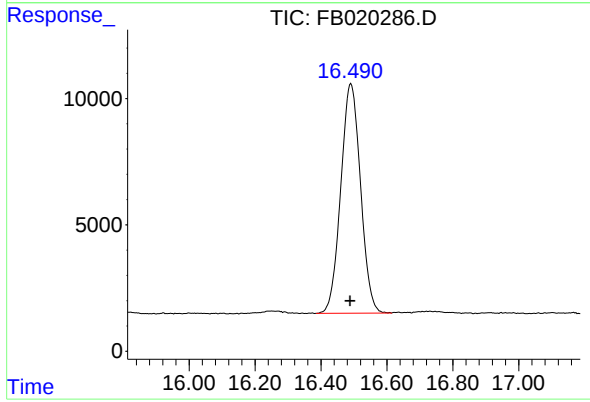

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.002 min
Response: 377905
Conc: 19.06 ng/ml