

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
 Data File : FB020295.D
 Signal(s) : FID2B.CH
 Acq On : 19 Mar 2019 19:01
 Operator : MJ/SJ
 Sample : K1989-03
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 20 00:15:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	369668	14.081 ng/ml
Target Compounds			
6) t Toluene	10.884	4313	0.117 ng/ml
7) t Ethylbenzene	13.352	6540	0.278 ng/ml
8) t m-Xylene	13.467	10560	0.495 ng/ml
9) t O-Xylene	14.198	5566	0.294 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	26851	1.354 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
Data File : FB020295.D
Signal(s) : FID2B.CH
Acq On : 19 Mar 2019 19:01
Operator : MJ/SJ
Sample : K1989-03
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 20 00:15:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

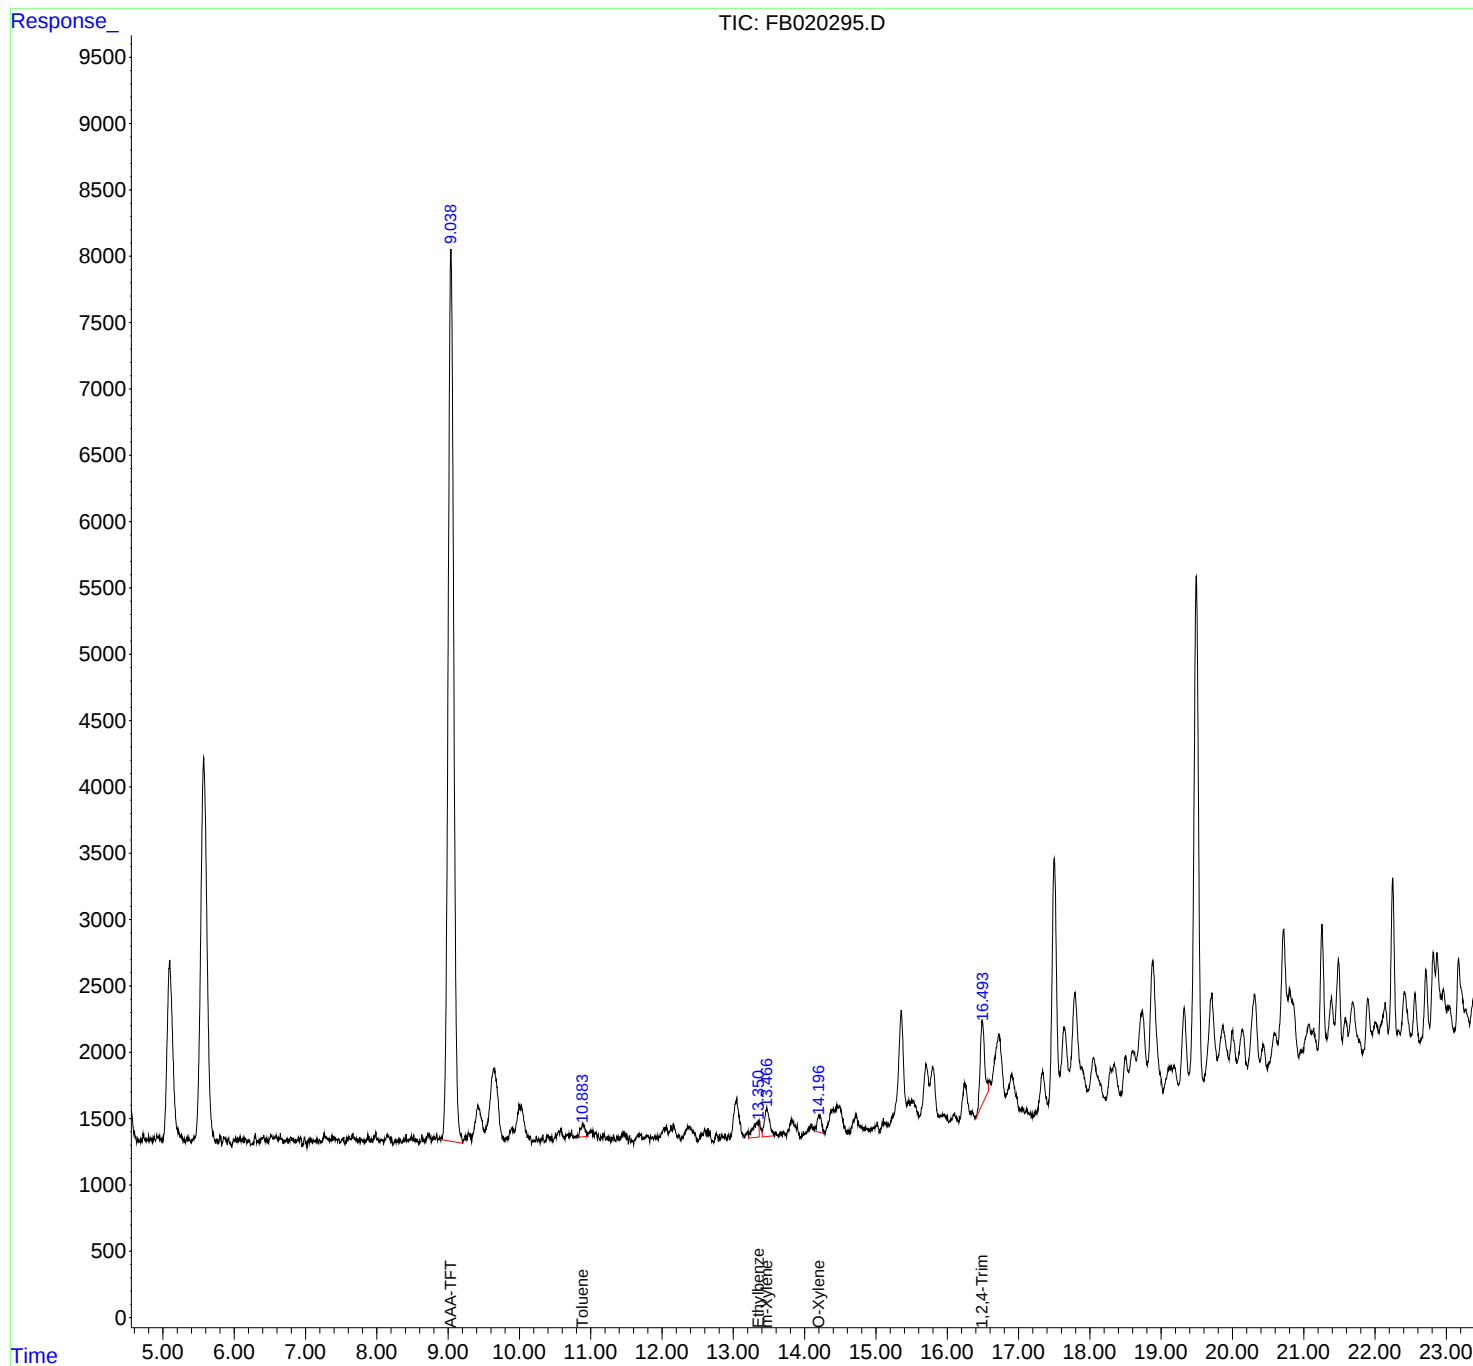


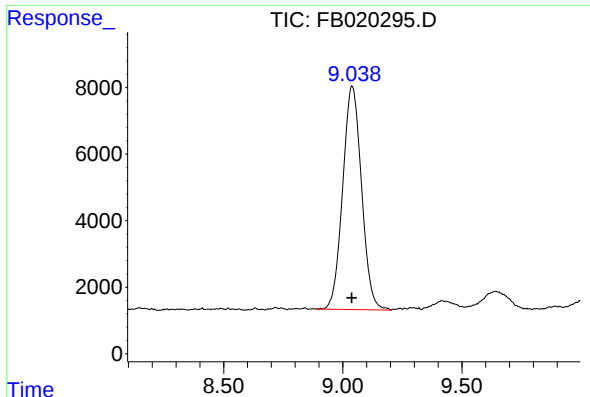

#5 AAA-TFT


R.T.: 9.039 min
Delta R.T.: 0.001 min
Response: 369668
Conc: 14.08 ng/ml

Instrument :
FID_B
ClientSampleId :

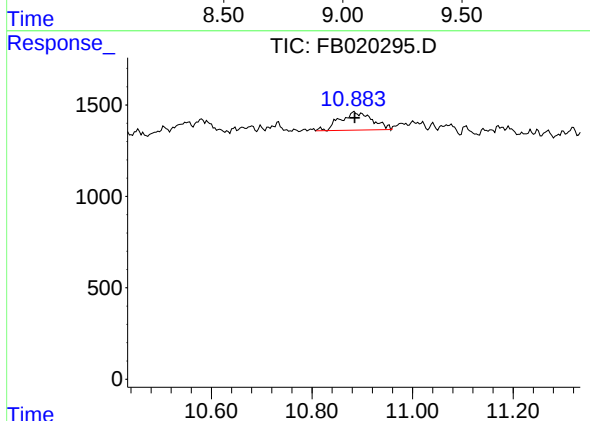


#6 Toluene

R.T.: 10.884 min
Delta R.T.: -0.001 min
Response: 4313
Conc: 0.12 ng/ml

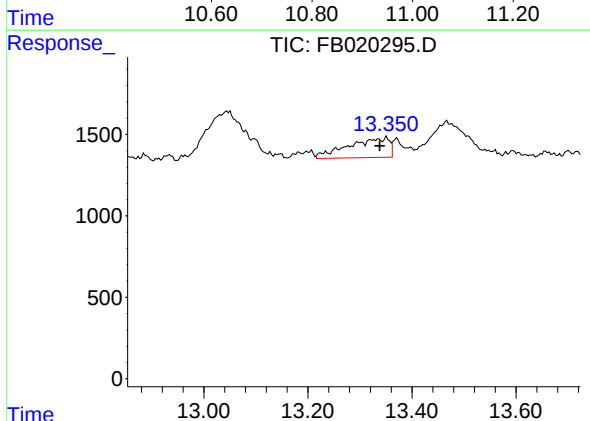


#7 Ethylbenzene

R.T.: 13.352 min
Delta R.T.: 0.014 min
Response: 6540
Conc: 0.28 ng/ml

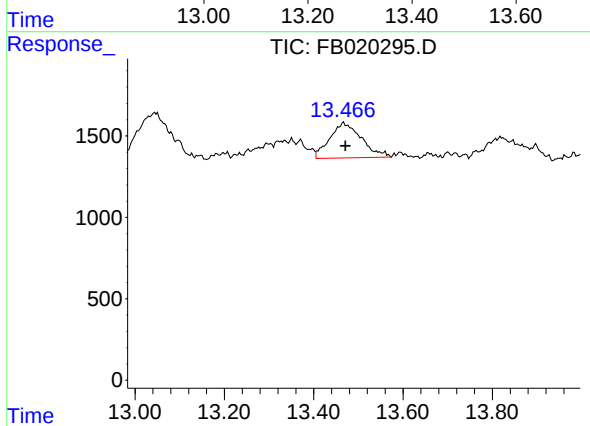

#8 m-Xylene


R.T.: 13.467 min
Delta R.T.: -0.004 min
Response: 10560
Conc: 0.50 ng/ml

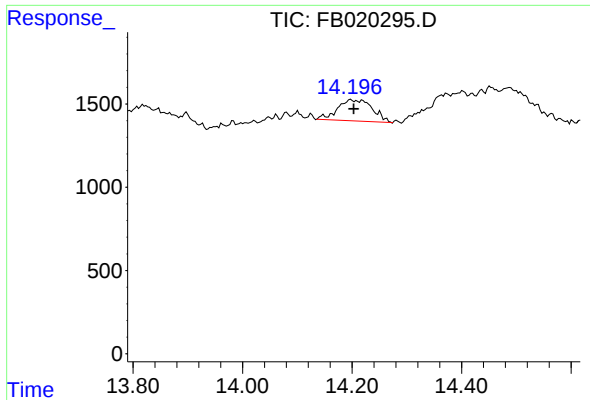

#9 O-Xylene

R.T.: 14.198 min
Delta R.T.: -0.005 min
Response: 5566
Conc: 0.29 ng/ml

Instrument :
FID_B
ClientSampleId :

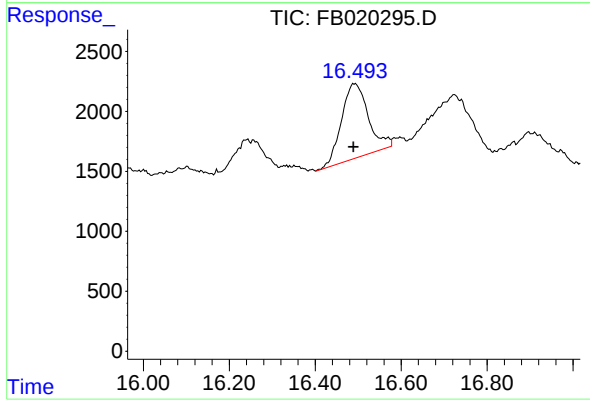

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: 0.003 min
Response: 26851
Conc: 1.35 ng/ml