

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
 Data File : FB020296.D
 Signal(s) : FID2B.CH
 Acq On : 19 Mar 2019 19:31
 Operator : MJ/SJ
 Sample : K1984-03 50X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 20 00:15:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	490354	18.678 ng/ml
Target Compounds			
4) t Benzene	8.159	4980	0.107 ng/ml
6) t Toluene	10.912	7973	0.216 ng/ml
7) t Ethylbenzene	13.312	6470	0.275 ng/ml
10) t 1,2,4-Trimethylbenzene	16.519	1591	0.080 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
Data File : FB020296.D
Signal(s) : FID2B.CH
Acq On : 19 Mar 2019 19:31
Operator : MJ/SJ
Sample : K1984-03 50X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 20 00:15:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

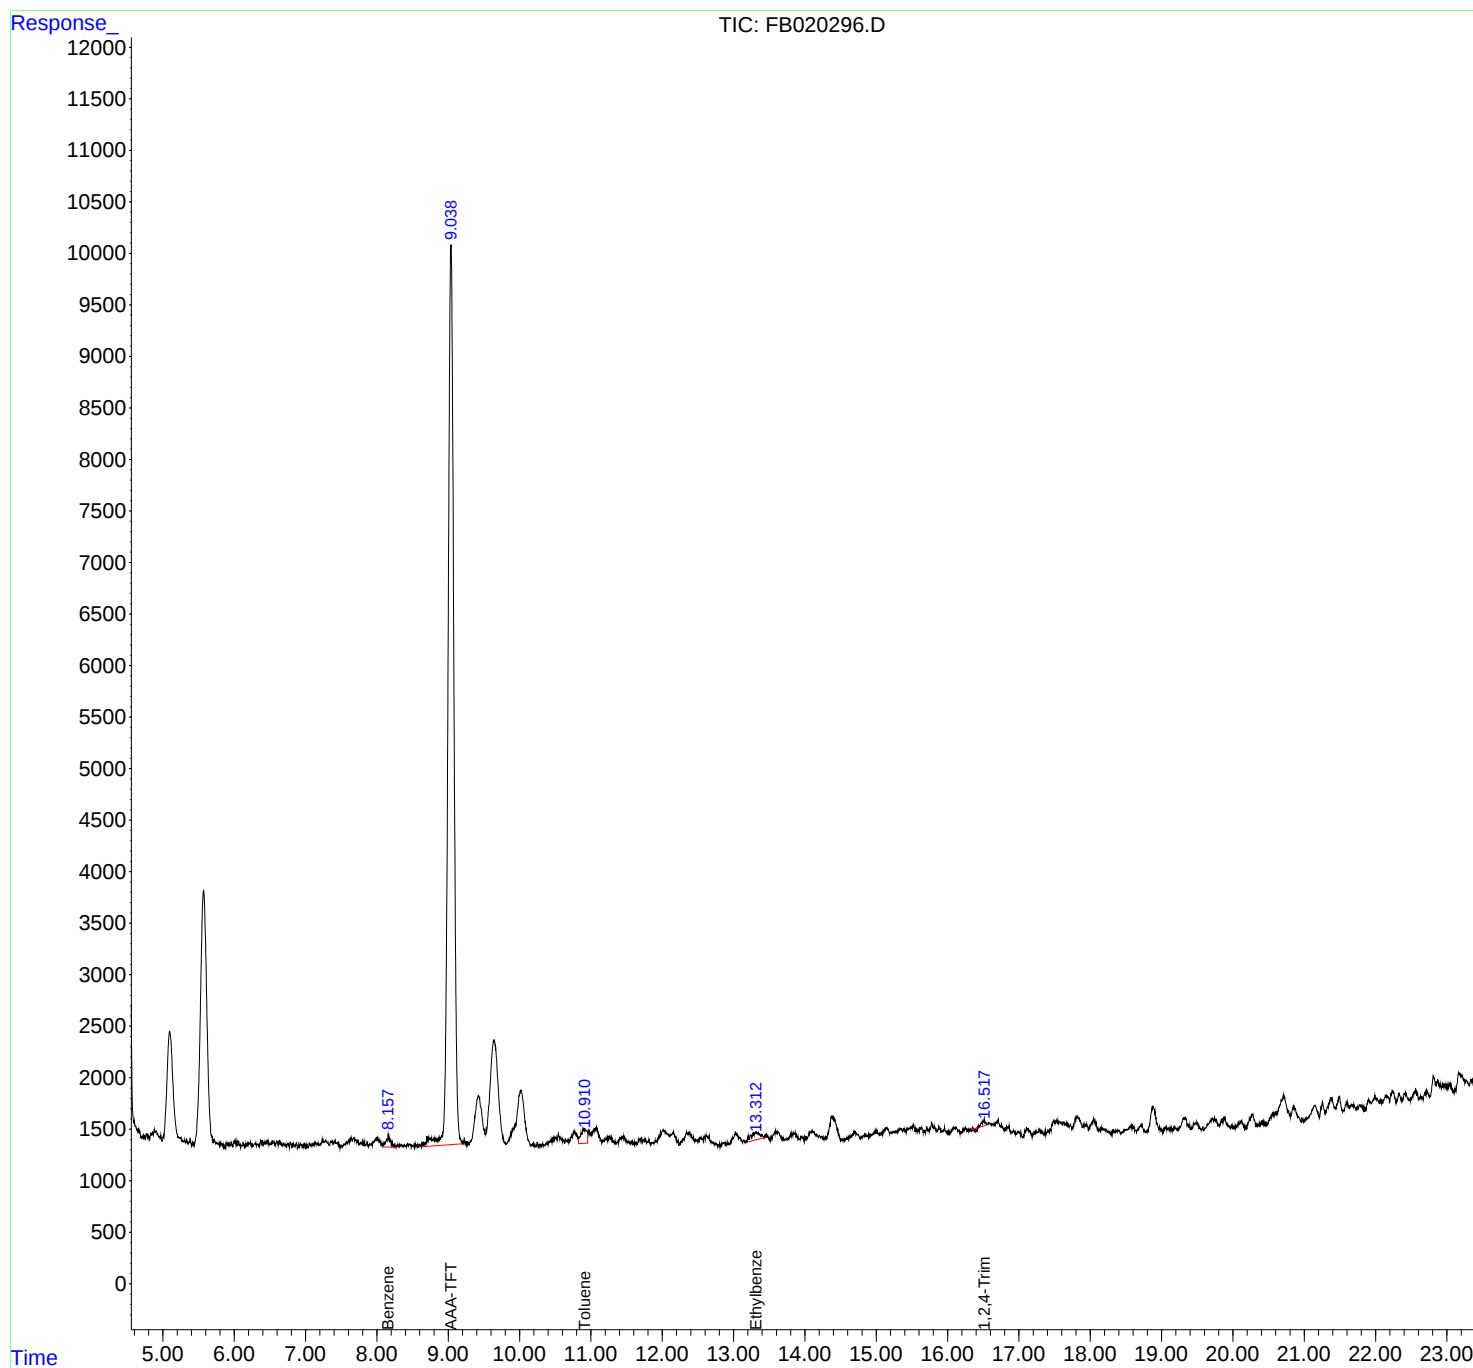


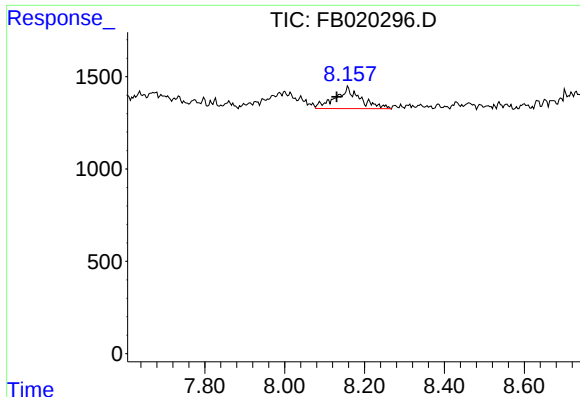

#4 Benzene


R.T.: 8.159 min
Delta R.T.: 0.028 min
Response: 4980
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :

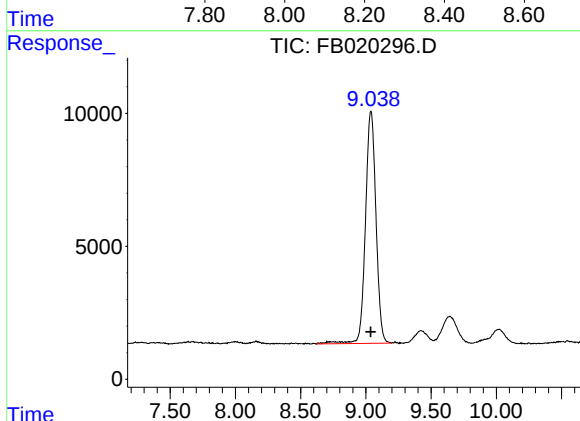


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 490354
Conc: 18.68 ng/ml

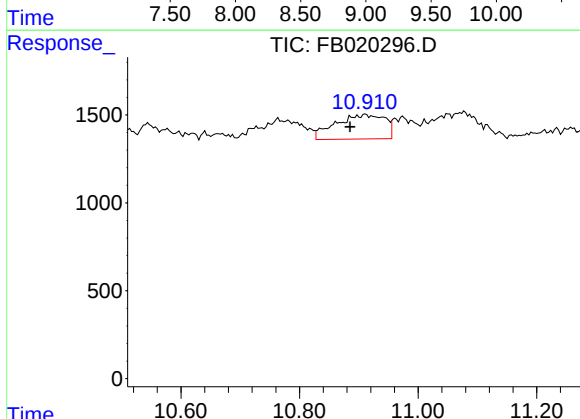


#6 Toluene

R.T.: 10.912 min
Delta R.T.: 0.027 min
Response: 7973
Conc: 0.22 ng/ml

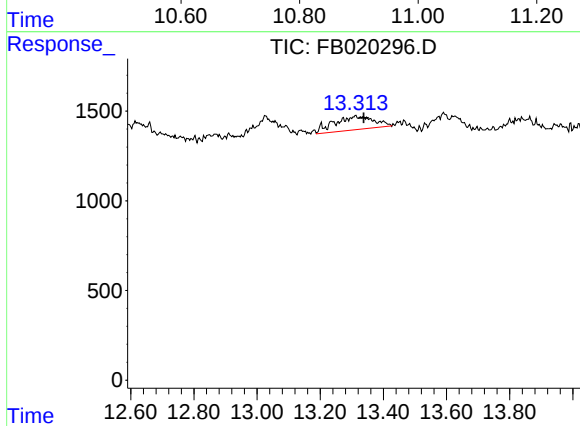

#7 Ethylbenzene

R.T.: 13.312 min
Delta R.T.: -0.026 min
Response: 6470
Conc: 0.27 ng/ml

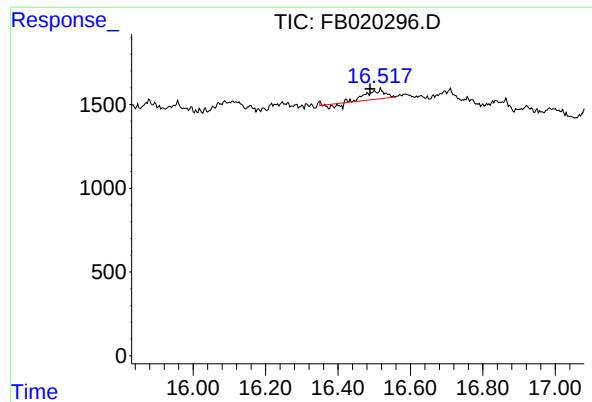

#10 1,2,4-Trimethylbenzene

R.T.: 16.519 min
Delta R.T.: 0.030 min
Response: 1591
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :