

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
 Data File : FB020287.D
 Signal(s) : FID2B.CH
 Acq On : 19 Mar 2019 14:58
 Operator : MJ/SJ
 Sample : K1692-03MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-02-031819MSD

Integration File: Calibration.e
 Quant Time: Mar 20 00:14:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.041	488788	18.619 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	849624	25.186 ng/ml
2) t 2,2,4-Trimethylpentane	7.666	656832	20.029 ng/ml
3) t n-Heptane	7.996	297130	7.140 ng/ml
4) t Benzene	8.134	425589	9.141 ng/ml
6) t Toluene	10.888	936422	25.341 ng/ml
7) t Ethylbenzene	13.340	203525	8.650 ng/ml
8) t m-Xylene	13.474	390962	18.328 ng/ml
9) t O-Xylene	14.205	374886	19.790 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	370305	18.672 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031919\
Data File : FB020287.D
Signal(s) : FID2B.CH
Acq On : 19 Mar 2019 14:58
Operator : MJ/SJ
Sample : K1692-03MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-02-031819MSD

Integration File: Calibration.e
Quant Time: Mar 20 00:14:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

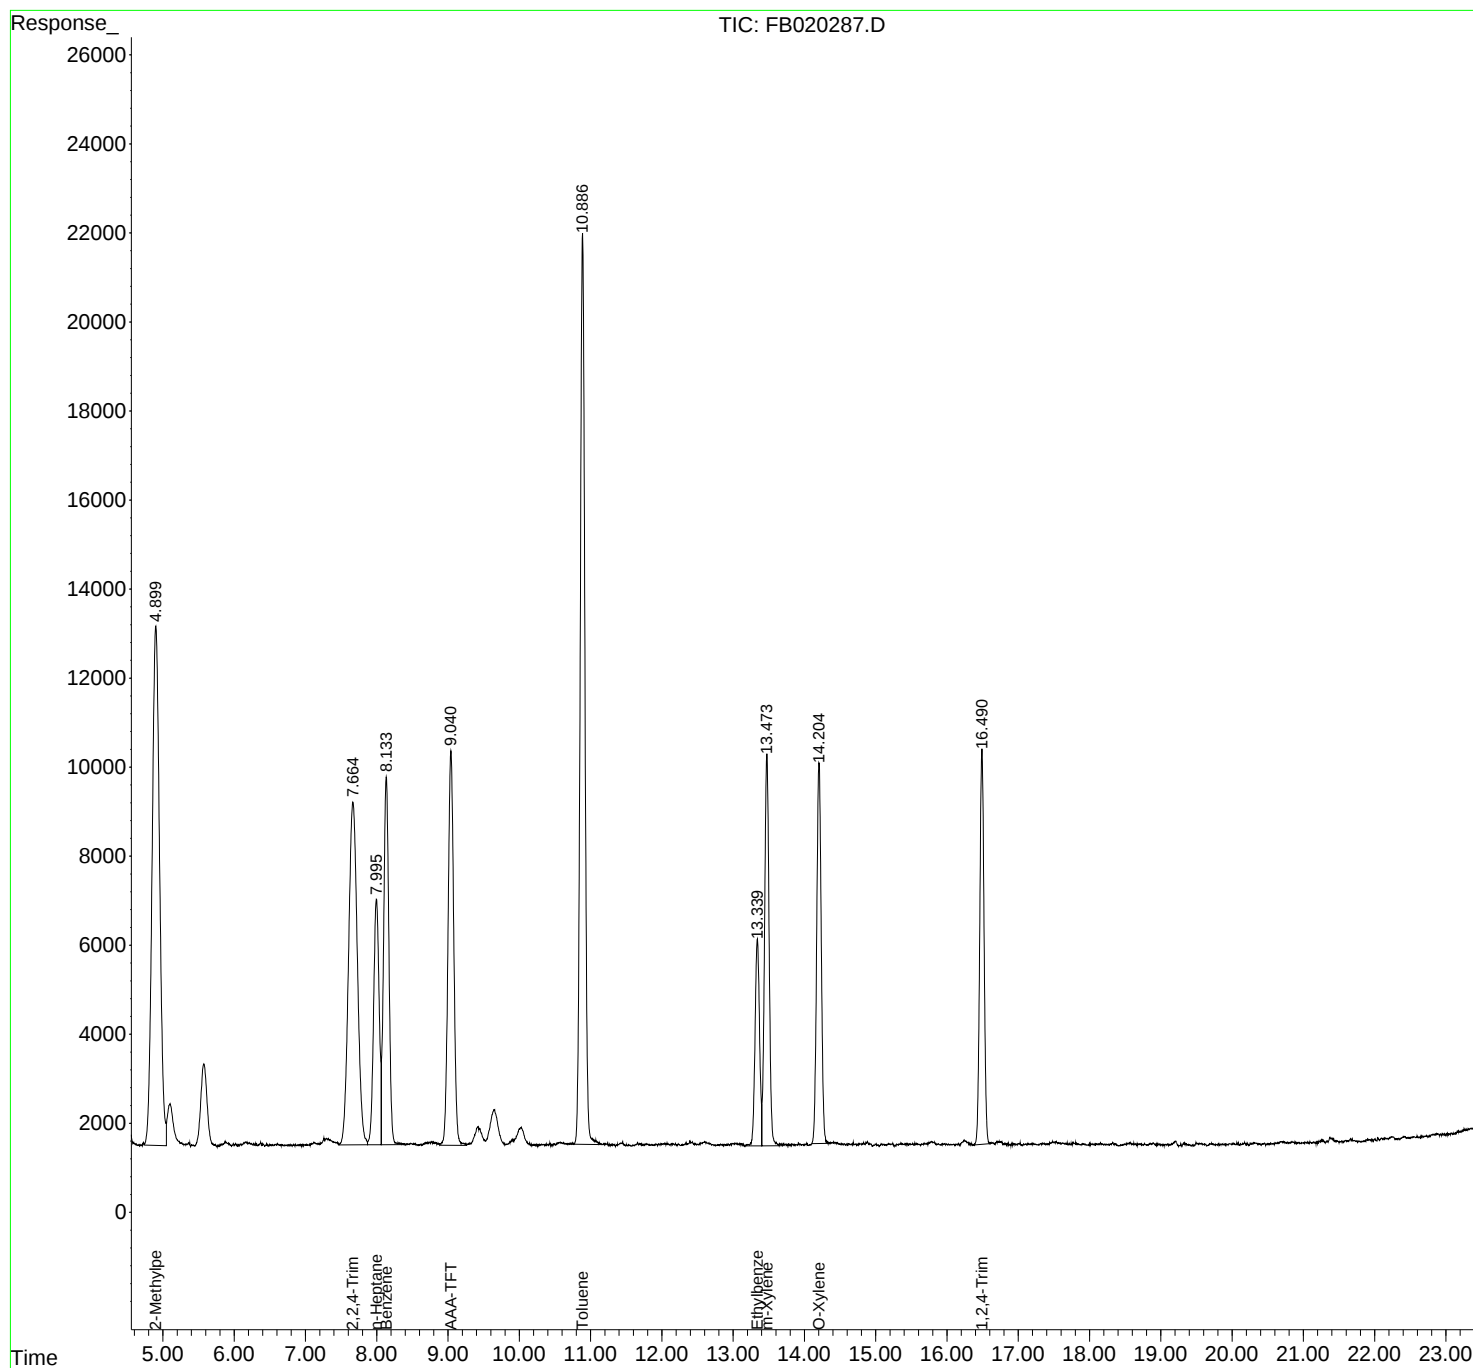


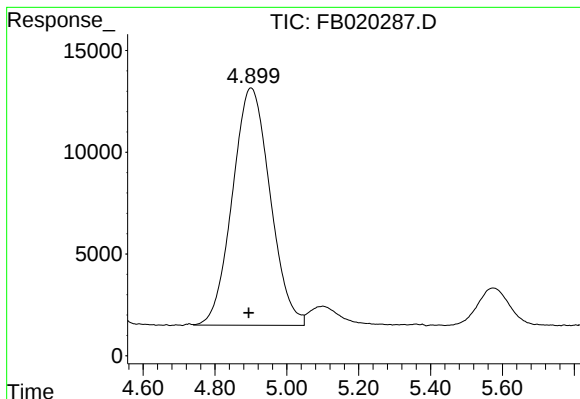

#1 2-Methylpentane


R.T.: 4.901 min
Delta R.T.: 0.007 min
Response: 849624
Conc: 25.19 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-031819MSD

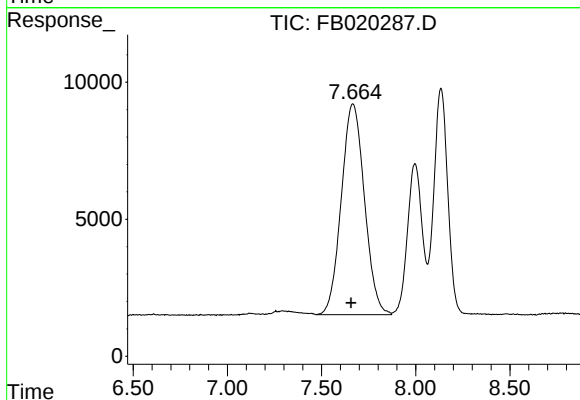


#2 2,2,4-Trimethylpentane

R.T.: 7.666 min
Delta R.T.: 0.009 min
Response: 656832
Conc: 20.03 ng/ml

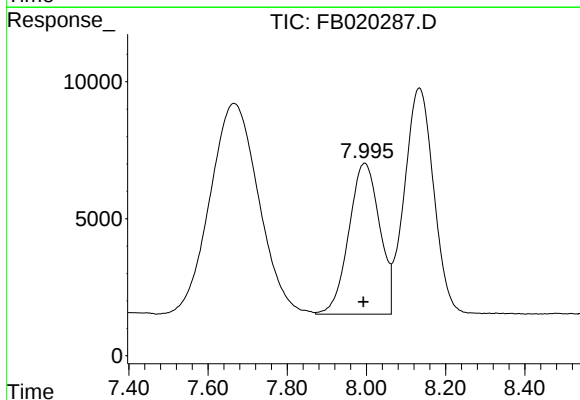


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.004 min
Response: 297130
Conc: 7.14 ng/ml

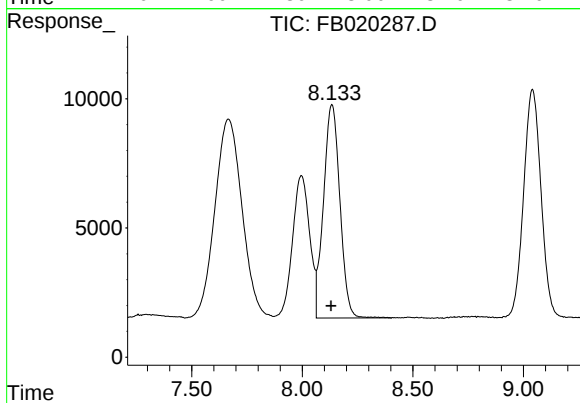

#4 Benzene


R.T.: 8.134 min
Delta R.T.: 0.004 min
Response: 425589
Conc: 9.14 ng/ml

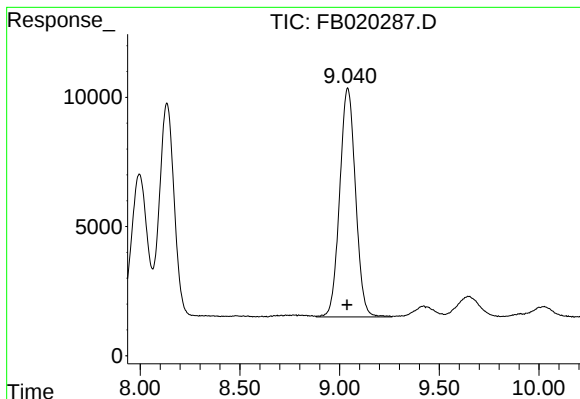

#5 AAA-TFT


R.T.: 9.041 min
Delta R.T.: 0.003 min
Response: 488788
Conc: 18.62 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-031819MSD

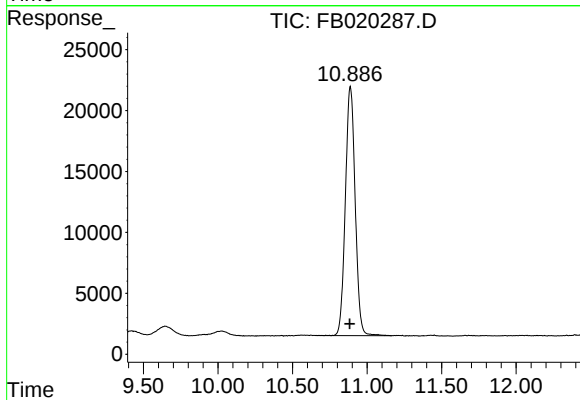


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.003 min
Response: 936422
Conc: 25.34 ng/ml

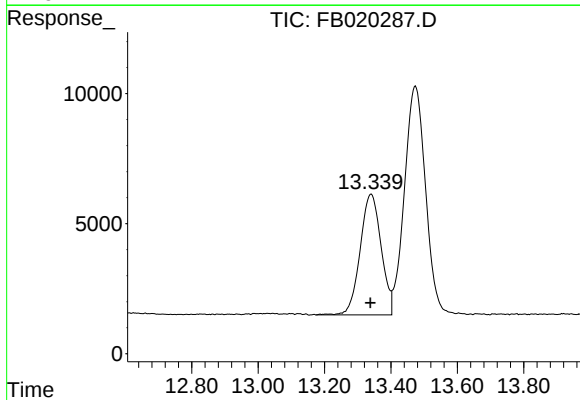


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: 0.003 min
Response: 203525
Conc: 8.65 ng/ml

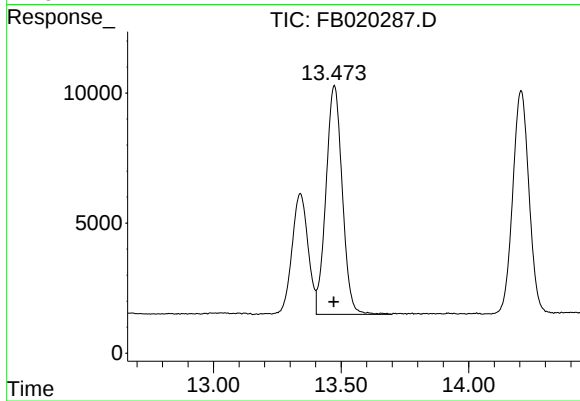

#8 m-Xylene


R.T.: 13.474 min
Delta R.T.: 0.002 min
Response: 390962
Conc: 18.33 ng/ml

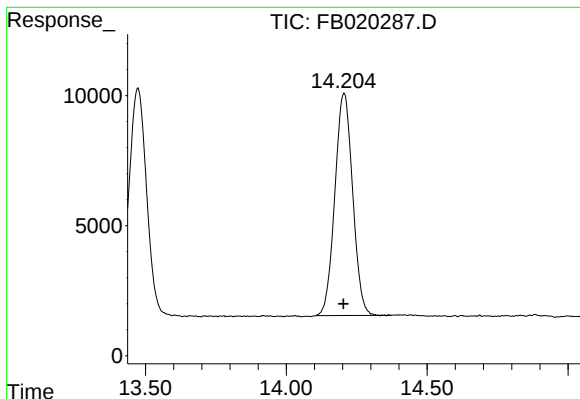

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.002 min
Response: 374886
Conc: 19.79 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-031819MSD

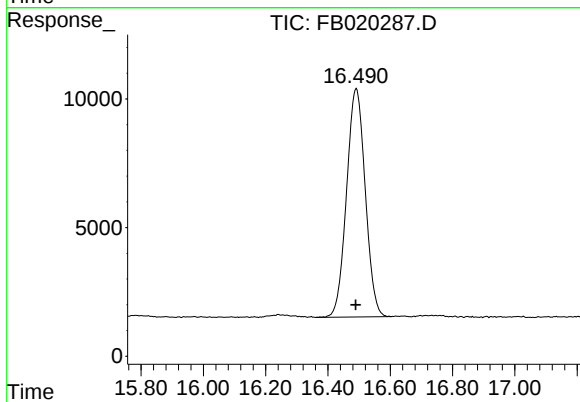

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.002 min
Response: 370305
Conc: 18.67 ng/ml