

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031920\
 Data File : FB023999.D
 Signal(s) : FID2B.CH
 Acq On : 19 Mar 2020 16:08
 Operator : DD/AJ
 Sample : L1978-11
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 20 00:49:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	614688	29.200 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.681	2285	0.074 ng/ml
2) t 2,2,4-Trimethylpentane	7.446	515	0.015 ng/ml
6) t Toluene	10.618	306	0.008 ng/ml
7) t Ethylbenzene	13.047	4460	0.117 ng/ml
8) t m-Xylene	13.141	1298	0.035 ng/ml
9) t O-Xylene	13.957	321	0.009 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031920\
Data File : FB023999.D
Signal(s) : FID2B.CH
Acq On : 19 Mar 2020 16:08
Operator : DD/AJ
Sample : L1978-11
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 20 00:49:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

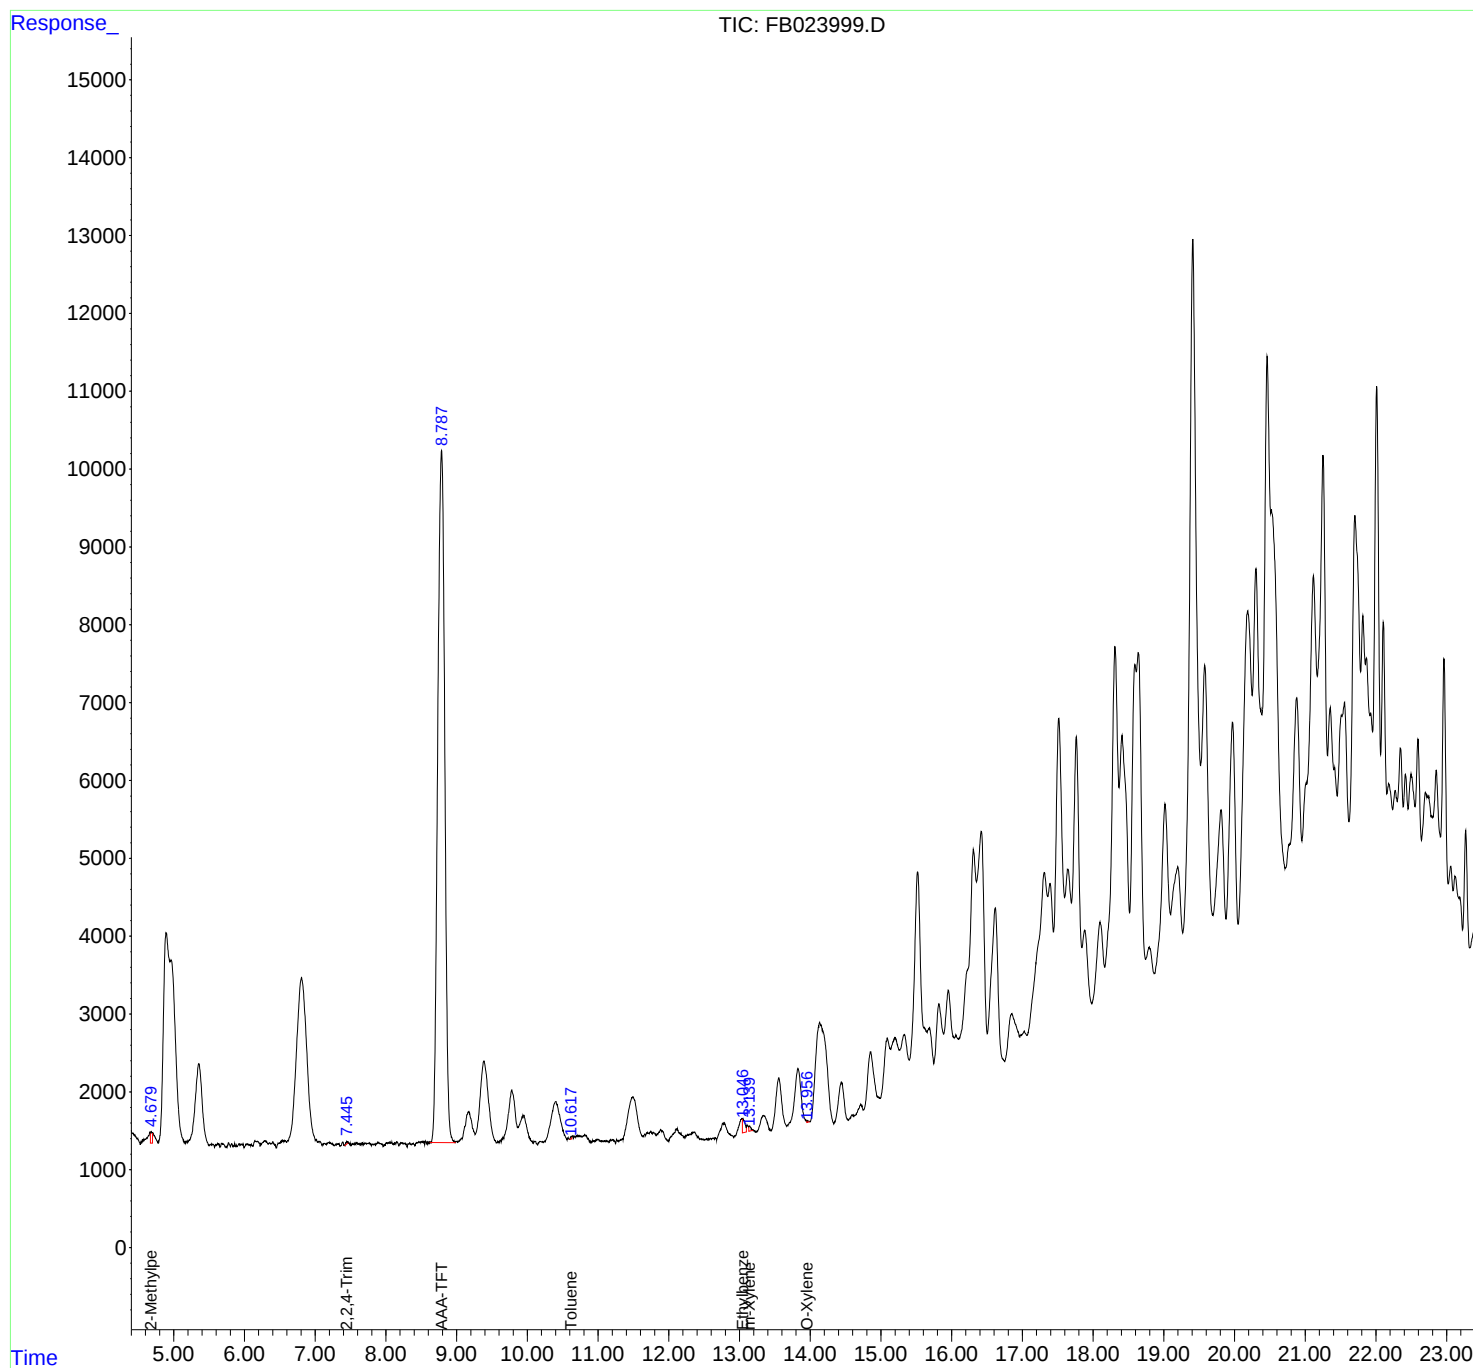

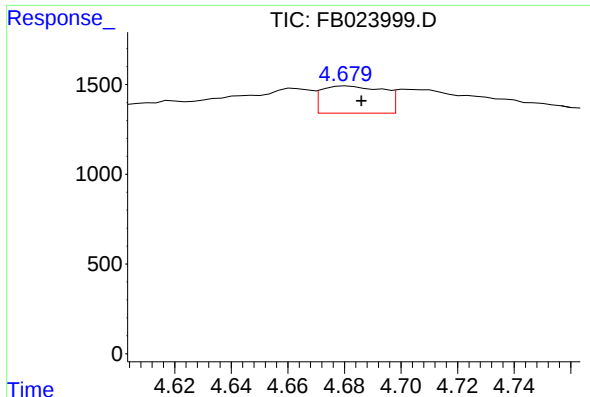


#1 2-Methylpentane

R.T.: 4.681 min
Delta R.T.: -0.005 min
Response: 2285
Conc: 0.07 ng/ml

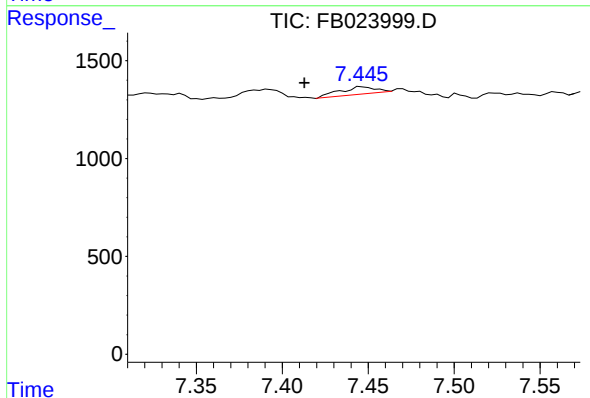


#2 2,2,4-Trimethylpentane

R.T.: 7.446 min
Delta R.T.: 0.033 min
Response: 515
Conc: 0.02 ng/ml

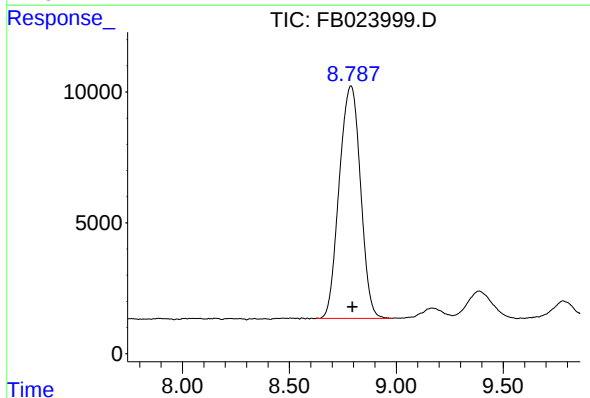


#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: -0.006 min
Response: 614688
Conc: 29.20 ng/ml

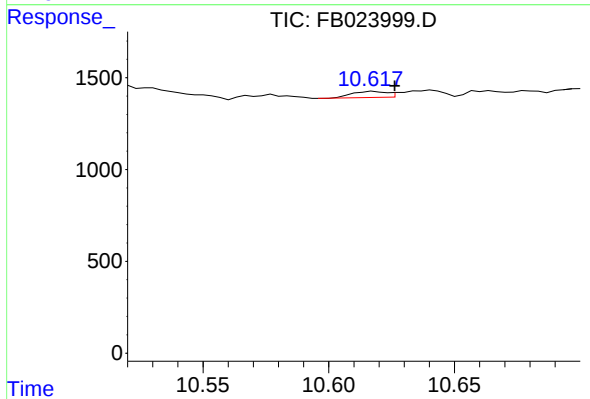


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.008 min
Response: 306
Conc: 0.01 ng/ml

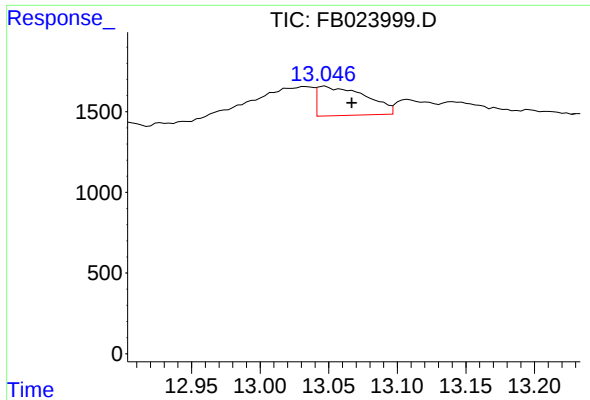


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.019 min
Response: 4460
Conc: 0.12 ng/ml

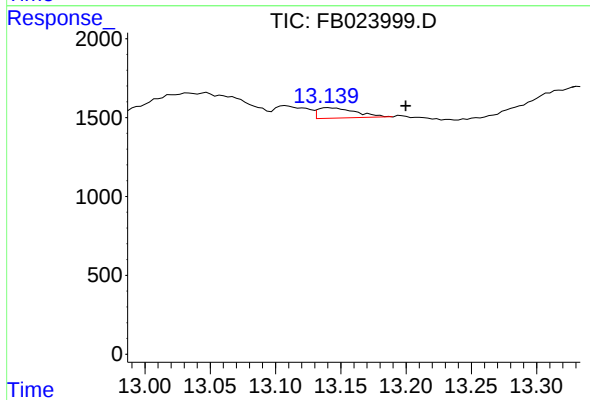

#8 m-Xylene

R.T.: 13.141 min
Delta R.T.: -0.059 min
Response: 1298
Conc: 0.04 ng/ml

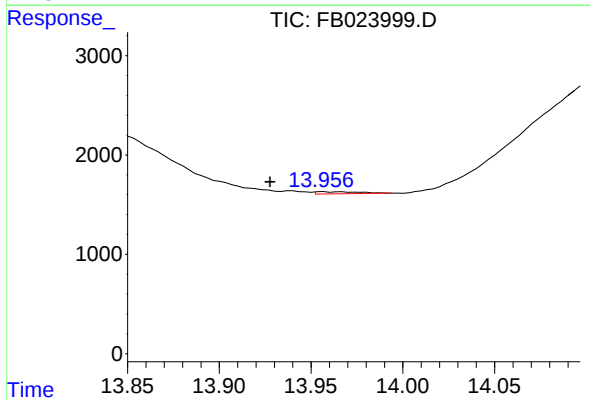

#9 O-Xylene

R.T.: 13.957 min
Delta R.T.: 0.030 min
Response: 321
Conc: 0.01 ng/ml