

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031920\
 Data File : FB023995.D
 Signal(s) : FID2B.CH
 Acq On : 19 Mar 2020 14:07
 Operator : DD/AJ
 Sample : L1978-03MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 20 00:48:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	425049	20.192 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	687706	22.252 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	703913	20.875 ng/ml
3) t n-Heptane	7.757	221646	6.690 ng/ml
4) t Benzene	7.891	359917	8.596 ng/ml
6) t Toluene	10.629	1023789	25.109 ng/ml
7) t Ethylbenzene	13.068	305083	7.985 ng/ml
8) t m-Xylene	13.202	592542	16.094 ng/ml
9) t O-Xylene	13.929	578675	16.271 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	493147	16.278 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031920\
Data File : FB023995.D
Signal(s) : FID2B.CH
Acq On : 19 Mar 2020 14:07
Operator : DD/AJ
Sample : L1978-03MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 20 00:48:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

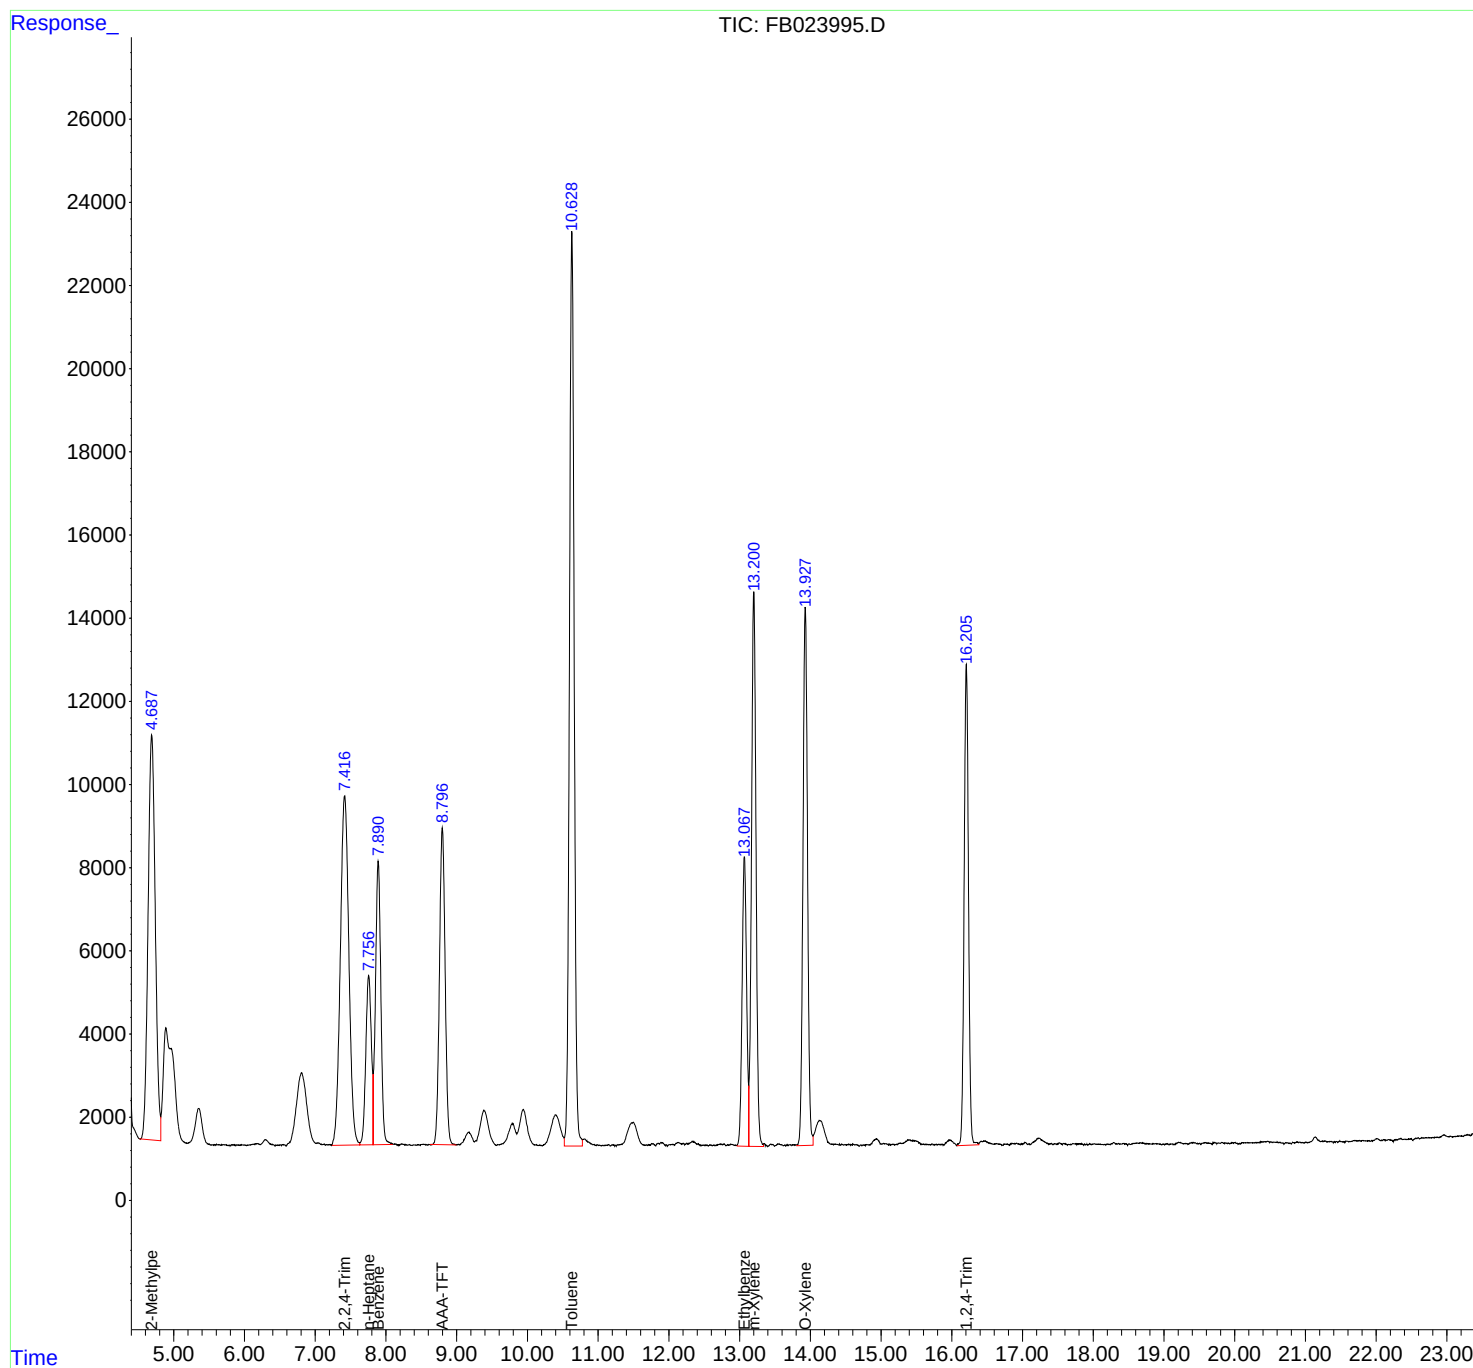

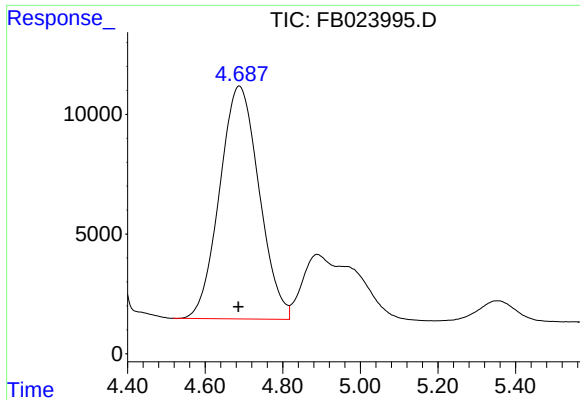


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.003 min
Response: 687706
Conc: 22.25 ng/ml

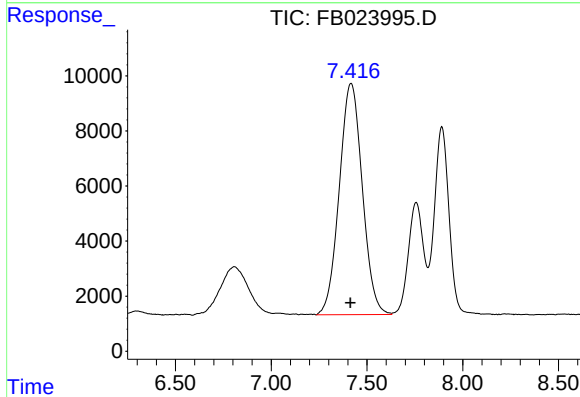


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.004 min
Response: 703913
Conc: 20.87 ng/ml

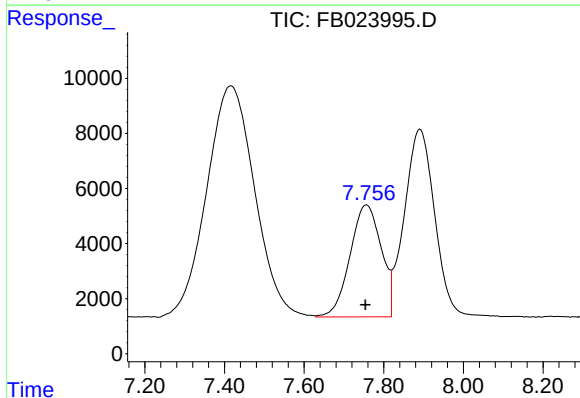


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.003 min
Response: 221646
Conc: 6.69 ng/ml

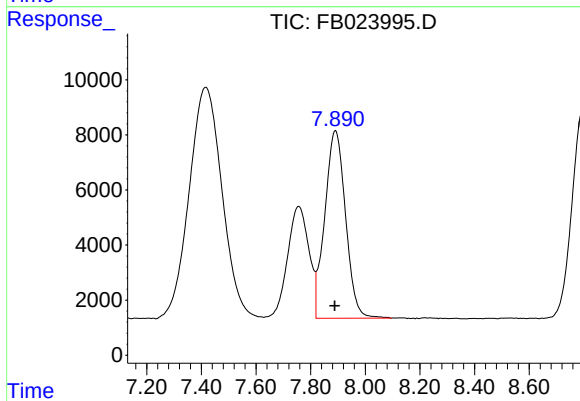


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.003 min
Response: 359917
Conc: 8.60 ng/ml

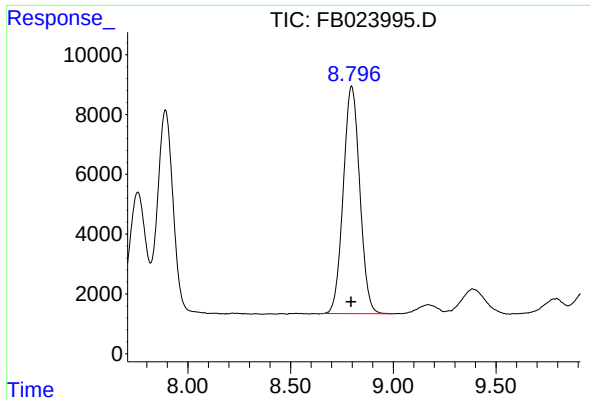


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.003 min
Response: 425049
Conc: 20.19 ng/ml

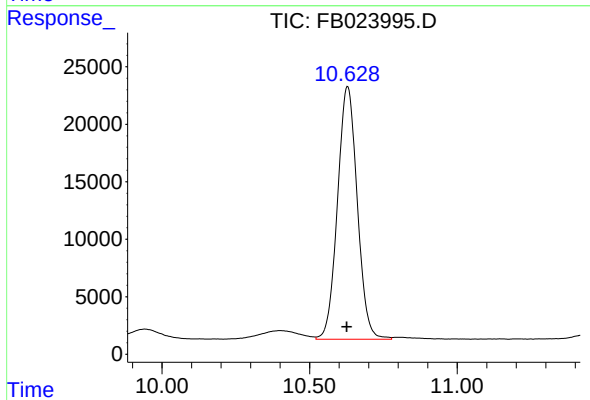


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.003 min
Response: 1023789
Conc: 25.11 ng/ml

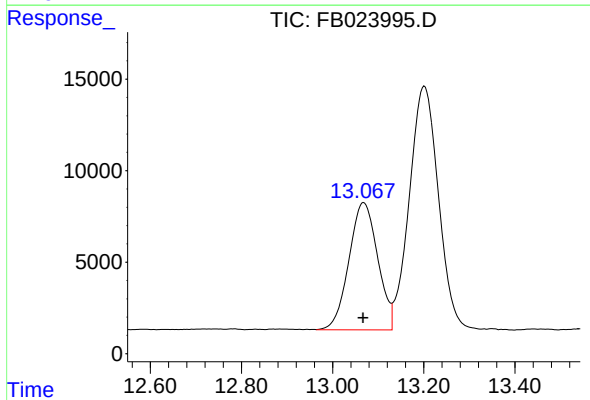


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: 0.002 min
Response: 305083
Conc: 7.99 ng/ml

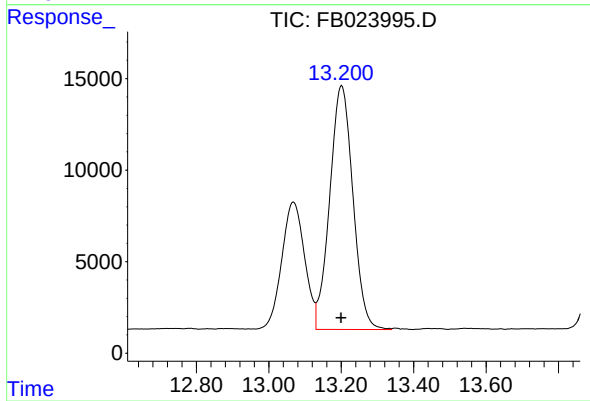


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.002 min
Response: 592542
Conc: 16.09 ng/ml

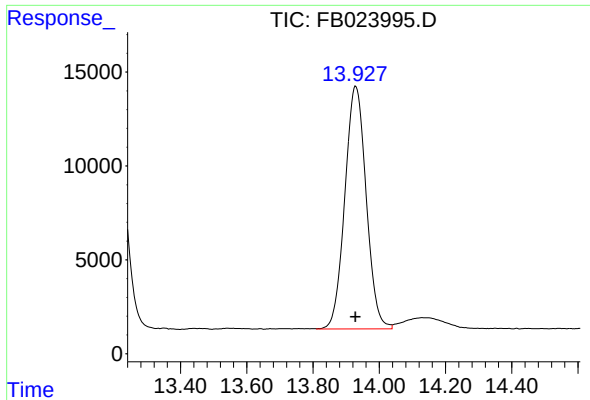

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.001 min
Response: 578675
Conc: 16.27 ng/ml

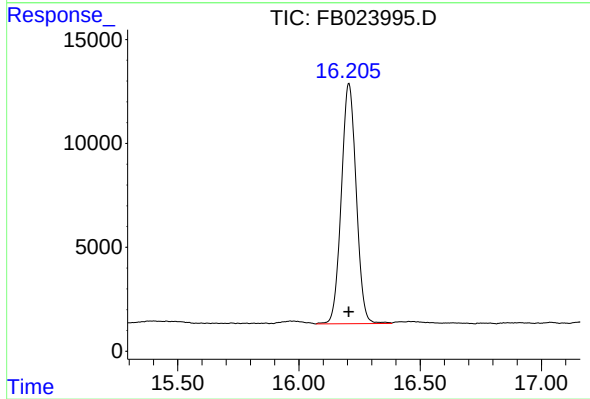

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 493147
Conc: 16.28 ng/ml