

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032019\
 Data File : FB020329.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2019 00:39
 Operator : MJ/SJ
 Sample : K1994-03 50X
 Misc : 5.00g/5.00ml DI DI WATER
 ALS Vial : 32 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 21 07:33:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	482504	18.379 ng/ml
Target Compounds			
7) t Ethylbenzene	13.319	27690	1.177 ng/ml
8) t m-Xylene	13.473	14620	0.685 ng/ml
9) t O-Xylene	14.208	9091	0.480 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	130599	6.585 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032019\
Data File : FB020329.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2019 00:39
Operator : MJ/SJ
Sample : K1994-03 50X
Misc : 5.00g/5.00ml DI DI WATER
ALS Vial : 32 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 21 07:33:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

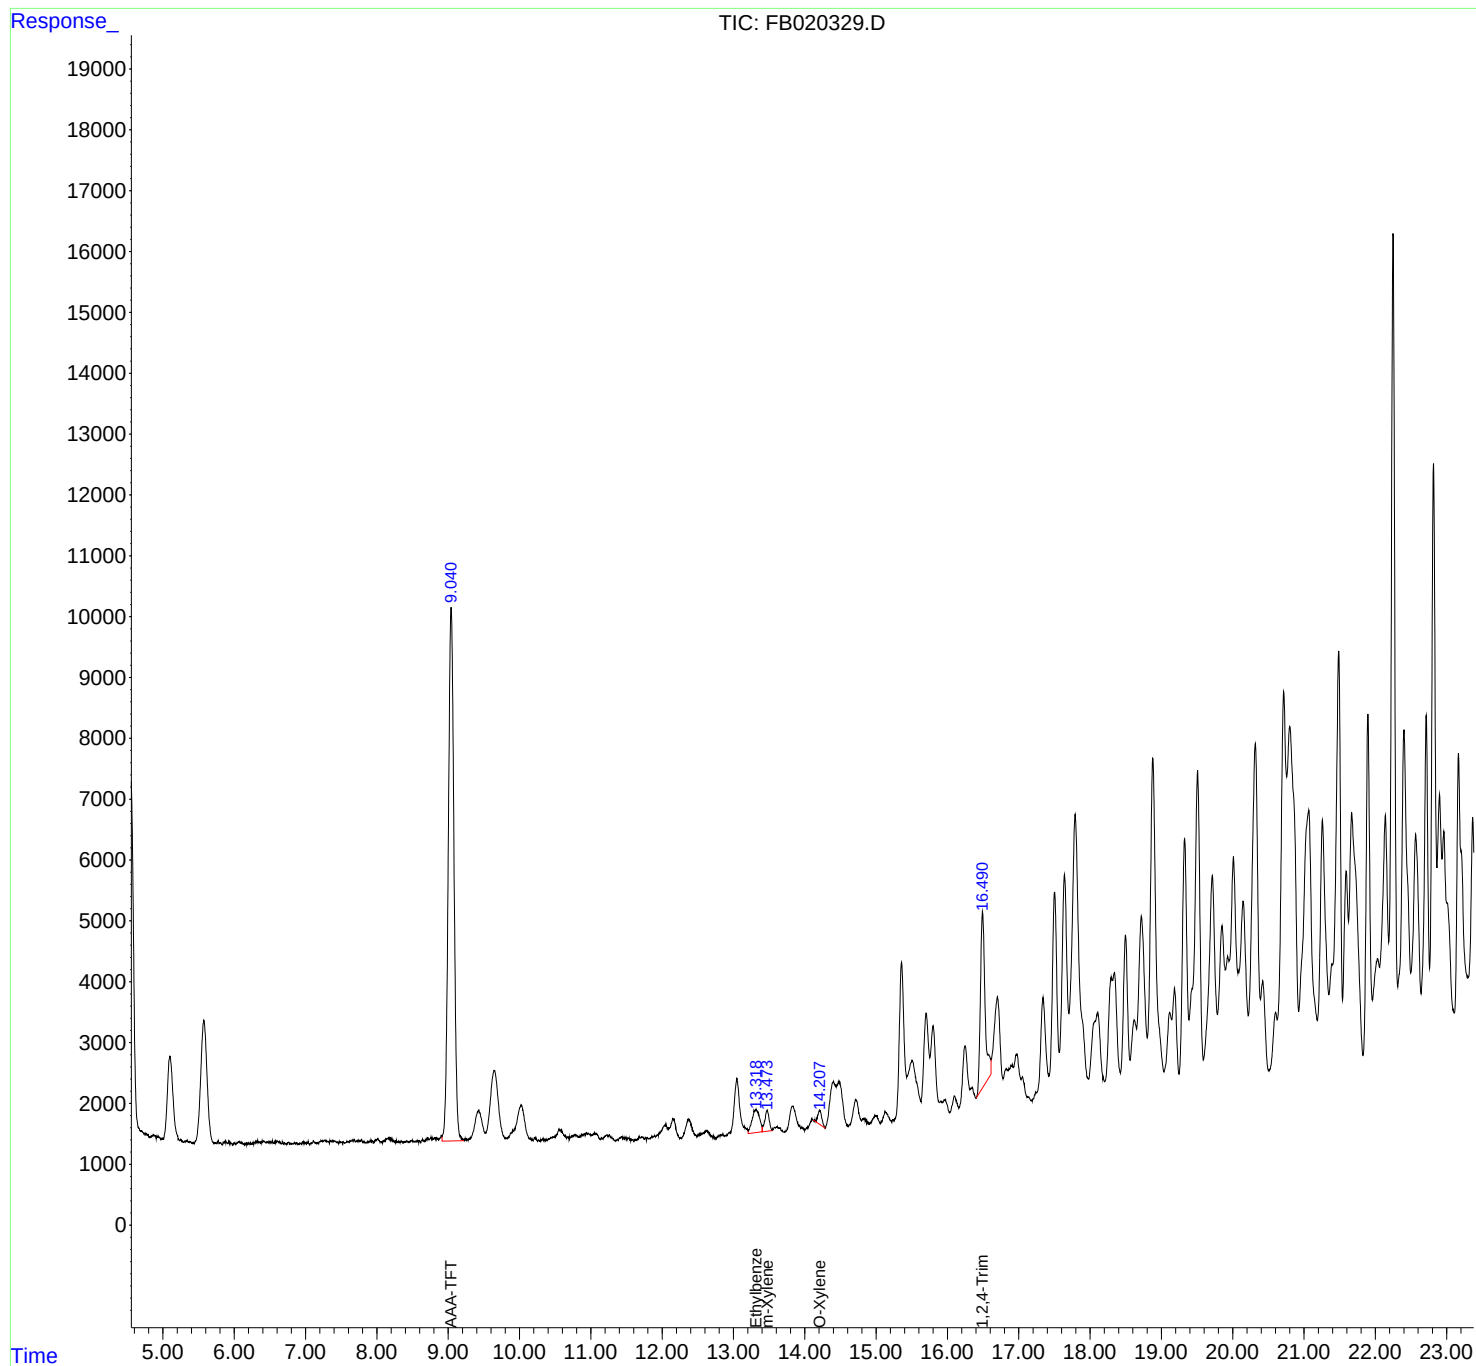

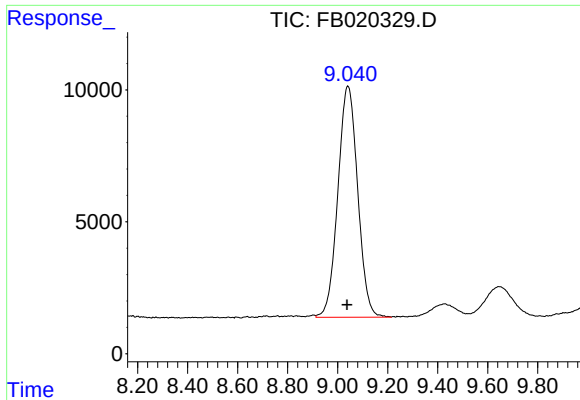


#5 AAA-TFT

R.T.: 9.042 min
 Delta R.T.: 0.003 min
 Response: 482504
 Conc: 18.38 ng/ml

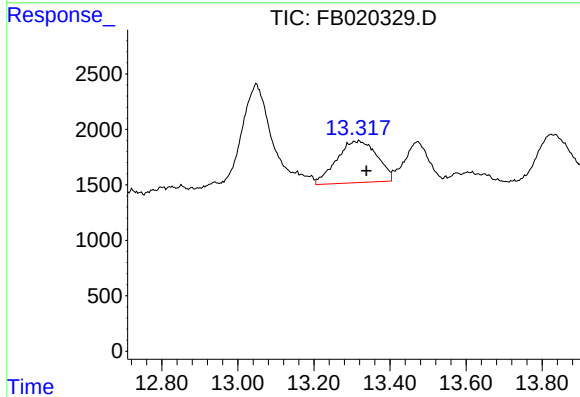


#7 Ethylbenzene

R.T.: 13.319 min
 Delta R.T.: -0.019 min
 Response: 27690
 Conc: 1.18 ng/ml

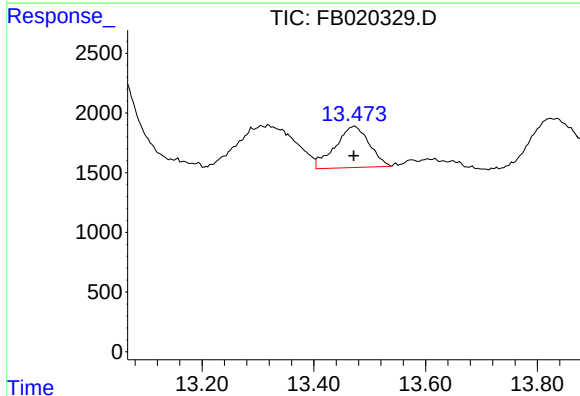


#8 m-Xylene

R.T.: 13.473 min
 Delta R.T.: 0.002 min
 Response: 14620
 Conc: 0.69 ng/ml

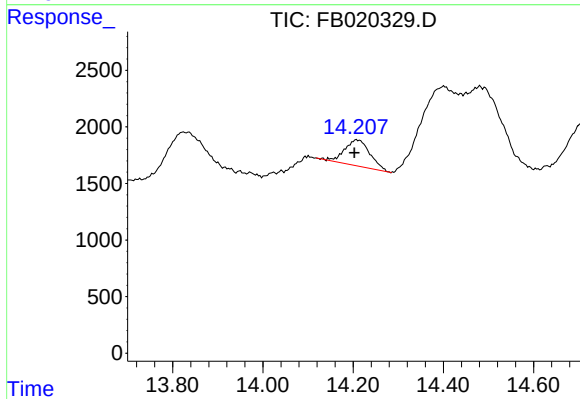

#9 O-Xylene

R.T.: 14.208 min
 Delta R.T.: 0.004 min
 Response: 9091
 Conc: 0.48 ng/ml

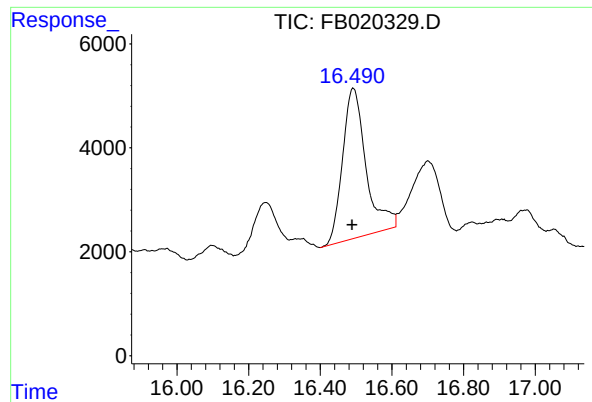

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: 0.004 min
Response: 130599
Conc: 6.59 ng/ml