

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032019\
 Data File : FB020301.D
 Signal(s) : FID2B.CH
 Acq On : 20 Mar 2019 9:48
 Operator : MJ/SJ
 Sample : BSF0320S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 20 15:53:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.039	531962	20.263 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.897	1015981	30.118 ng/ml
2) t	2,2,4-Trimethylpentane	7.663	908343	27.698 ng/ml
3) t	n-Heptane	7.994	420231	10.098 ng/ml
4) t	Benzene	8.132	453363	9.738 ng/ml
6) t	Toluene	10.886	1036302	28.044 ng/ml
7) t	Ethylbenzene	13.338	223941	9.518 ng/ml
8) t	m-Xylene	13.471	430188	20.167 ng/ml
9) t	O-Xylene	14.204	407355	21.504 ng/ml
10) t	1,2,4-Trimethylbenzene	16.489	428710	21.617 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032019\
Data File : FB020301.D
Signal(s) : FID2B.CH
Acq On : 20 Mar 2019 9:48
Operator : MJ/SJ
Sample : BSF0320S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 20 15:53:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

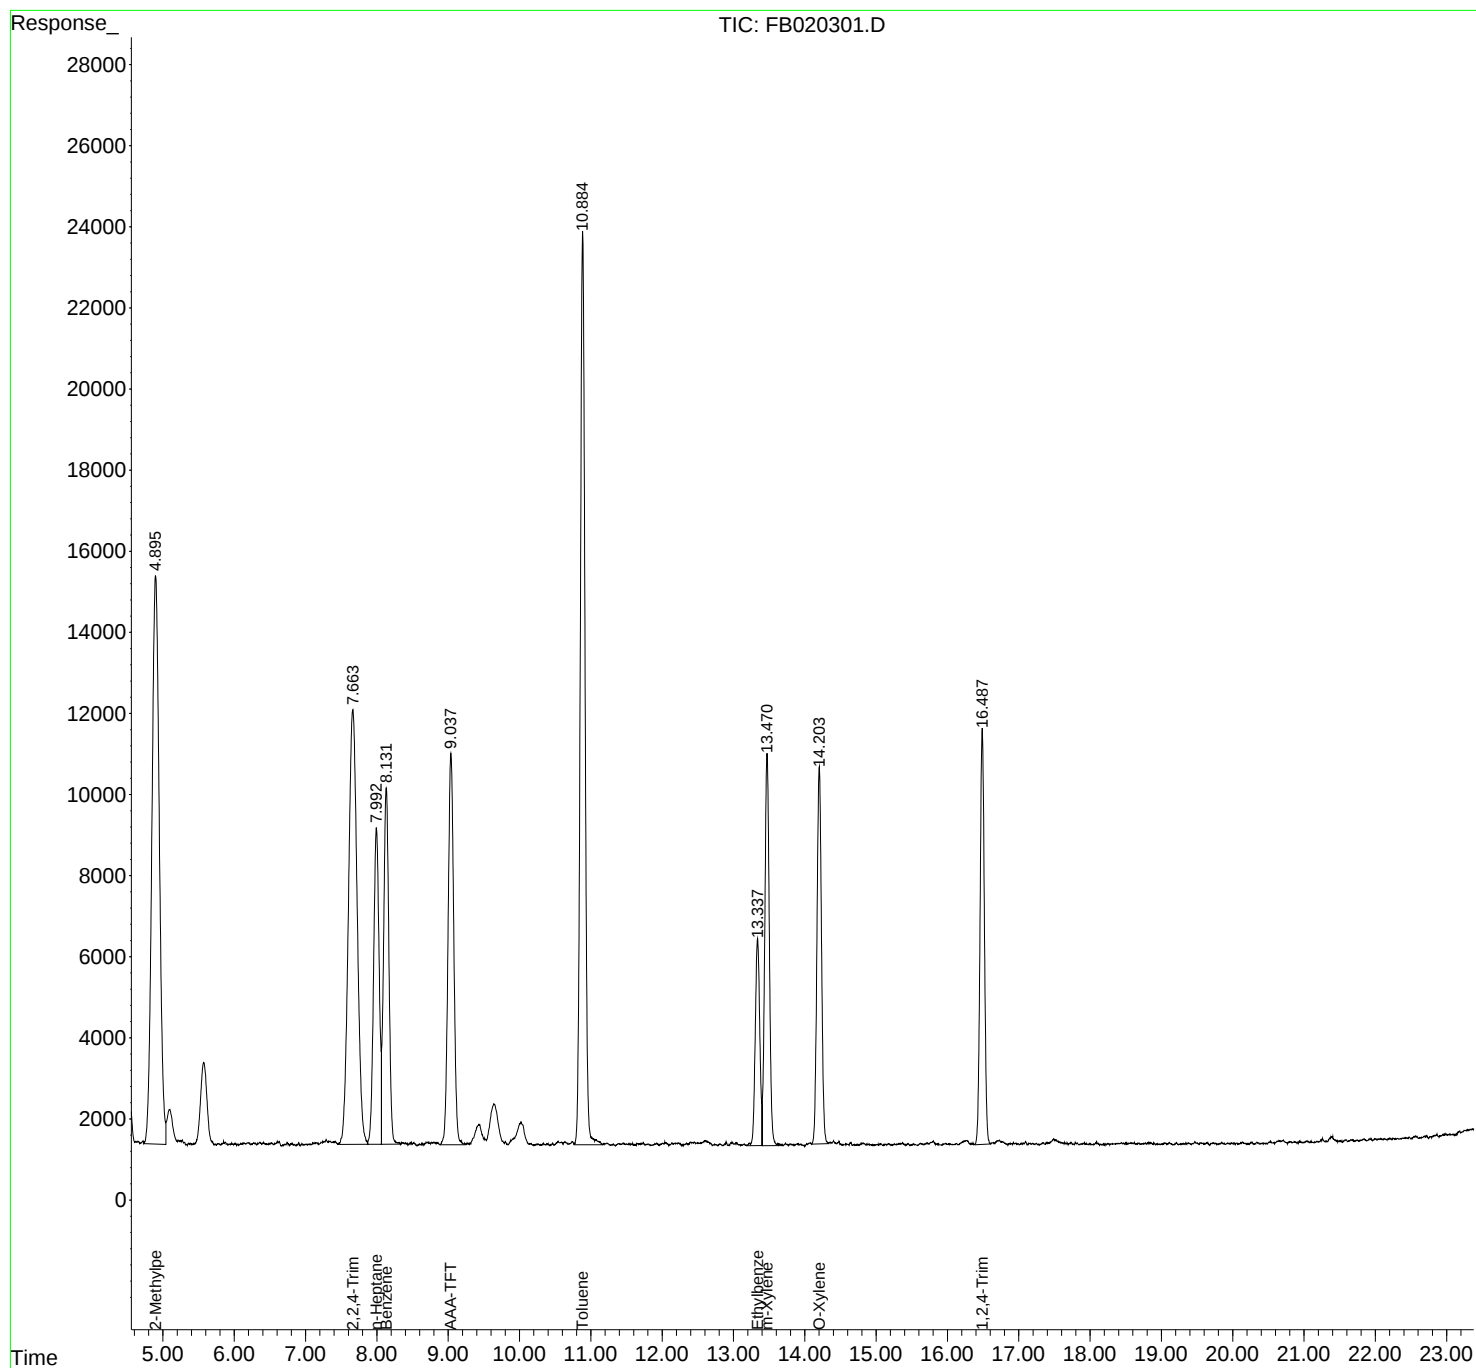

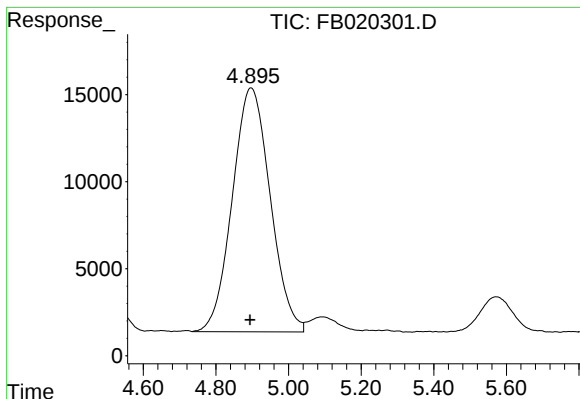


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: 0.003 min
Response: 1015981
Conc: 30.12 ng/ml

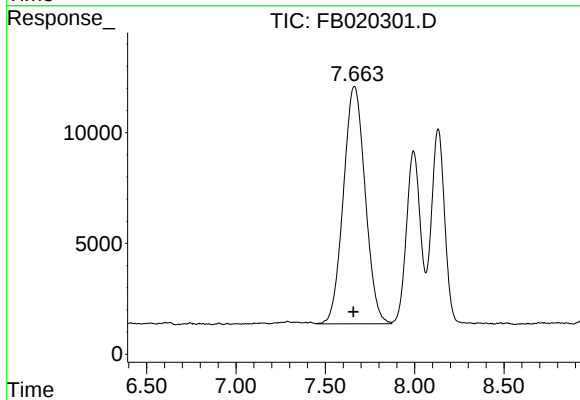


#2 2,2,4-Trimethylpentane

R.T.: 7.663 min
Delta R.T.: 0.006 min
Response: 908343
Conc: 27.70 ng/ml

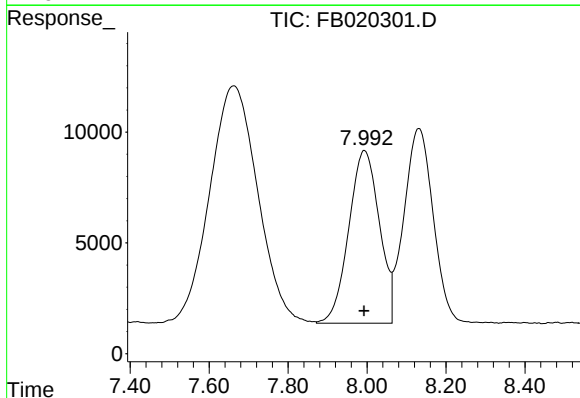


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: 0.002 min
Response: 420231
Conc: 10.10 ng/ml

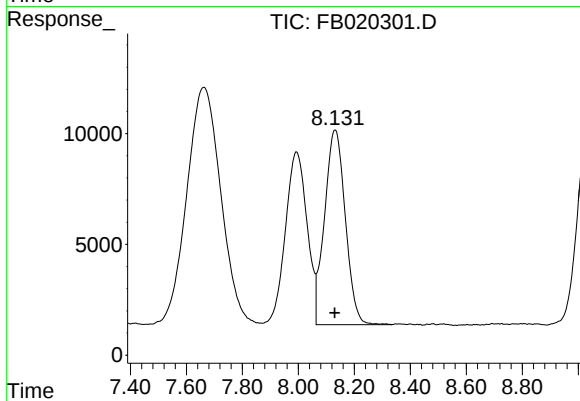


#4 Benzene

R.T.: 8.132 min
Delta R.T.: 0.002 min
Response: 453363
Conc: 9.74 ng/ml

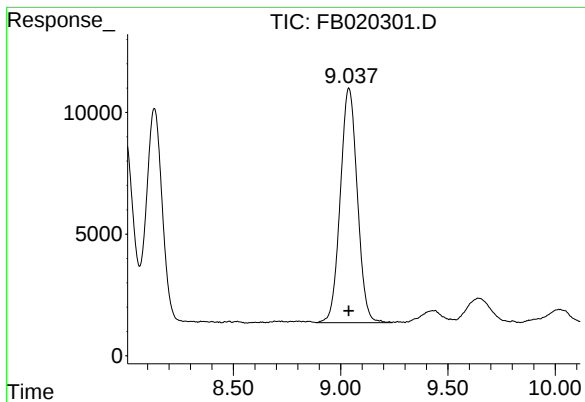


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 531962
Conc: 20.26 ng/ml

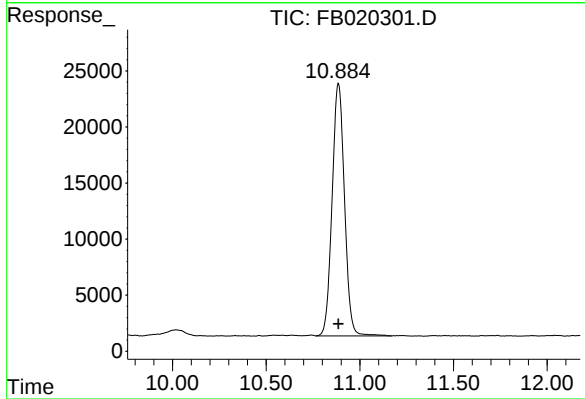


#6 Toluene

R.T.: 10.886 min
Delta R.T.: 0.000 min
Response: 1036302
Conc: 28.04 ng/ml

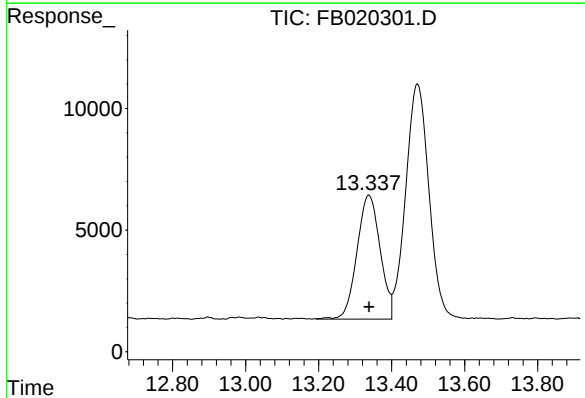


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.000 min
Response: 223941
Conc: 9.52 ng/ml

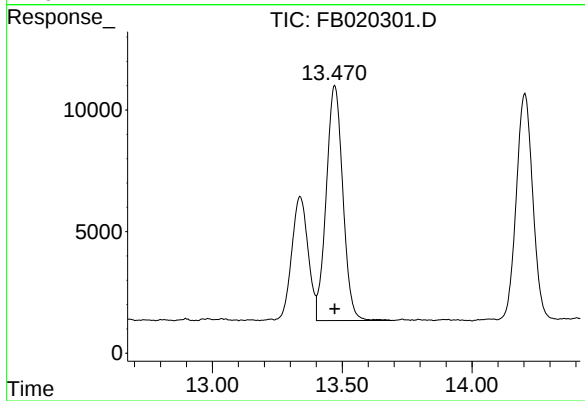


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: 0.000 min
Response: 430188
Conc: 20.17 ng/ml

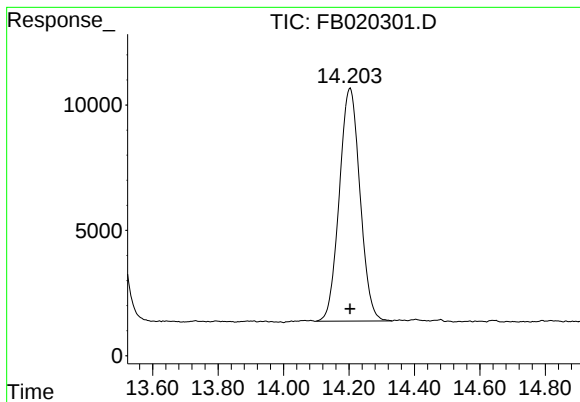

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.000 min
Response: 407355
Conc: 21.50 ng/ml

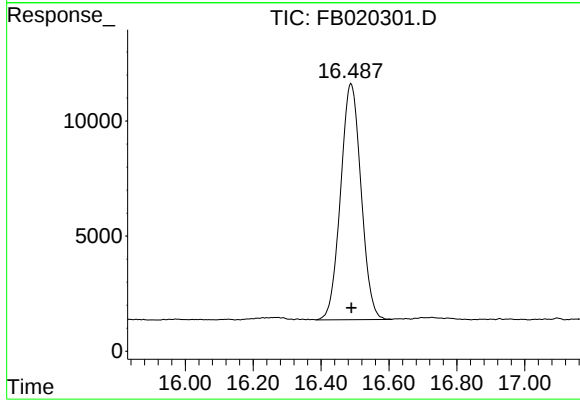

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.000 min
Response: 428710
Conc: 21.62 ng/ml