

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032020\
 Data File : FB024003.D
 Signal(s) : FID2B.CH
 Acq On : 20 Mar 2020 15:03
 Operator : DD/AJ
 Sample : BSF0320S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 20 23:02:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	426956	20.282 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.692	900184	29.127 ng/ml
2) t	2,2,4-Trimethylpentane	7.418	1063866	31.549 ng/ml
3) t	n-Heptane	7.759	339490	10.247 ng/ml
4) t	Benzene	7.894	421536	10.067 ng/ml
6) t	Toluene	10.632	1231007	30.191 ng/ml
7) t	Ethylbenzene	13.072	379608	9.936 ng/ml
8) t	m-Xylene	13.205	731897	19.879 ng/ml
9) t	O-Xylene	13.933	703779	19.788 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	608315	20.080 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032020\
Data File : FB024003.D
Signal(s) : FID2B.CH
Acq On : 20 Mar 2020 15:03
Operator : DD/AJ
Sample : BSF0320S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 20 23:02:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

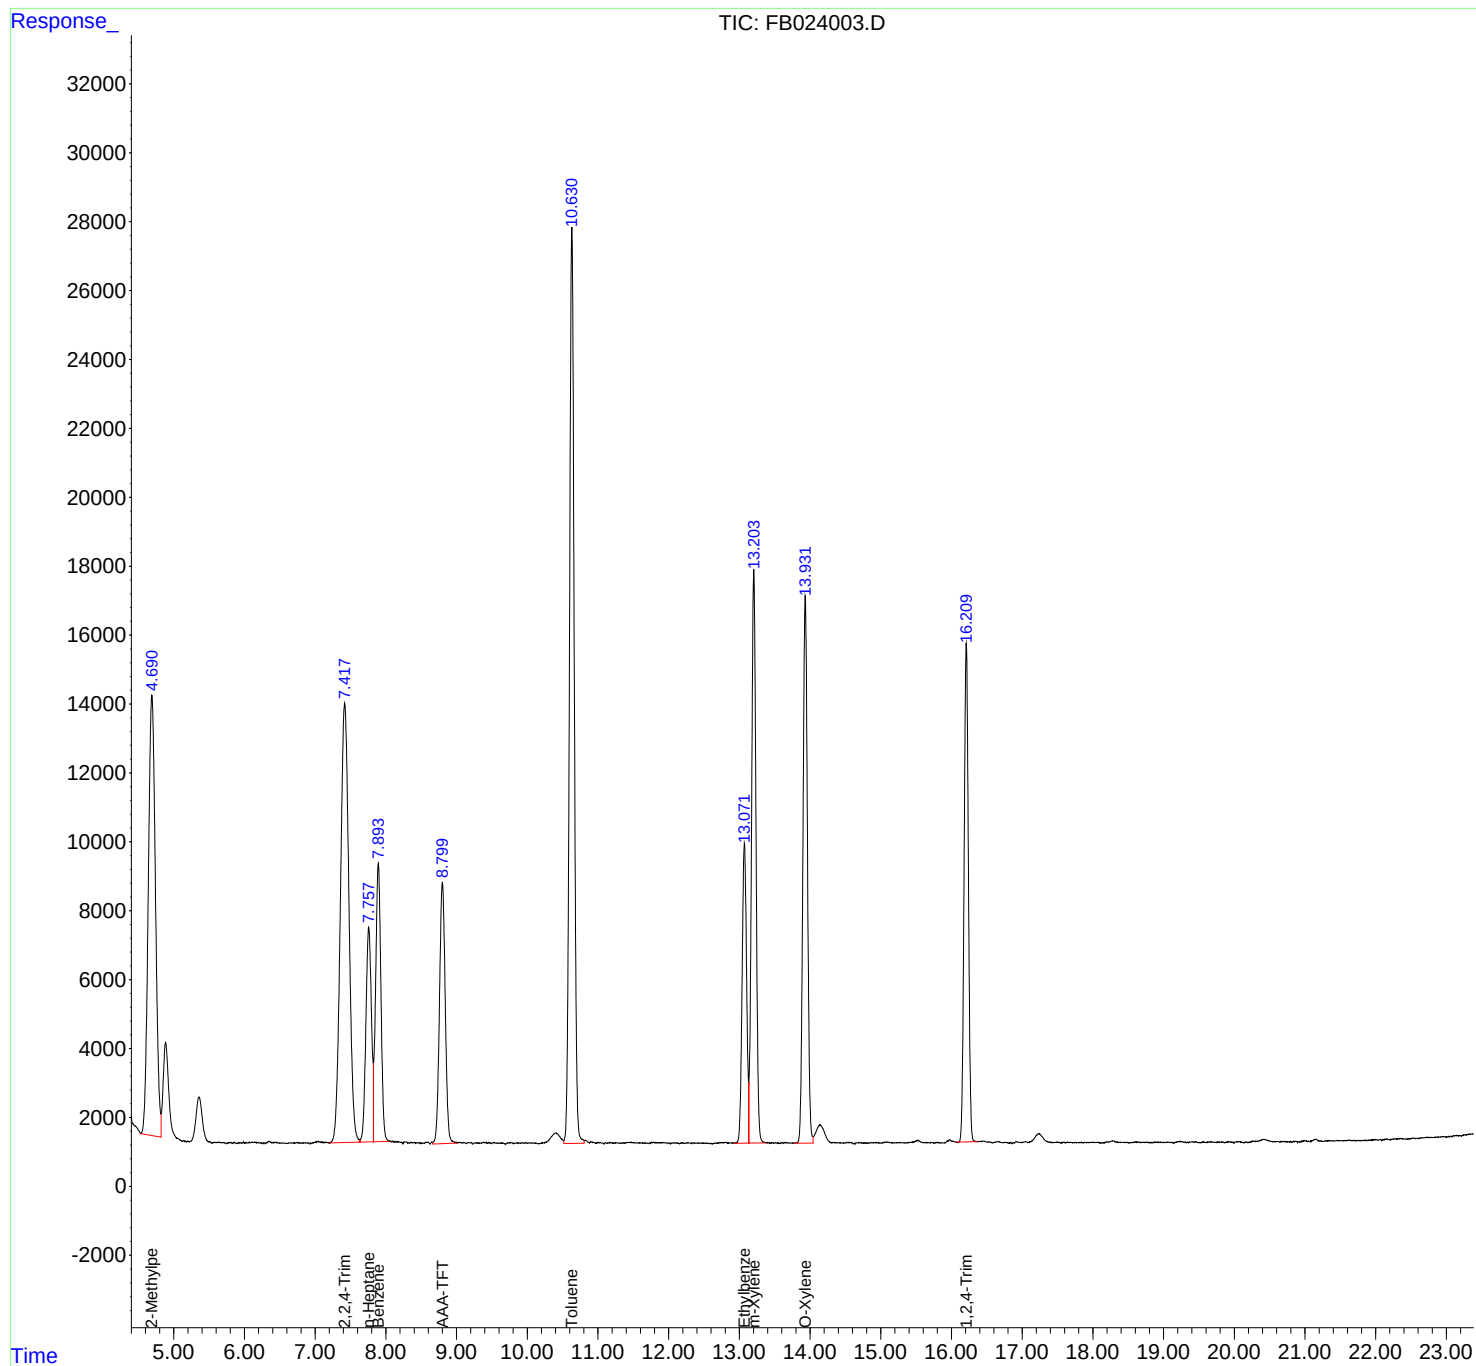

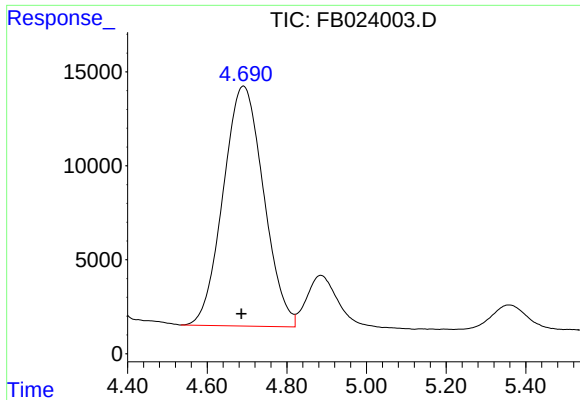


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.006 min
Response: 900184
Conc: 29.13 ng/ml

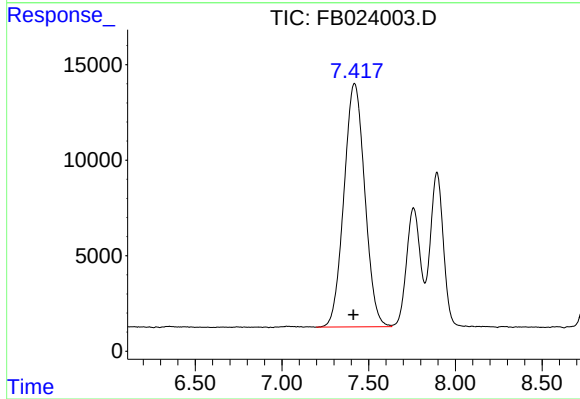


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.005 min
Response: 1063866
Conc: 31.55 ng/ml

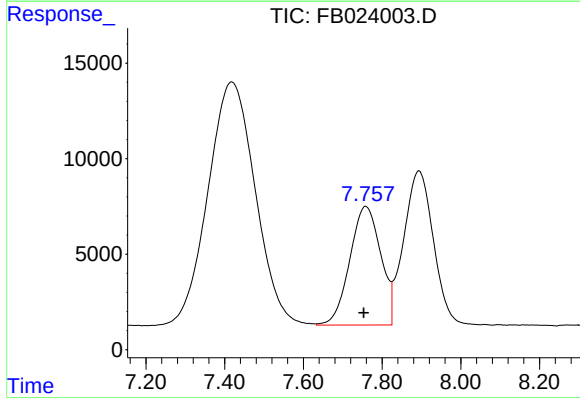


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.005 min
Response: 339490
Conc: 10.25 ng/ml

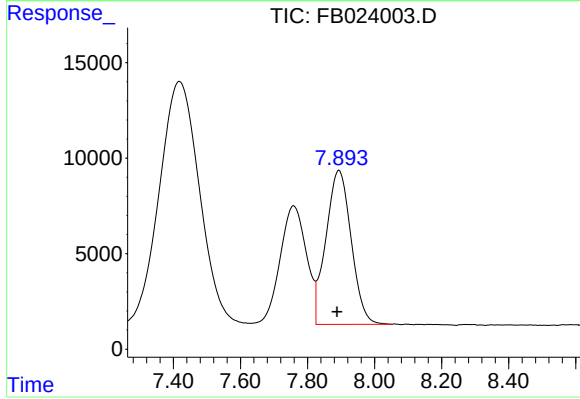


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.006 min
Response: 421536
Conc: 10.07 ng/ml

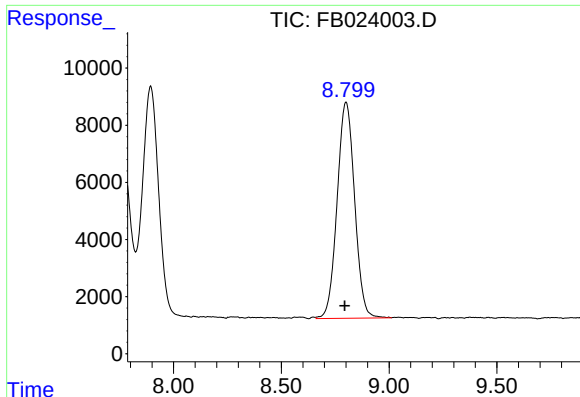


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.006 min
Response: 426956
Conc: 20.28 ng/ml

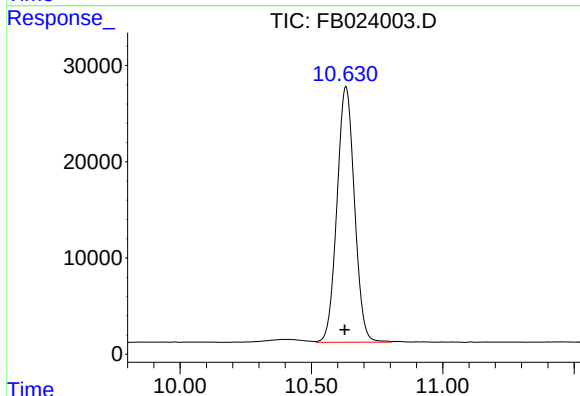


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.005 min
Response: 1231007
Conc: 30.19 ng/ml

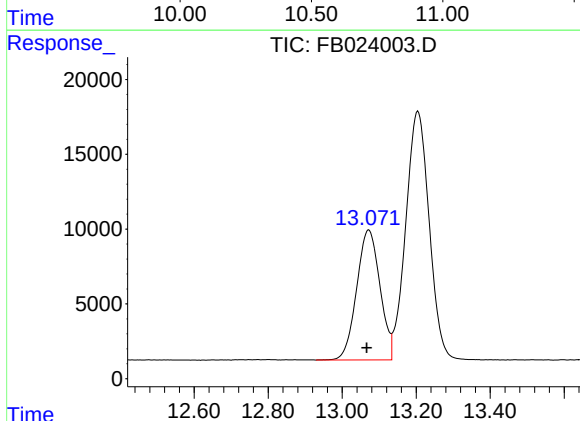


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.005 min
Response: 379608
Conc: 9.94 ng/ml

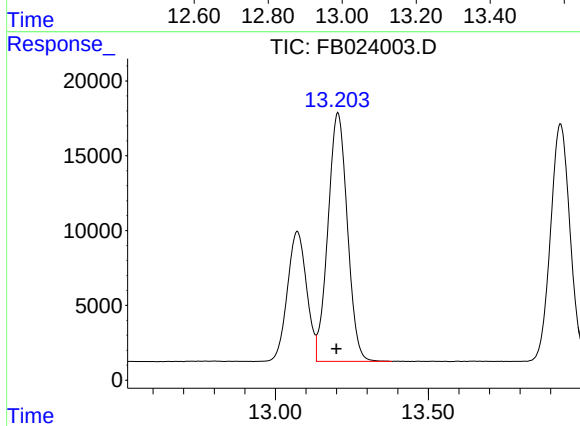


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.005 min
Response: 731897
Conc: 19.88 ng/ml

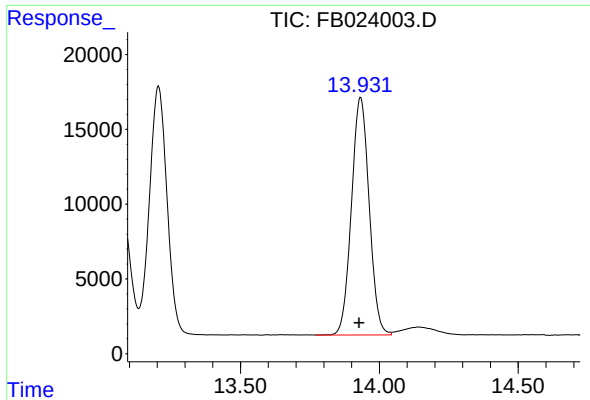

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.005 min
Response: 703779
Conc: 19.79 ng/ml

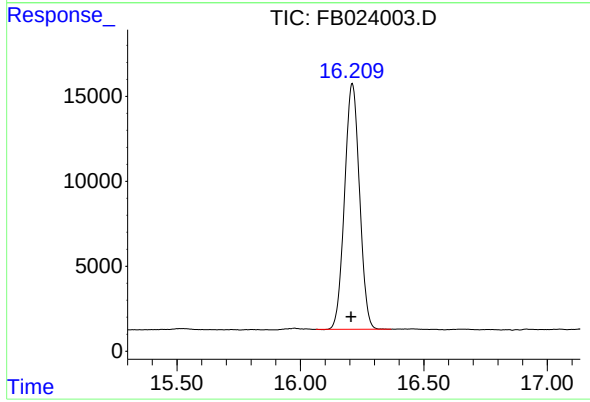

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.005 min
Response: 608315
Conc: 20.08 ng/ml