

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032023\
 Data File : FB029525.D
 Signal(s) : FID2B.CH
 Acq On : 20 Mar 2023 9:46
 Operator : YP/AJ
 Sample : BSF0320W1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 21 05:18:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	267834	22.106 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	436637	28.456 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	489733	29.073 ng/ml
3) t n-Heptane	7.748	169325	9.790 ng/ml
4) t Benzene	7.884	204249	10.062 ng/ml
6) t Toluene	10.617	601145	30.455 ng/ml
7) t Ethylbenzene	13.054	188237	10.111 ng/ml
8) t m-Xylene	13.186	370653	19.924 ng/ml
9) t O-Xylene	13.913	355730	19.319 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	345404	18.544 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032023\
Data File : FB029525.D
Signal(s) : FID2B.CH
Acq On : 20 Mar 2023 9:46
Operator : YP/AJ
Sample : BSF0320W1
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 21 05:18:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

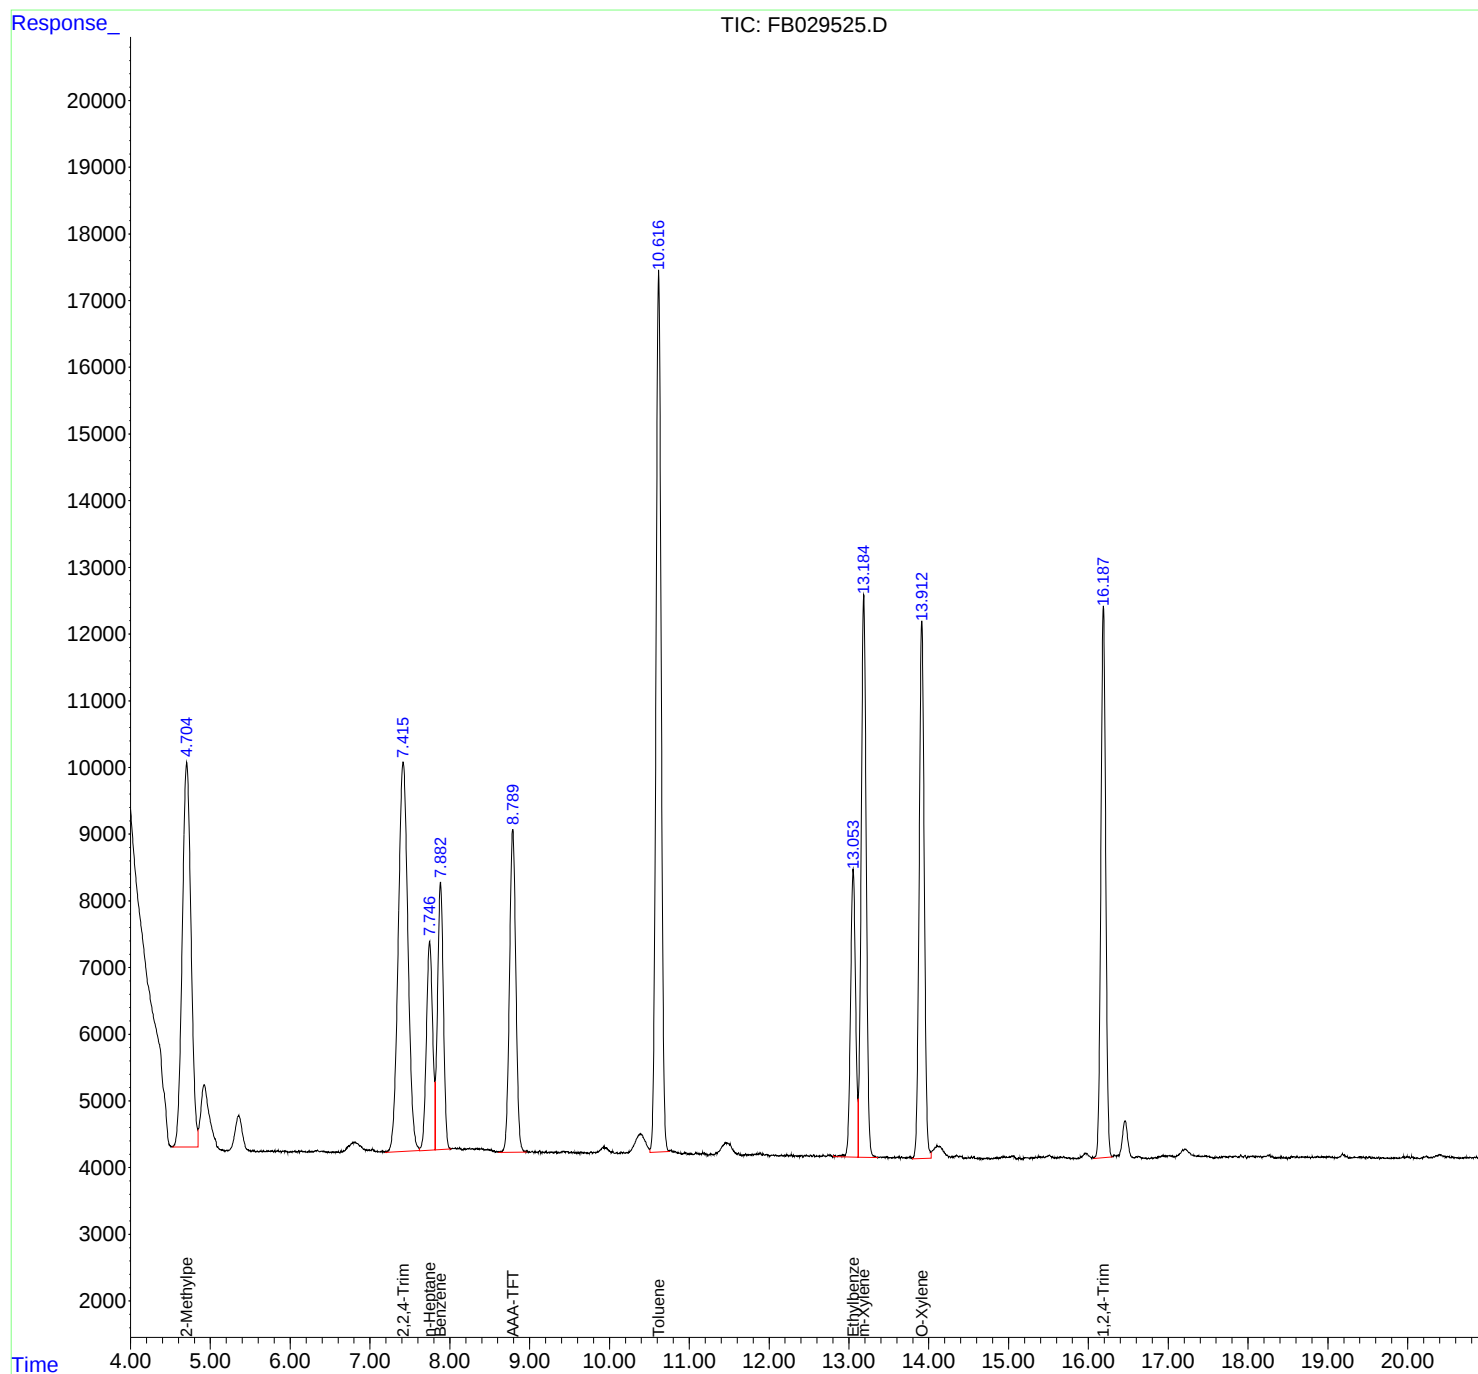

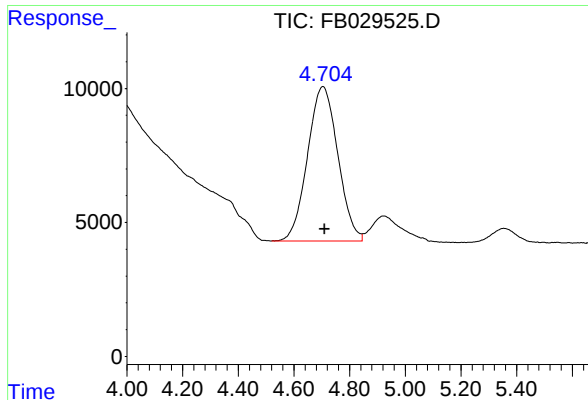


#1 2-Methylpentane

R.T.: 4.705 min
Delta R.T.: -0.005 min
Response: 436637
Conc: 28.46 ng/ml

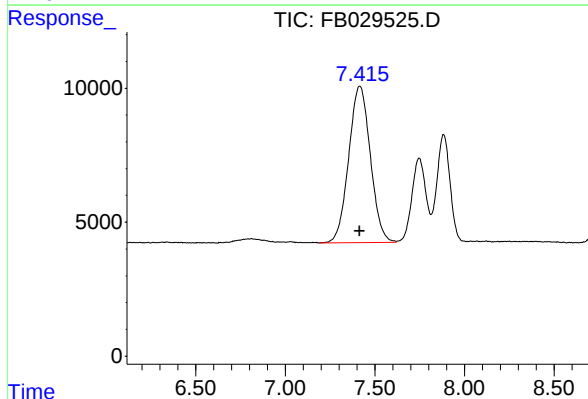


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 489733
Conc: 29.07 ng/ml

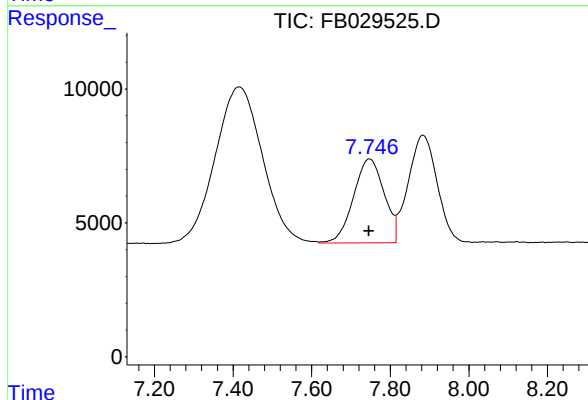


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.002 min
Response: 169325
Conc: 9.79 ng/ml

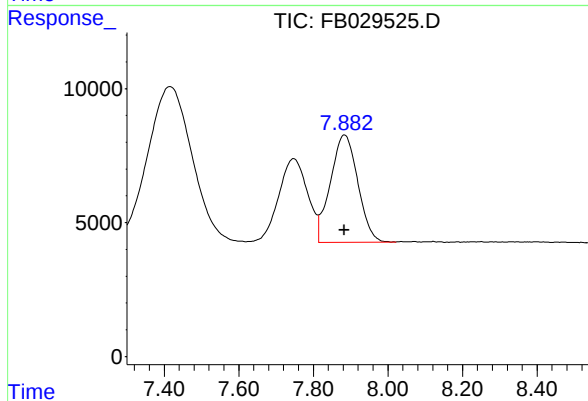


#4 Benzene

R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 204249
Conc: 10.06 ng/ml

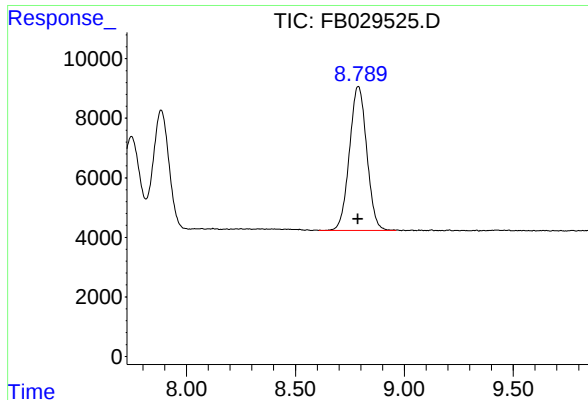


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.002 min
Response: 267834
Conc: 22.11 ng/ml

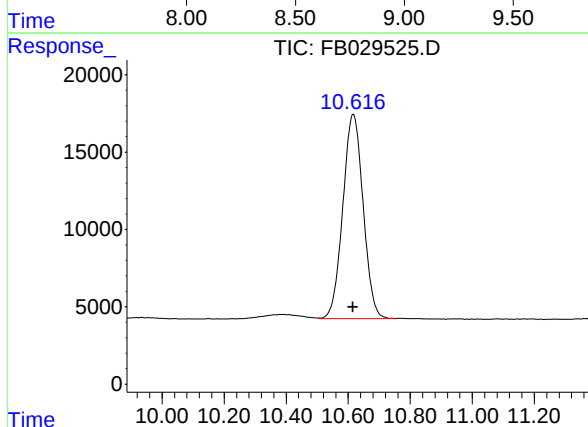


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.001 min
Response: 601145
Conc: 30.45 ng/ml

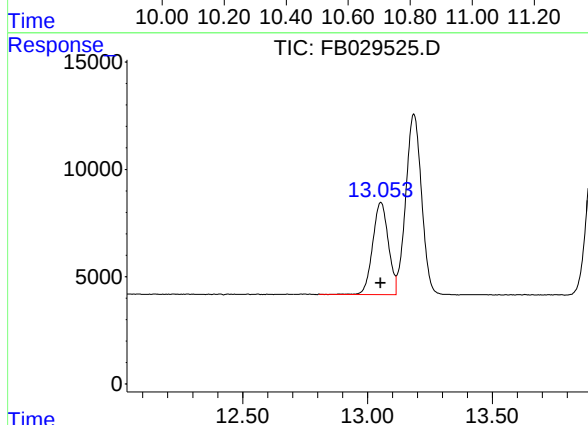


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 188237
Conc: 10.11 ng/ml

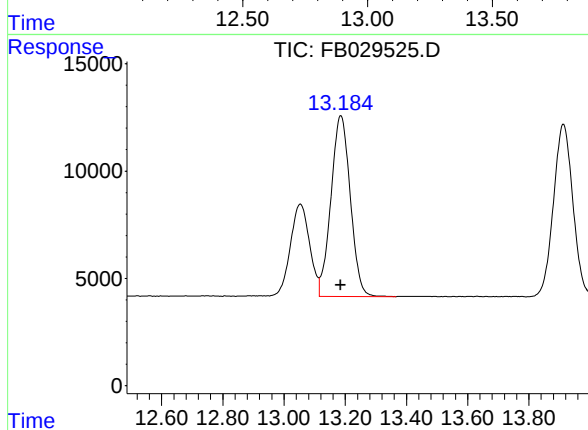


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.001 min
Response: 370653
Conc: 19.92 ng/ml

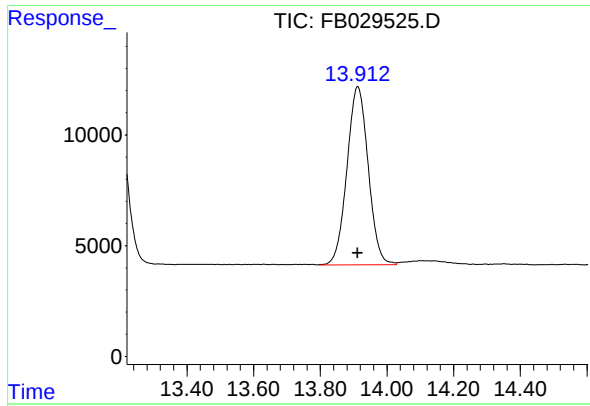

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.001 min
Response: 355730
Conc: 19.32 ng/ml

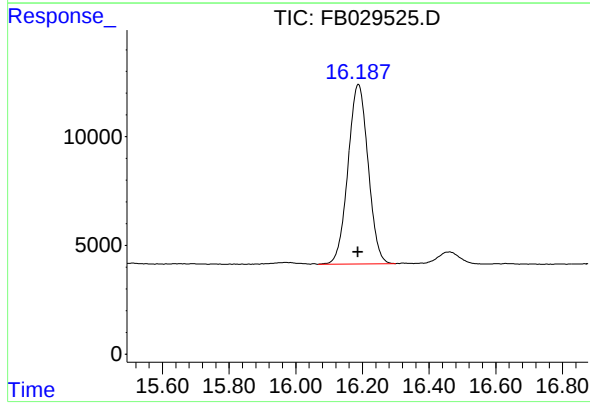

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.001 min
Response: 345404
Conc: 18.54 ng/ml