

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032119\
 Data File : FB020336.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2019 10:46
 Operator : MJ/SJ
 Sample : K1690-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 22 02:03:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	487463	18.568 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.900	907415	26.900 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	783926	23.905 ng/ml
3) t n-Heptane	7.995	336257	8.080 ng/ml
4) t Benzene	8.133	450952	9.686 ng/ml
6) t Toluene	10.887	1015697	27.486 ng/ml
7) t Ethylbenzene	13.340	208076	8.844 ng/ml
8) t m-Xylene	13.473	385968	18.094 ng/ml
9) t O-Xylene	14.205	371397	19.606 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	360674	18.187 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032119\
Data File : FB020336.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2019 10:46
Operator : MJ/SJ
Sample : K1690-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 22 02:03:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

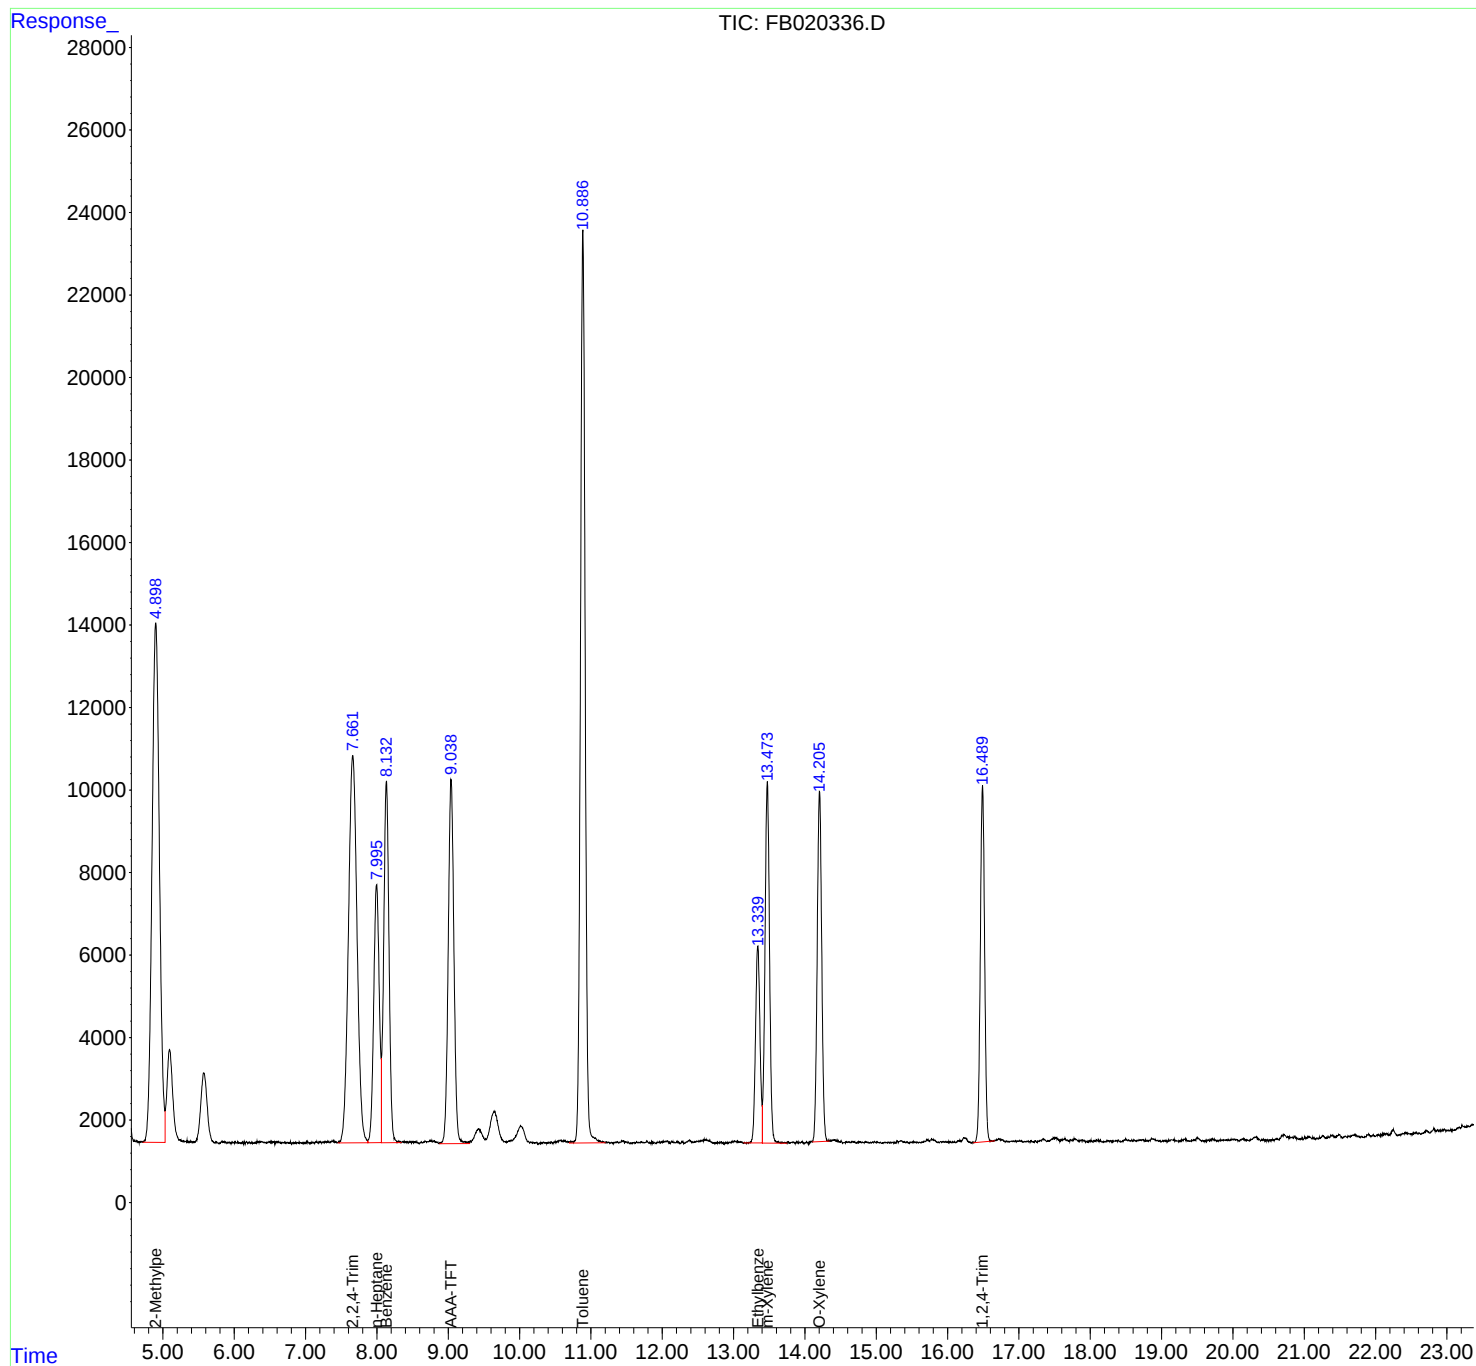

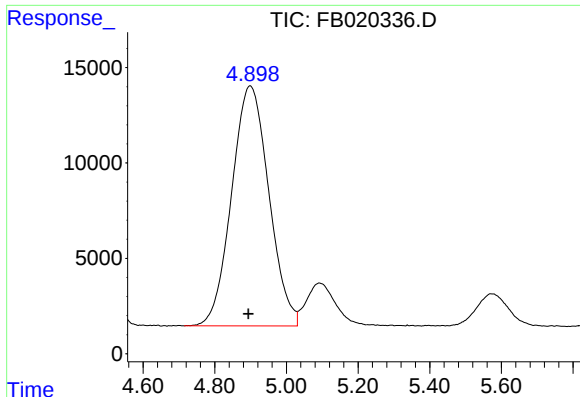


#1 2-Methylpentane

R.T.: 4.900 min
Delta R.T.: 0.006 min
Response: 907415
Conc: 26.90 ng/ml

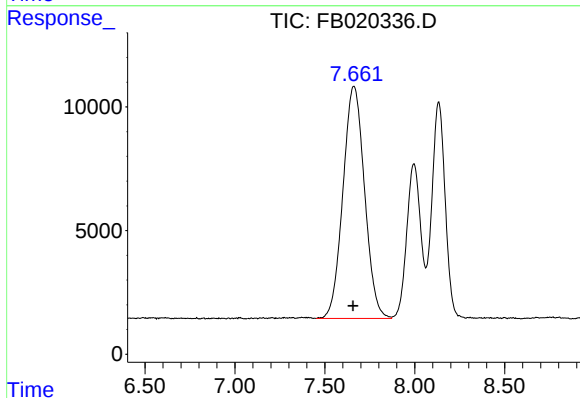


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: 0.004 min
Response: 783926
Conc: 23.90 ng/ml

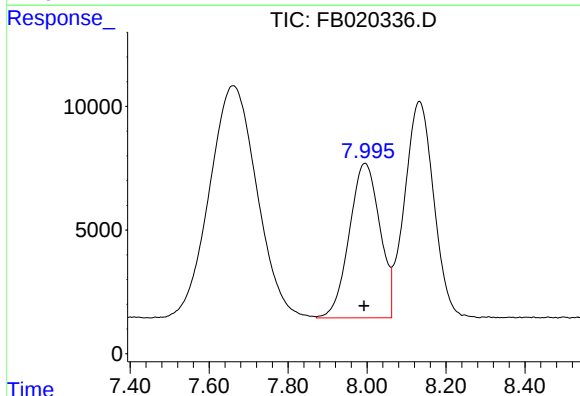


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.003 min
Response: 336257
Conc: 8.08 ng/ml

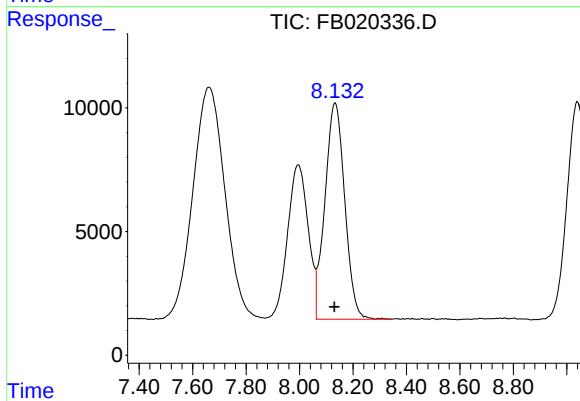


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.003 min
Response: 450952
Conc: 9.69 ng/ml

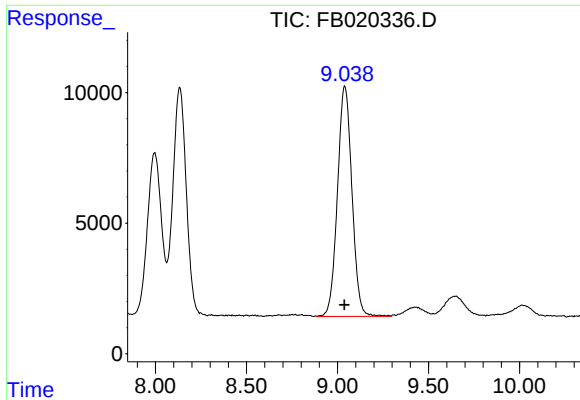


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.002 min
Response: 487463
Conc: 18.57 ng/ml

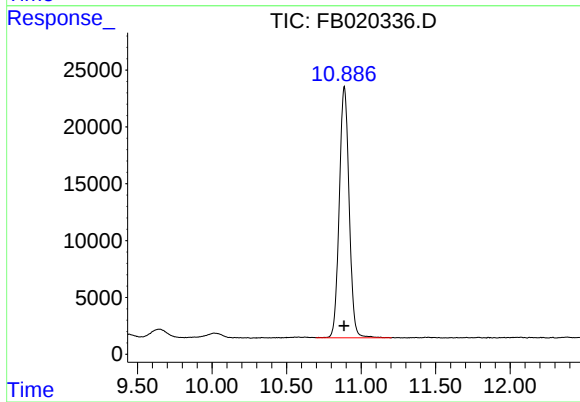


#6 Toluene

R.T.: 10.887 min
Delta R.T.: 0.002 min
Response: 1015697
Conc: 27.49 ng/ml

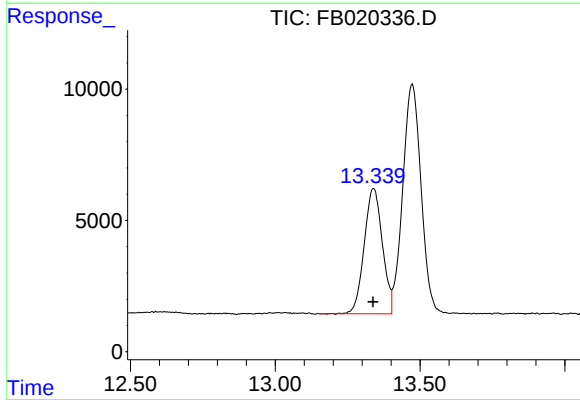


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: 0.002 min
Response: 208076
Conc: 8.84 ng/ml

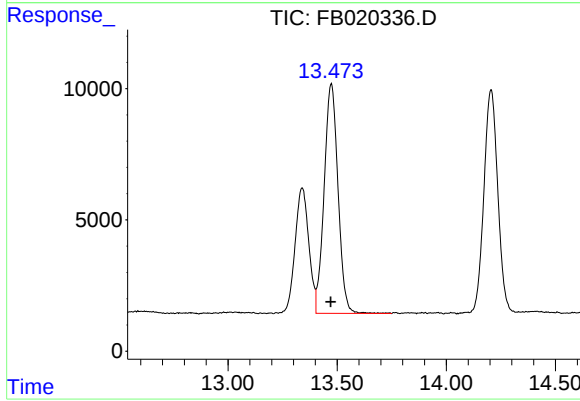


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: 0.002 min
Response: 385968
Conc: 18.09 ng/ml

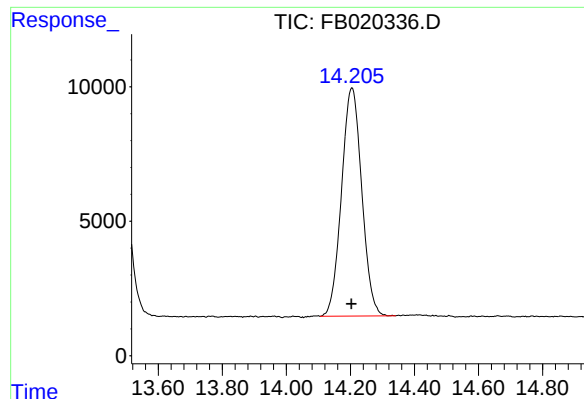

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.002 min
Response: 371397
Conc: 19.61 ng/ml

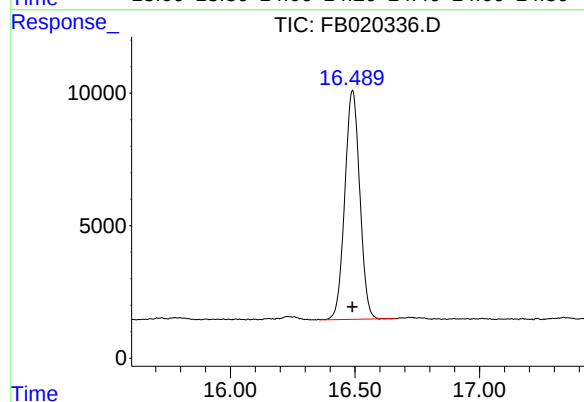

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.002 min
Response: 360674
Conc: 18.19 ng/ml