

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032119\
 Data File : FB020333.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2019 9:17
 Operator : MJ/SJ
 Sample : BSF0321S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 22 02:02:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	549283	20.923 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	1082867	32.101 ng/ml
2) t 2,2,4-Trimethylpentane	7.660	1026483	31.301 ng/ml
3) t n-Heptane	7.994	438109	10.527 ng/ml
4) t Benzene	8.132	473866	10.178 ng/ml
6) t Toluene	10.886	1075305	29.099 ng/ml
7) t Ethylbenzene	13.338	233778	9.936 ng/ml
8) t m-Xylene	13.472	452154	21.196 ng/ml
9) t O-Xylene	14.203	430588	22.731 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	448231	22.601 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032119\
Data File : FB020333.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2019 9:17
Operator : MJ/SJ
Sample : BSF0321S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 22 02:02:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

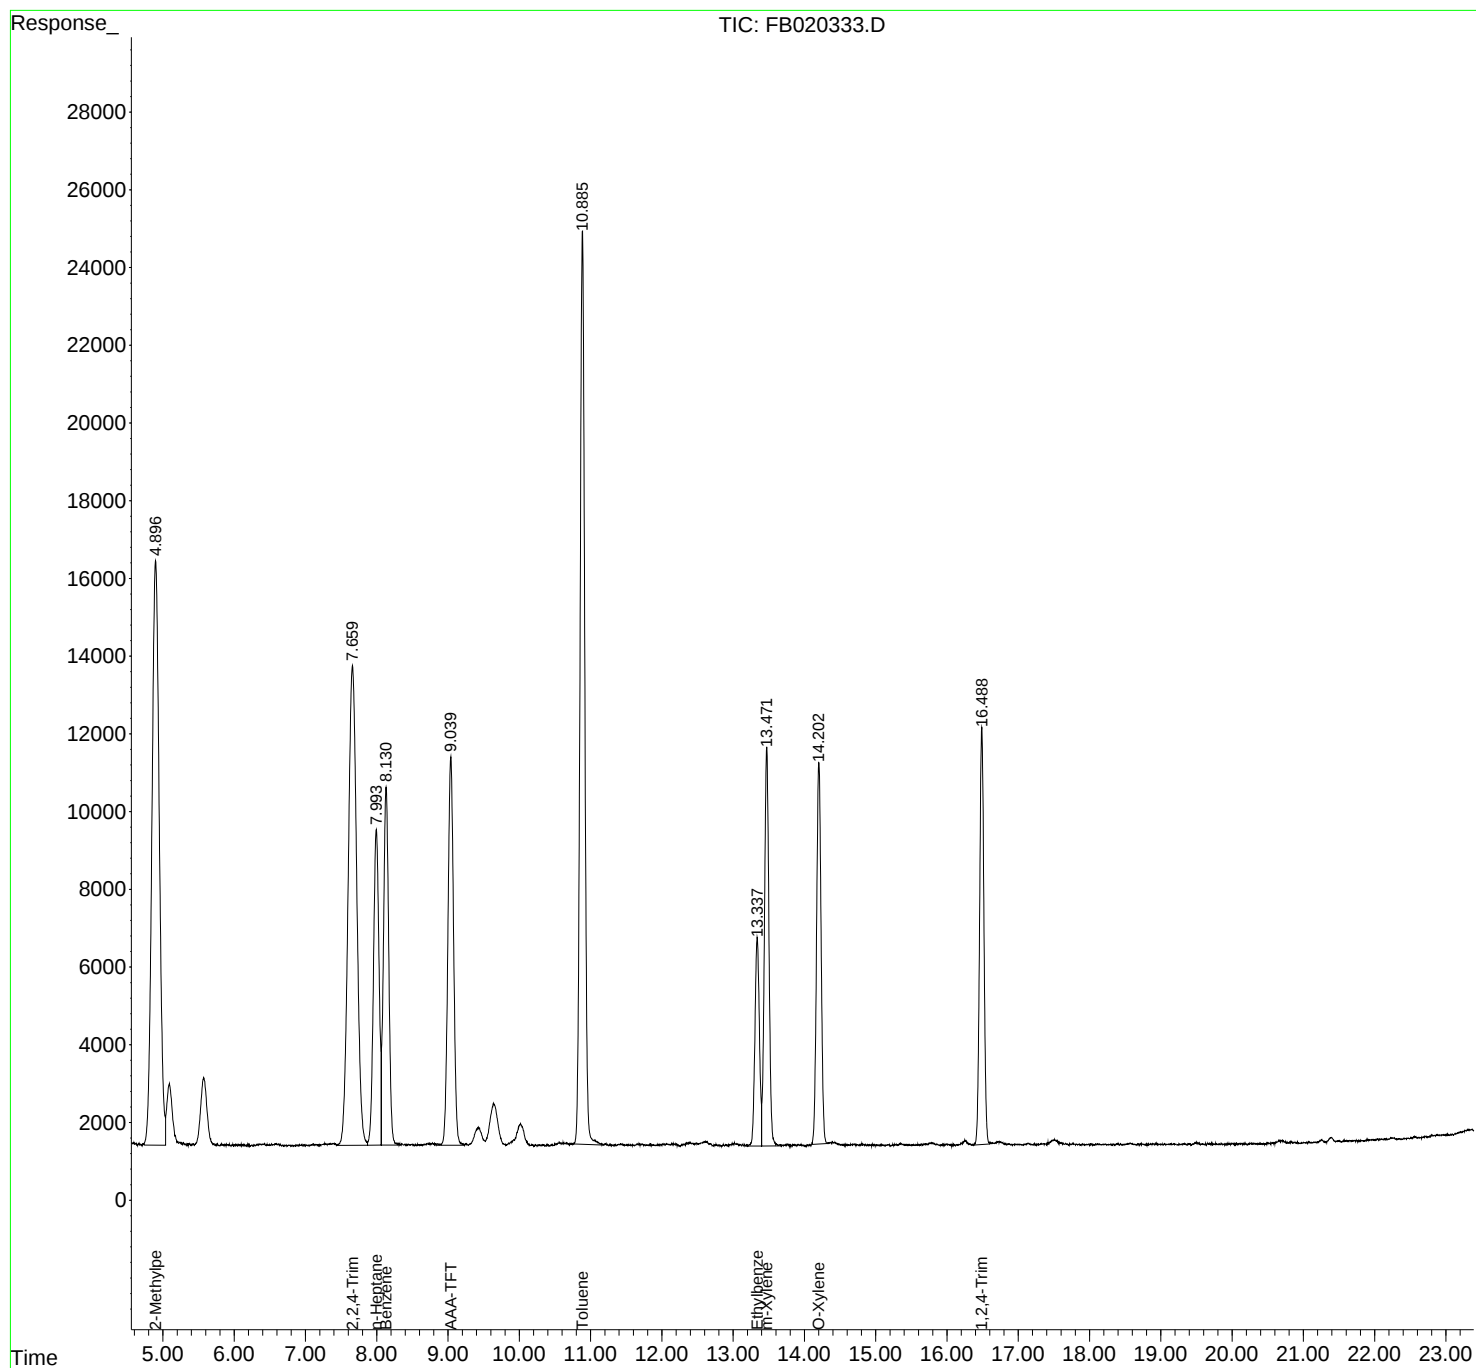

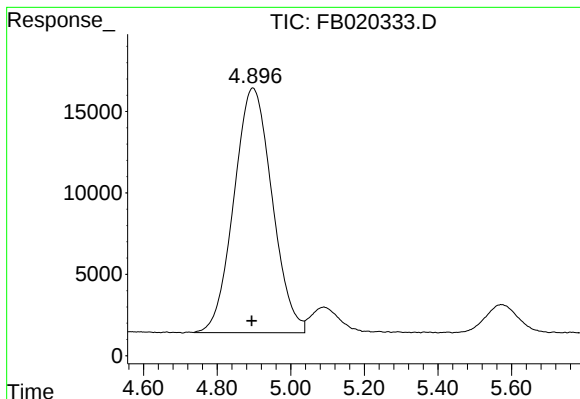


#1 2-Methylpentane

R.T.: 4.898 min
Delta R.T.: 0.004 min
Response: 1082867
Conc: 32.10 ng/ml

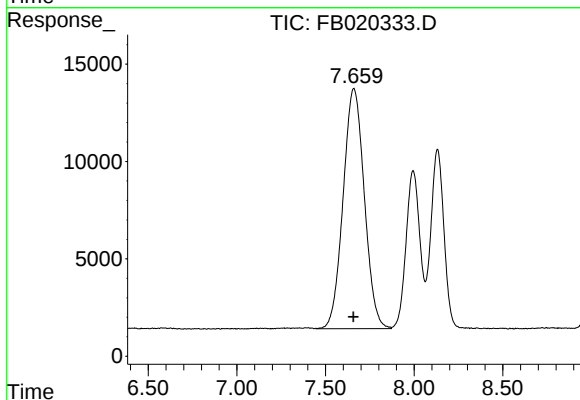


#2 2,2,4-Trimethylpentane

R.T.: 7.660 min
Delta R.T.: 0.002 min
Response: 1026483
Conc: 31.30 ng/ml

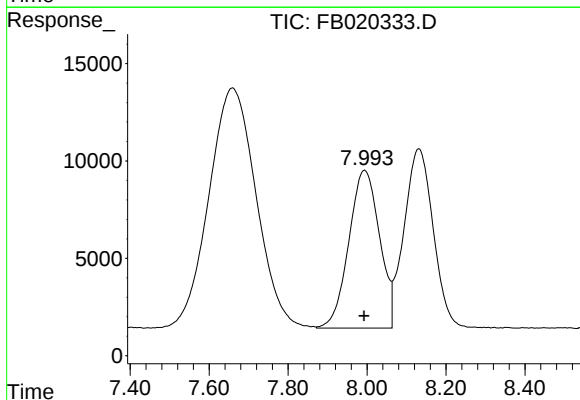


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: 0.002 min
Response: 438109
Conc: 10.53 ng/ml

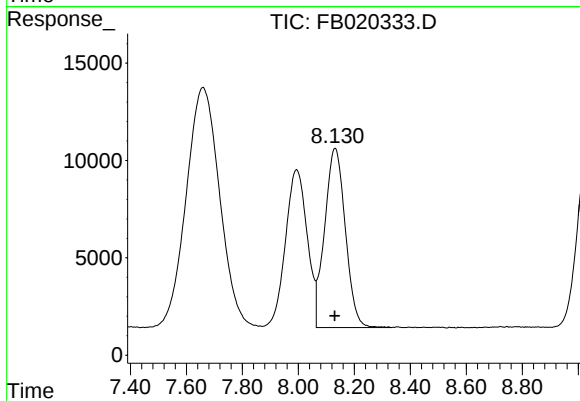


#4 Benzene

R.T.: 8.132 min
Delta R.T.: 0.002 min
Response: 473866
Conc: 10.18 ng/ml

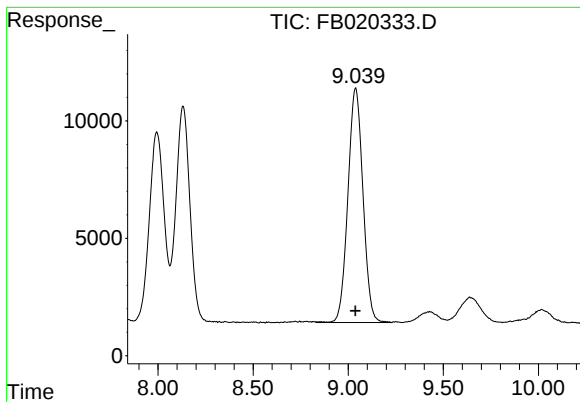


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.001 min
Response: 549283
Conc: 20.92 ng/ml

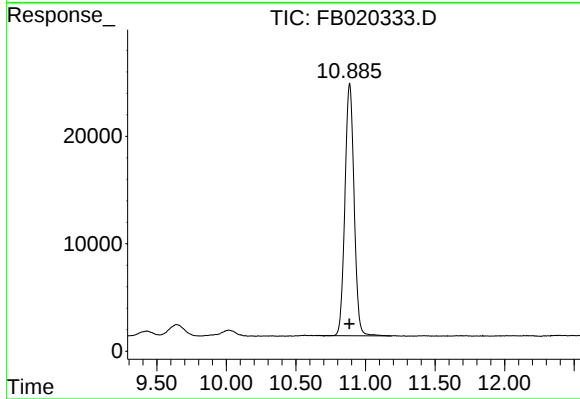


#6 Toluene

R.T.: 10.886 min
Delta R.T.: 0.000 min
Response: 1075305
Conc: 29.10 ng/ml

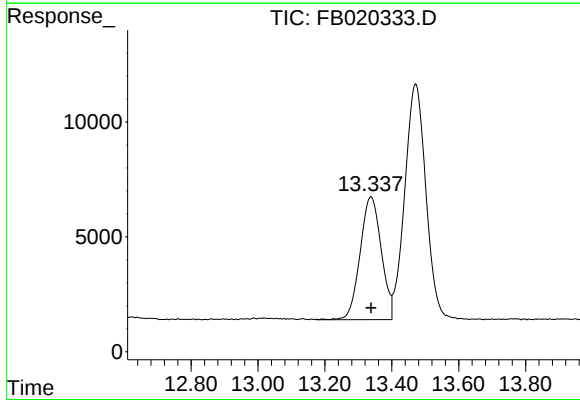


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.000 min
Response: 233778
Conc: 9.94 ng/ml

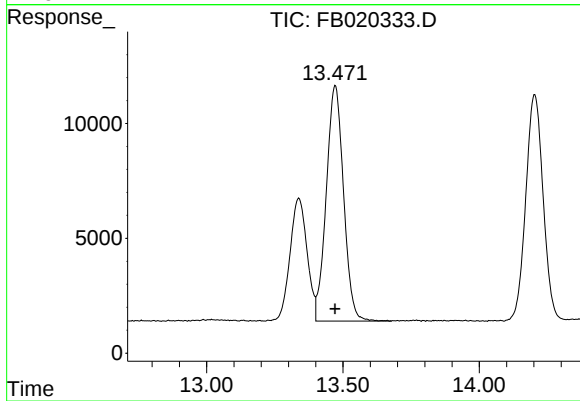


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: 0.000 min
Response: 452154
Conc: 21.20 ng/ml

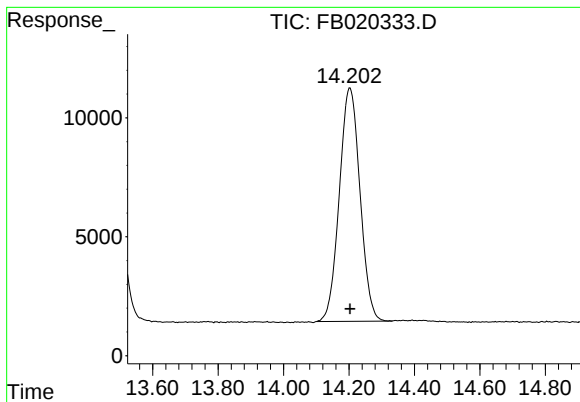

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.000 min
Response: 430588
Conc: 22.73 ng/ml

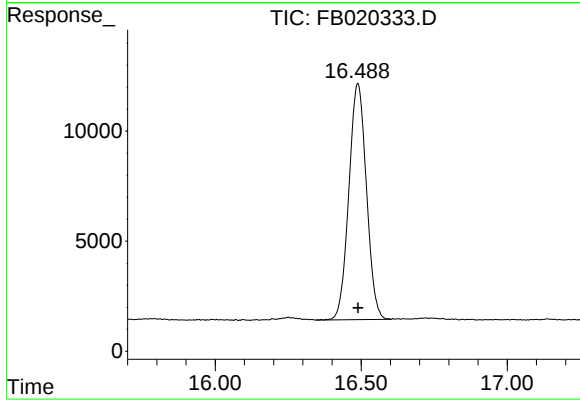

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.000 min
Response: 448231
Conc: 22.60 ng/ml