

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032122\
 Data File : FB026749.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2022 14:08
 Operator : AJ/MA
 Sample : BSF0317S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 22 02:27:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	273843	26.097 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	553587	29.238 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	606646	29.268 ng/ml
3) t n-Heptane	7.748	199320	10.070 ng/ml
4) t Benzene	7.884	230156	9.974 ng/ml
6) t Toluene	10.618	655750	29.953 ng/ml
7) t Ethylbenzene	13.055	198587	9.881 ng/ml
8) t m-Xylene	13.188	395932	19.647 ng/ml
9) t O-Xylene	13.915	387545	19.426 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	389676	19.558 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032122\
Data File : FB026749.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2022 14:08
Operator : AJ/MA
Sample : BSF0317S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 22 02:27:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

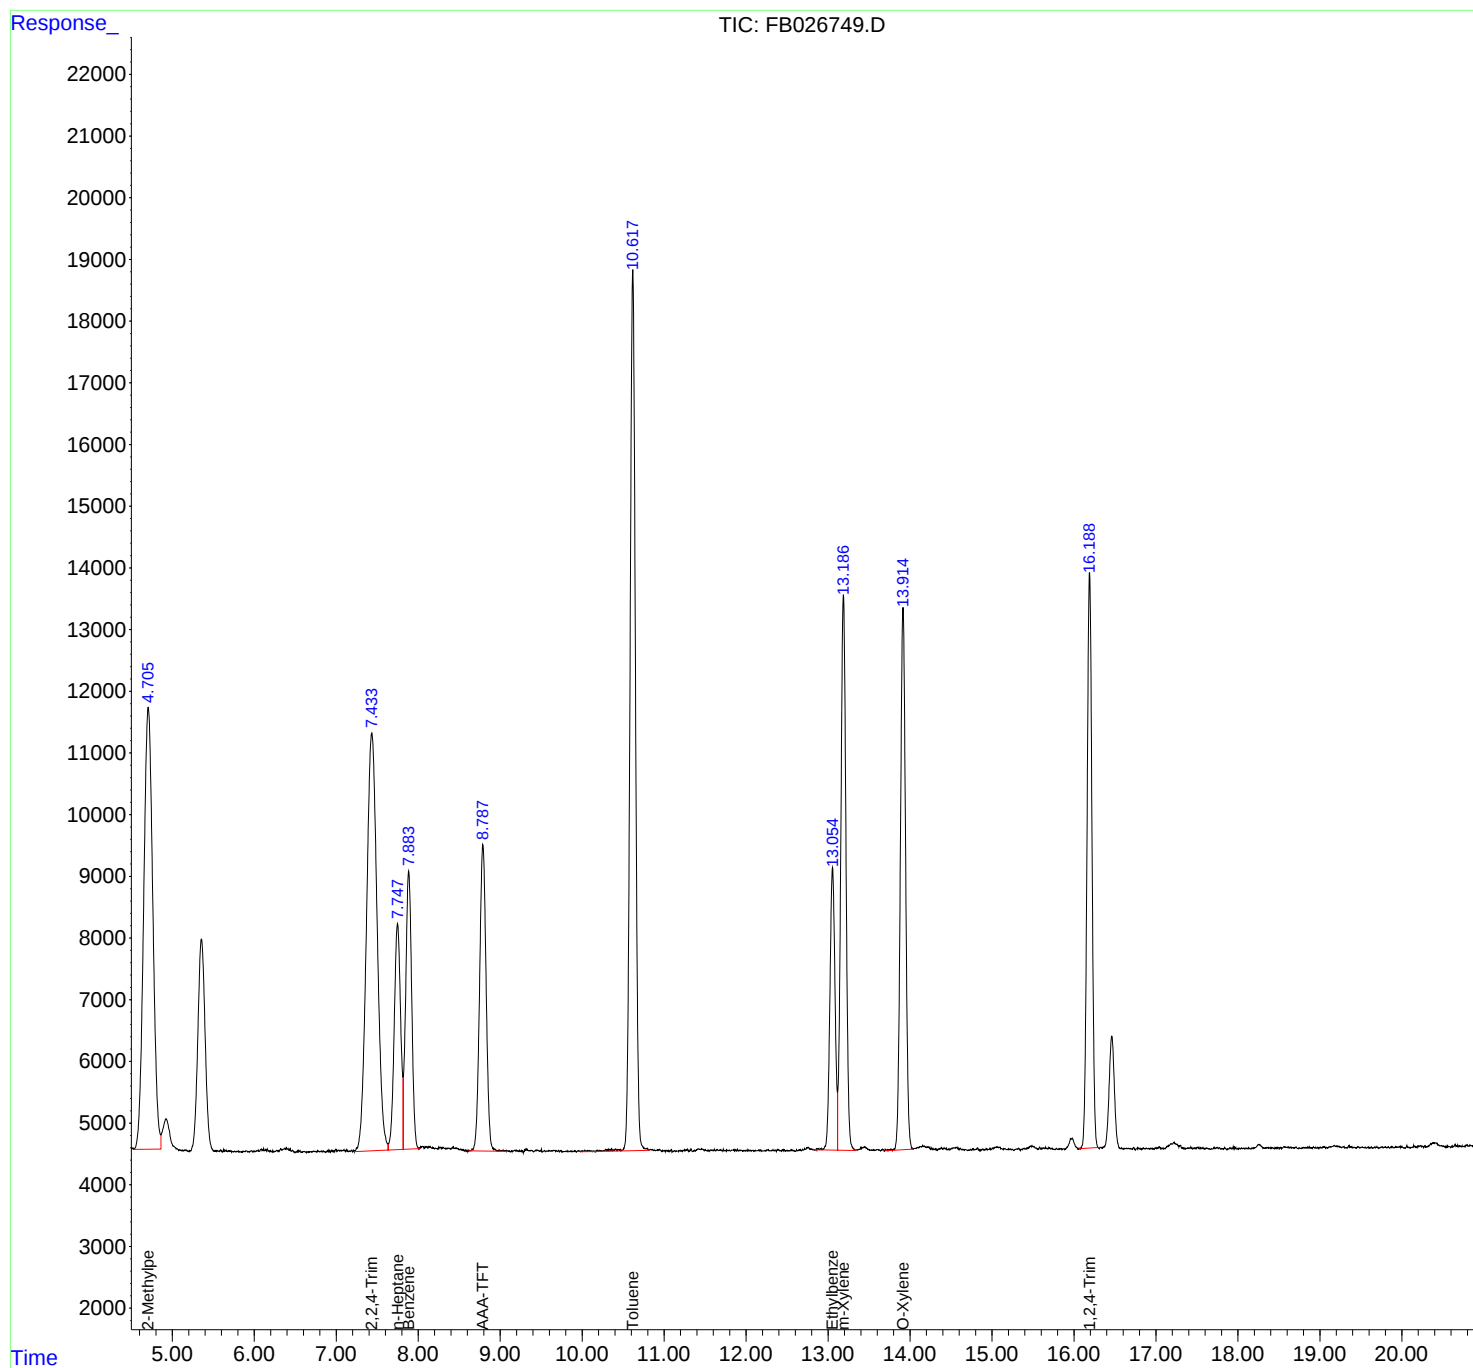

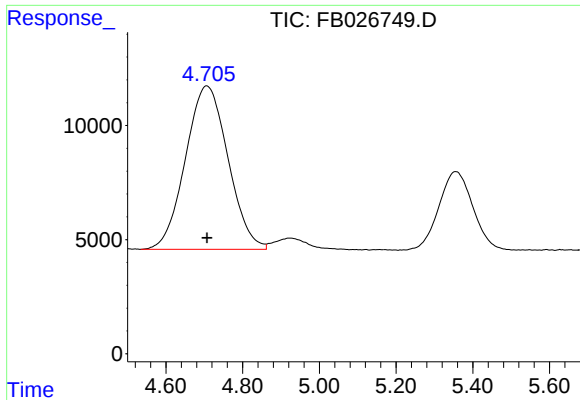


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 553587
Conc: 29.24 ng/ml

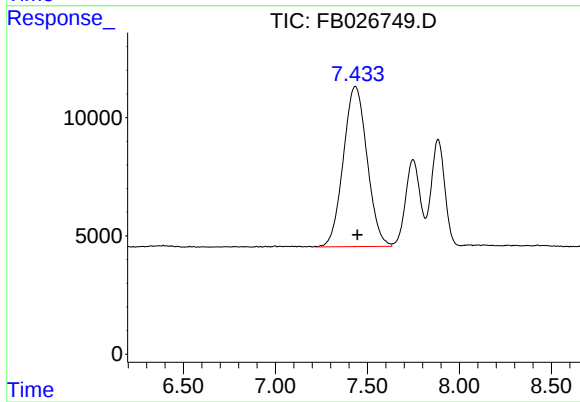


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: -0.012 min
Response: 606646
Conc: 29.27 ng/ml

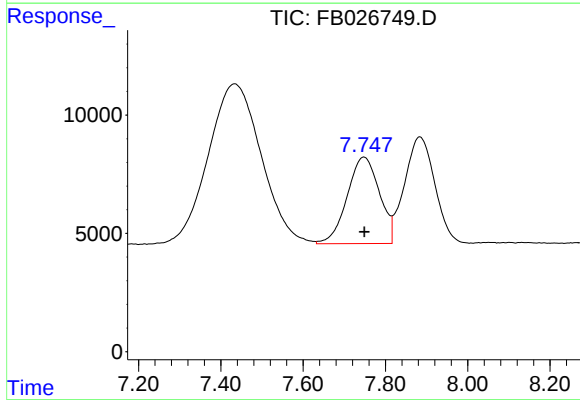


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 199320
Conc: 10.07 ng/ml

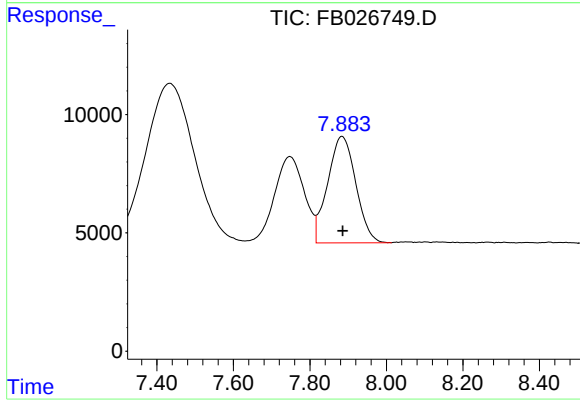


#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 230156
Conc: 9.97 ng/ml

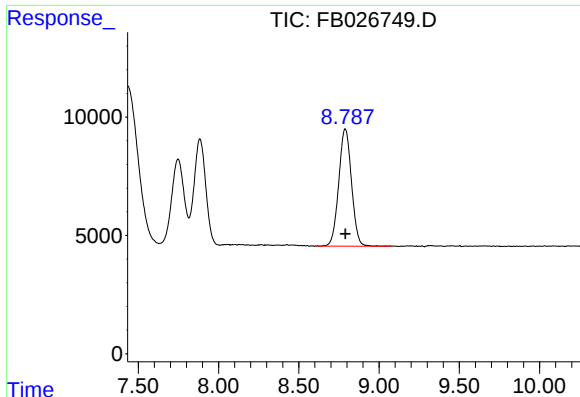


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 273843
Conc: 26.10 ng/ml

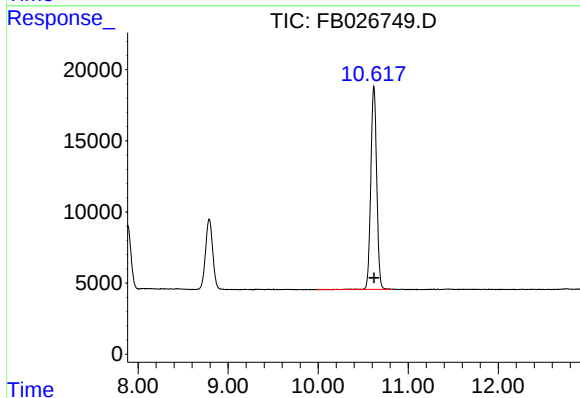


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 655750
Conc: 29.95 ng/ml

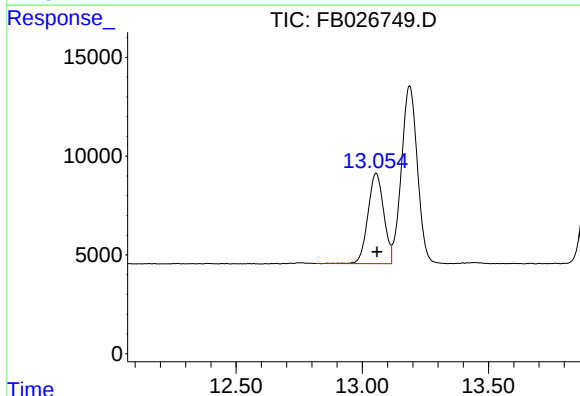


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 198587
Conc: 9.88 ng/ml

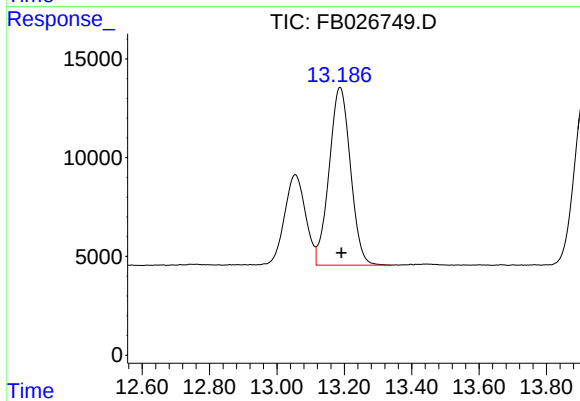


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 395932
Conc: 19.65 ng/ml

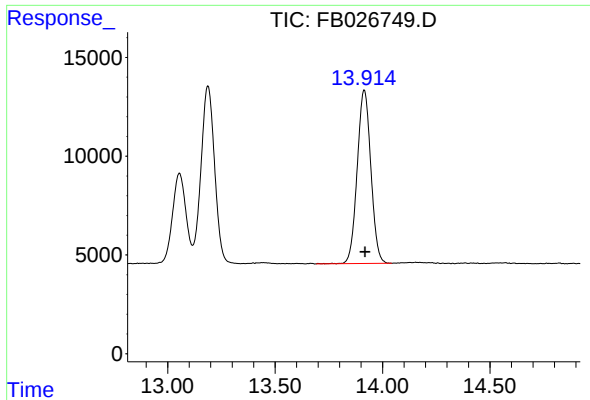

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.004 min
Response: 387545
Conc: 19.43 ng/ml

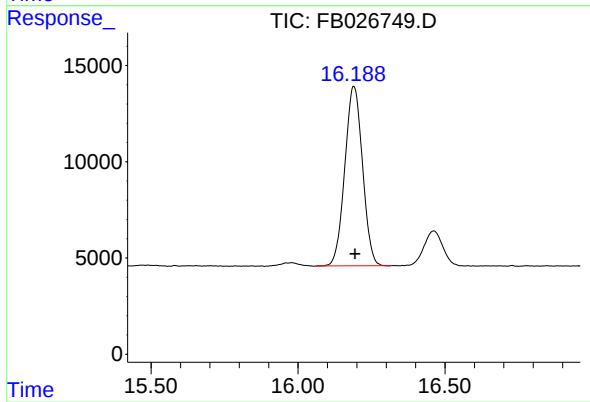

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 389676
Conc: 19.56 ng/ml