

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032122\
Data File : FB026750.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2022 14:57
Operator : AJ/MA
Sample : N1966-04
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 22 02:27:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	191849	18.283 ng/ml
Target Compounds			
4) t Benzene	7.887	13735	0.595 ng/ml
8) t m-Xylene	13.186	5942	0.295 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032122\
Data File : FB026750.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2022 14:57
Operator : AJ/MA
Sample : N1966-04
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 22 02:27:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

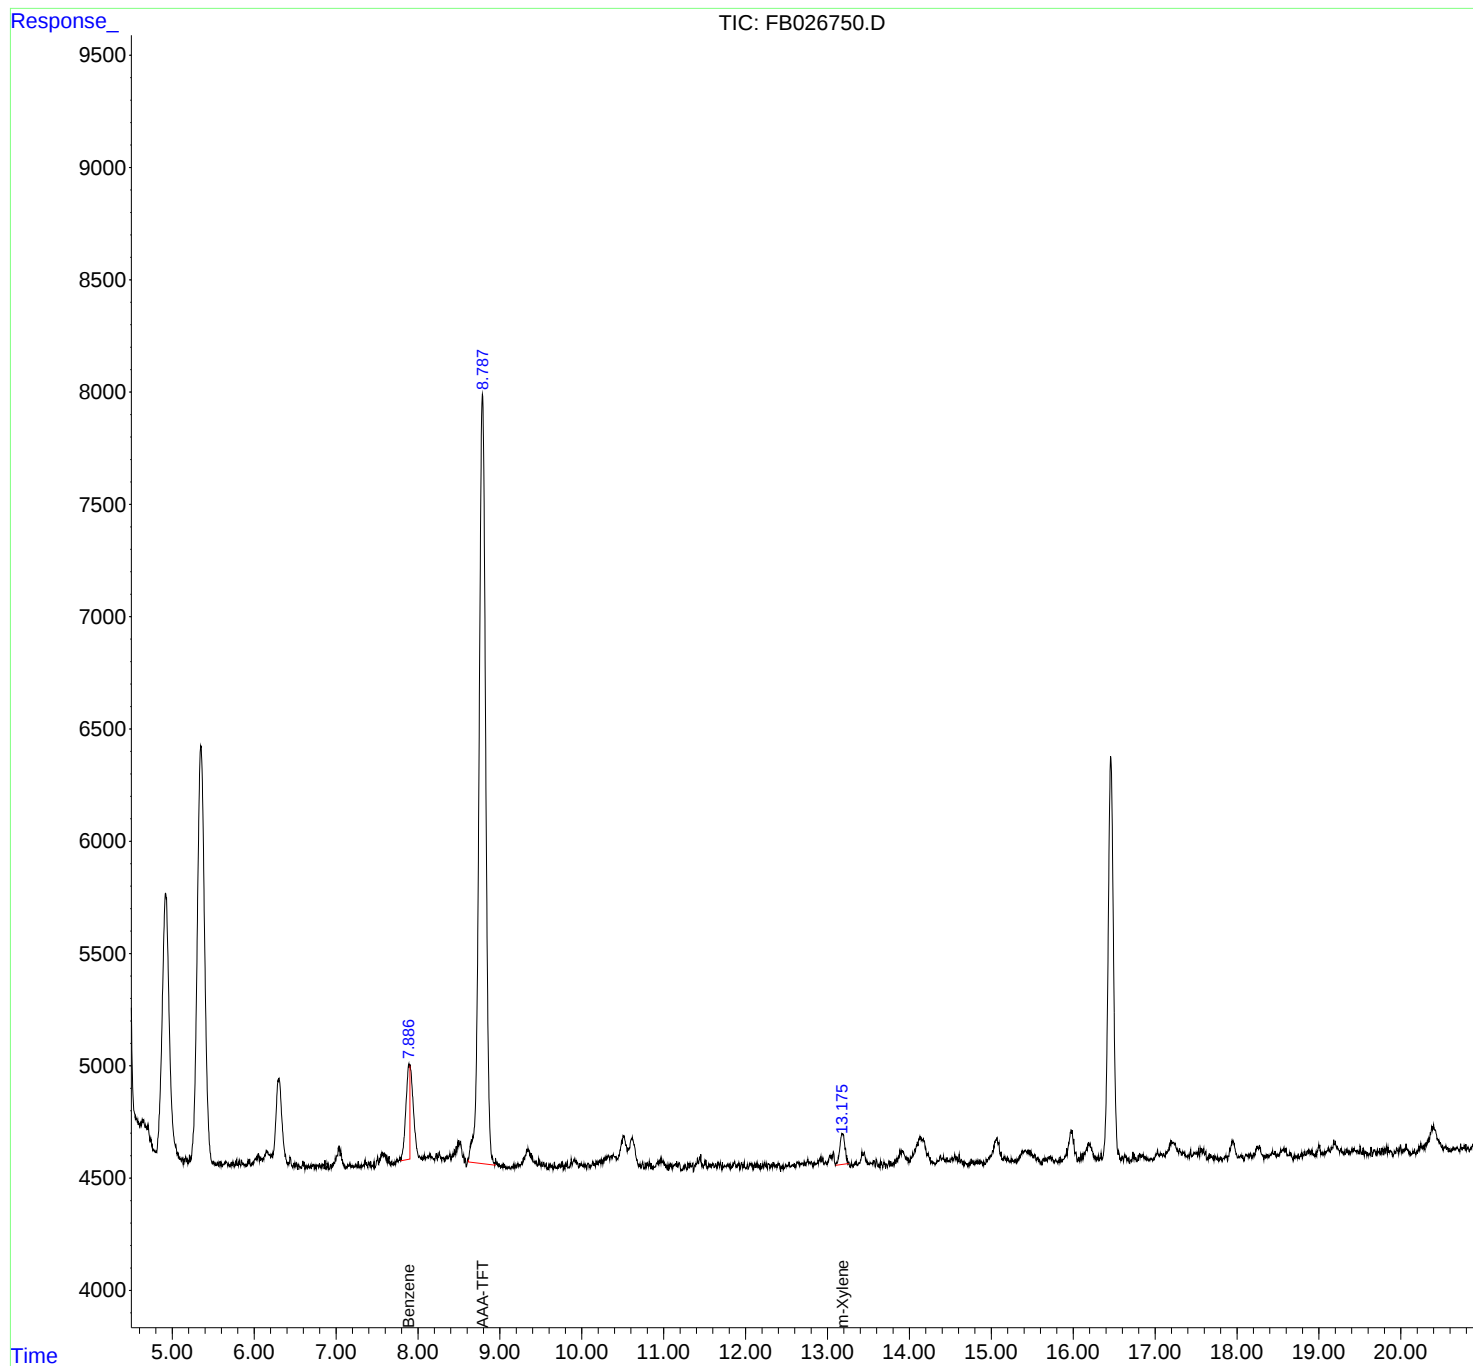

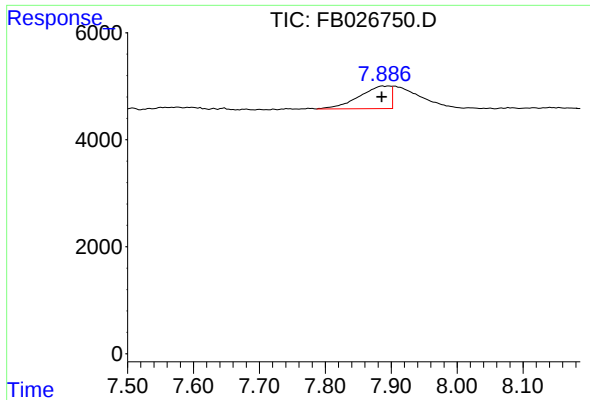


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.001 min
Response: 13735
Conc: 0.60 ng/ml

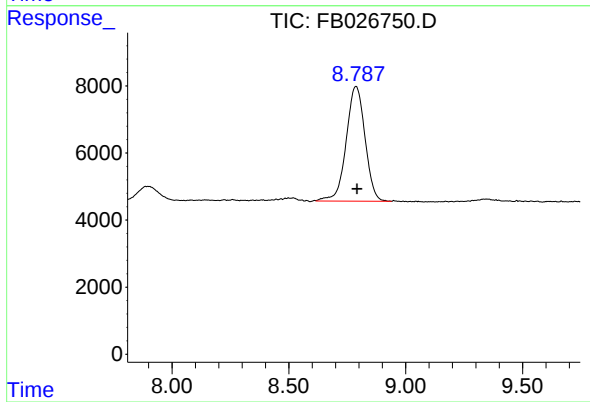

#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 191849
Conc: 18.28 ng/ml

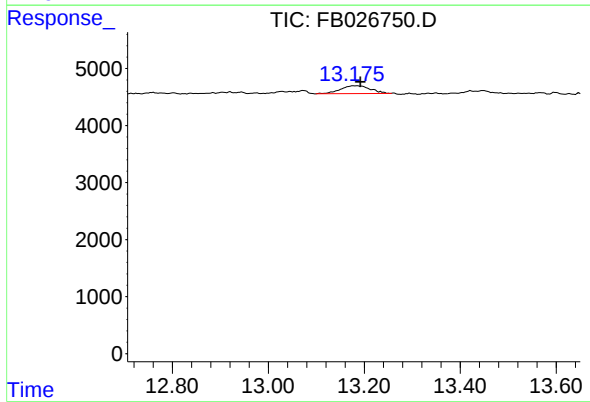

#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.006 min
Response: 5942
Conc: 0.29 ng/ml