

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
 Data File : PS018663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 01:53
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 02:48:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.810	1542.8E6	434.3E6	542.112	617.232
Target Compounds							
8) T	DICHLORPROP	0.000	7.622	0	8223917	N.D.	10.389
11) T	2,4,5-TP ...	9.274f	8.640f	50584162	8931359	3.326	2.048 #
13) T	2,4-DB	10.004f	0.000	45310	0	<MDL	N.D. #
14) T	DINOSEB	11.175f	0.000	6684530	0	<MDL	N.D. #
15) T	Picloram	11.029	10.874	26299799	5768833	1.279	1.085
16) T	DCPA	0.000	10.874f	0	5768833	N.D.	1.097


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032122\
Data File : PS018663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 01:53
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 02:48:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

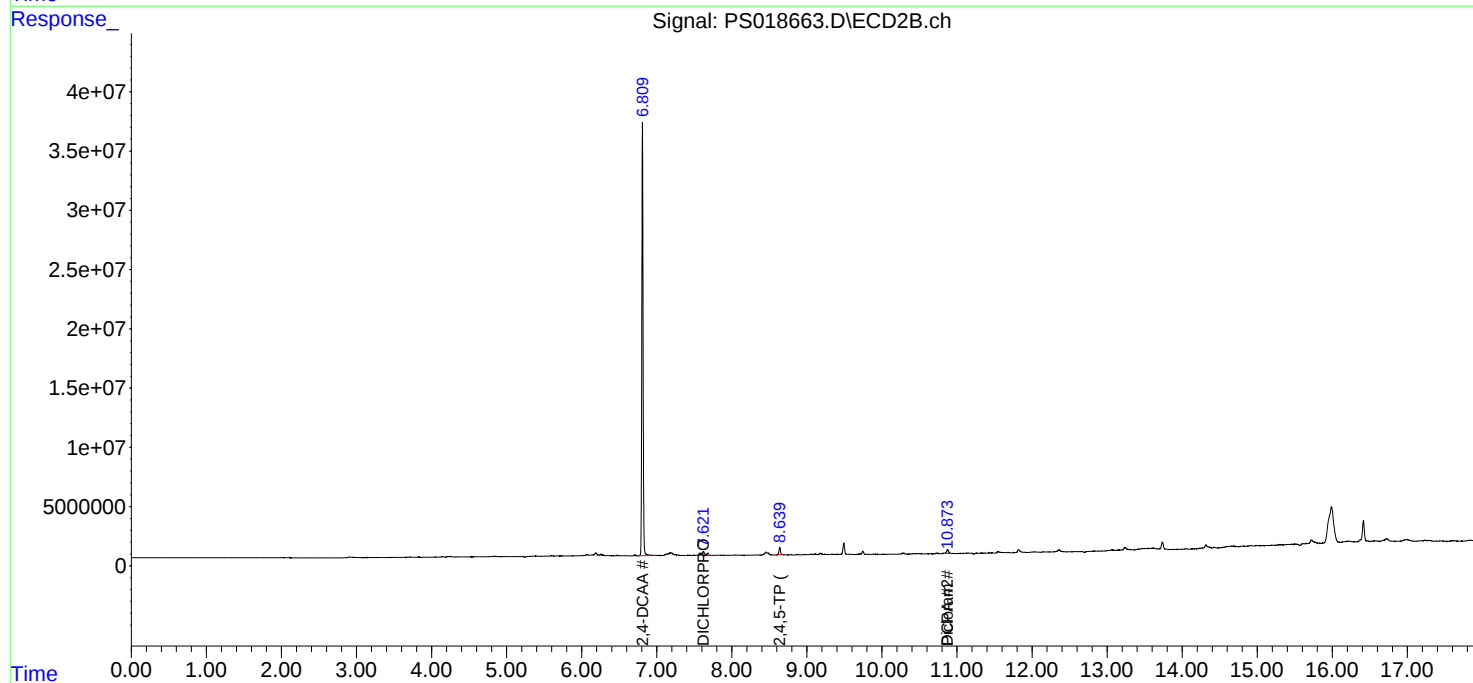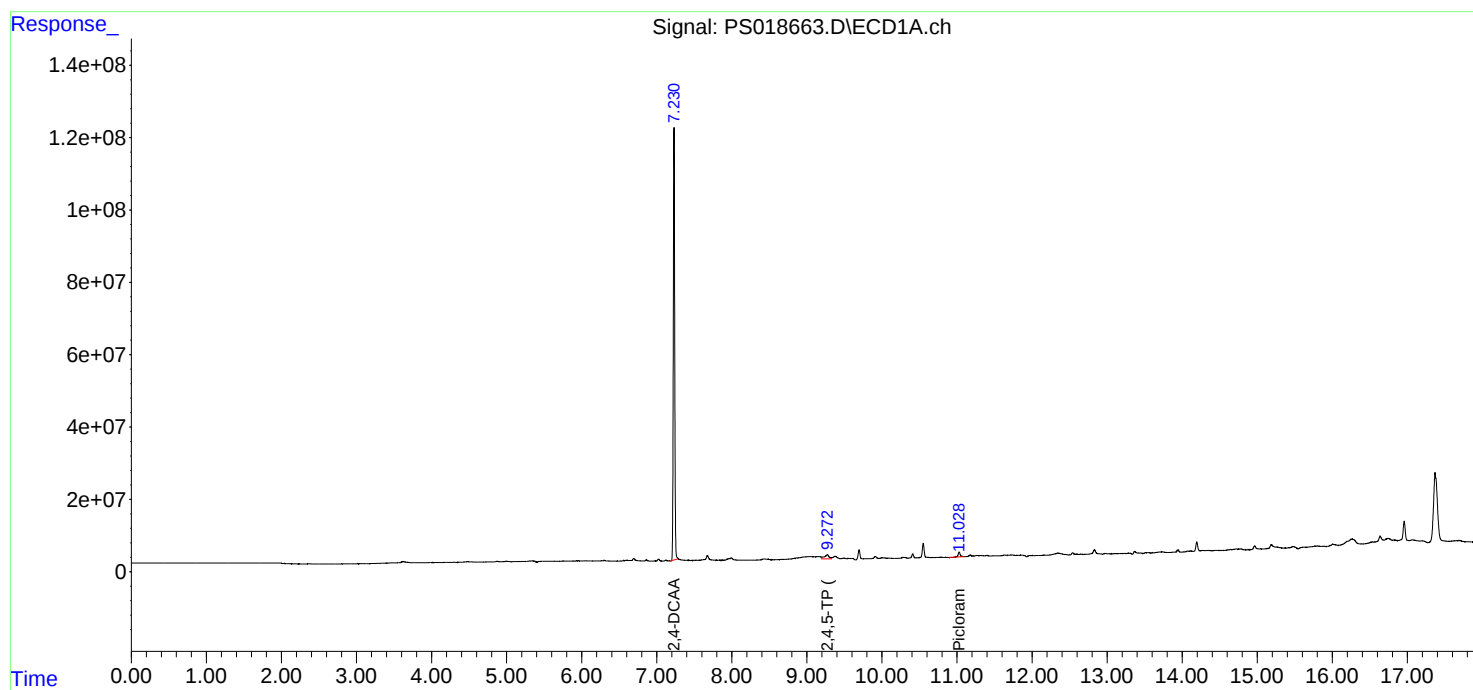

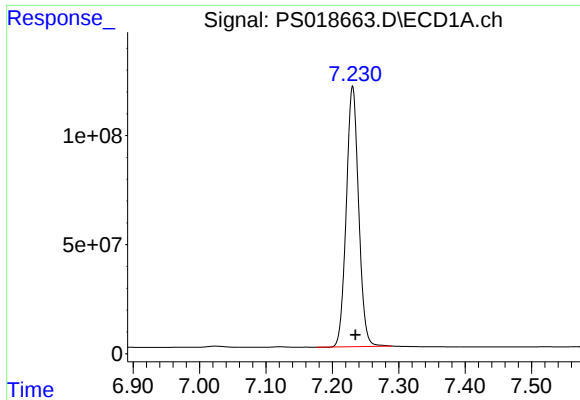


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.004 min
Response: 1542805777
Conc: 542.11 ng/ml

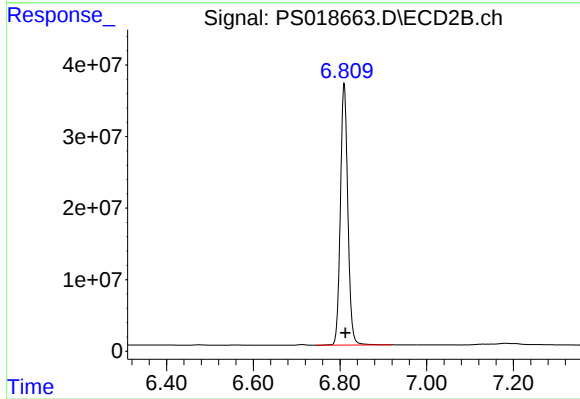


#4 2,4-DCAA

R.T.: 6.810 min
Delta R.T.: -0.003 min
Response: 434318517
Conc: 617.23 ng/ml

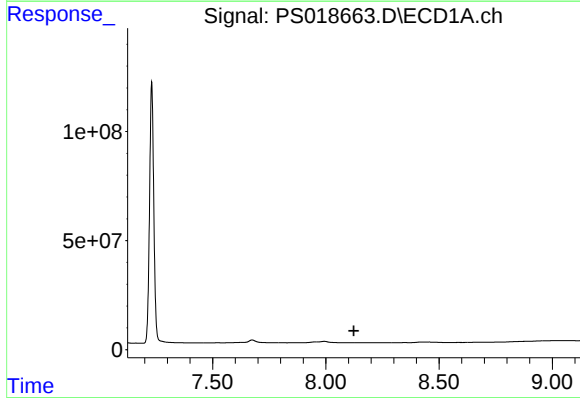


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

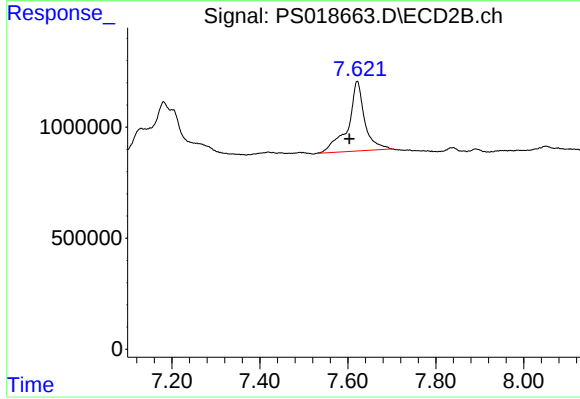


#8 DICHLORPROP

R.T.: 7.622 min
Delta R.T.: 0.018 min
Response: 8223917
Conc: 10.39 ng/ml

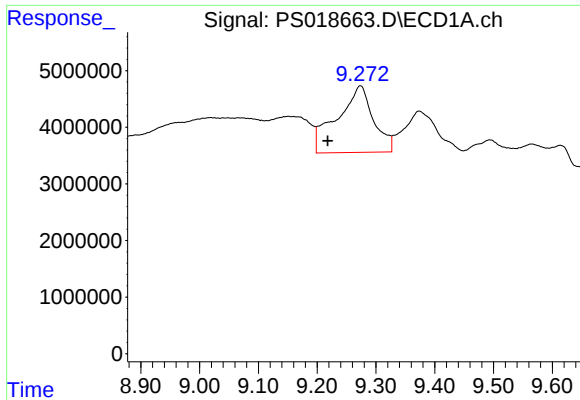


#11 2,4,5-TP (SILVEX)

R.T.: 9.274 min
Delta R.T.: 0.056 min
Response: 50584162
Conc: 3.33 ng/ml

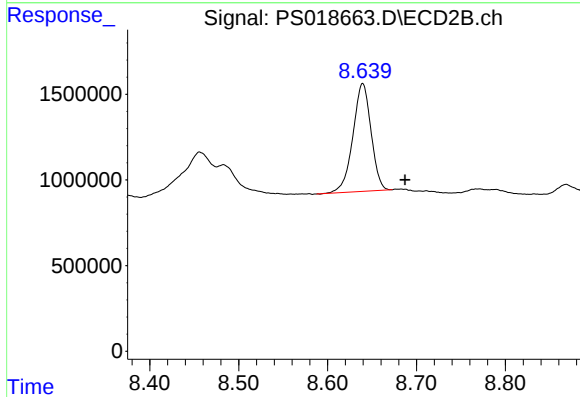


#11 2,4,5-TP (SILVEX)

R.T.: 8.640 min
Delta R.T.: -0.047 min
Response: 8931359
Conc: 2.05 ng/ml

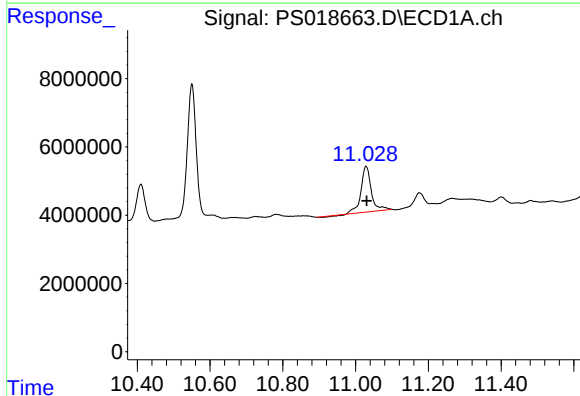


#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 26299799
Conc: 1.28 ng/ml

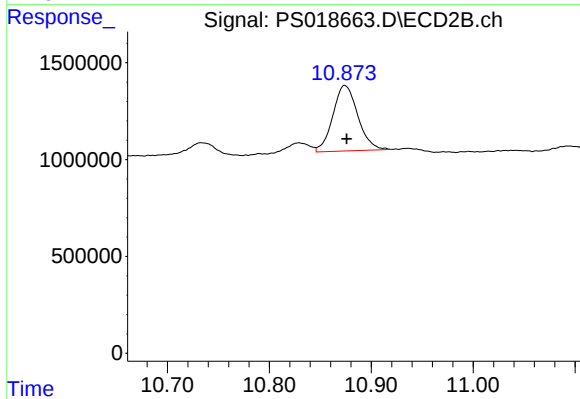


#15 Picloram

R.T.: 10.874 min
Delta R.T.: -0.002 min
Response: 5768833
Conc: 1.09 ng/ml

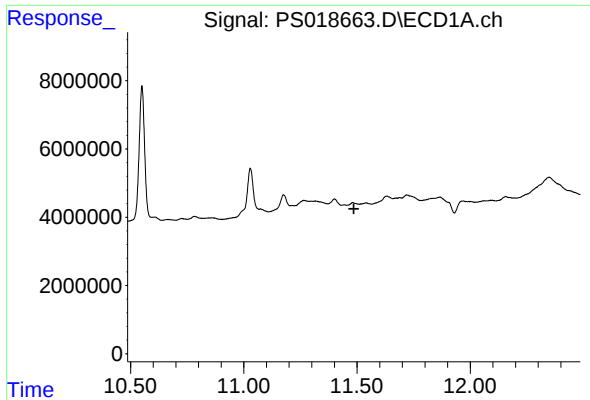

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

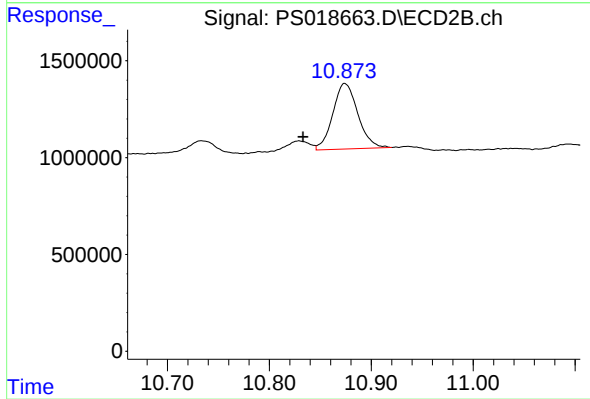

#16 DCPA

R.T.: 10.874 min
Delta R.T.: 0.041 min
Response: 5768833
Conc: 1.10 ng/ml