

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032122\
 Data File : FB026757.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2022 19:33
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Mar 22 02:28:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	138931	13.240 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	362790	19.161 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	424680	20.489 ng/ml
3) t n-Heptane	7.750	129031	6.519 ng/ml
4) t Benzene	7.886	169915	7.364 ng/ml
6) t Toluene	10.619	479901	21.921 ng/ml
7) t Ethylbenzene	13.055	148254	7.377 ng/ml
8) t m-Xylene	13.189	293025	14.540 ng/ml
9) t O-Xylene	13.915	300251	15.050 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	279071	14.006 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032122\
Data File : FB026757.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2022 19:33
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Mar 22 02:28:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

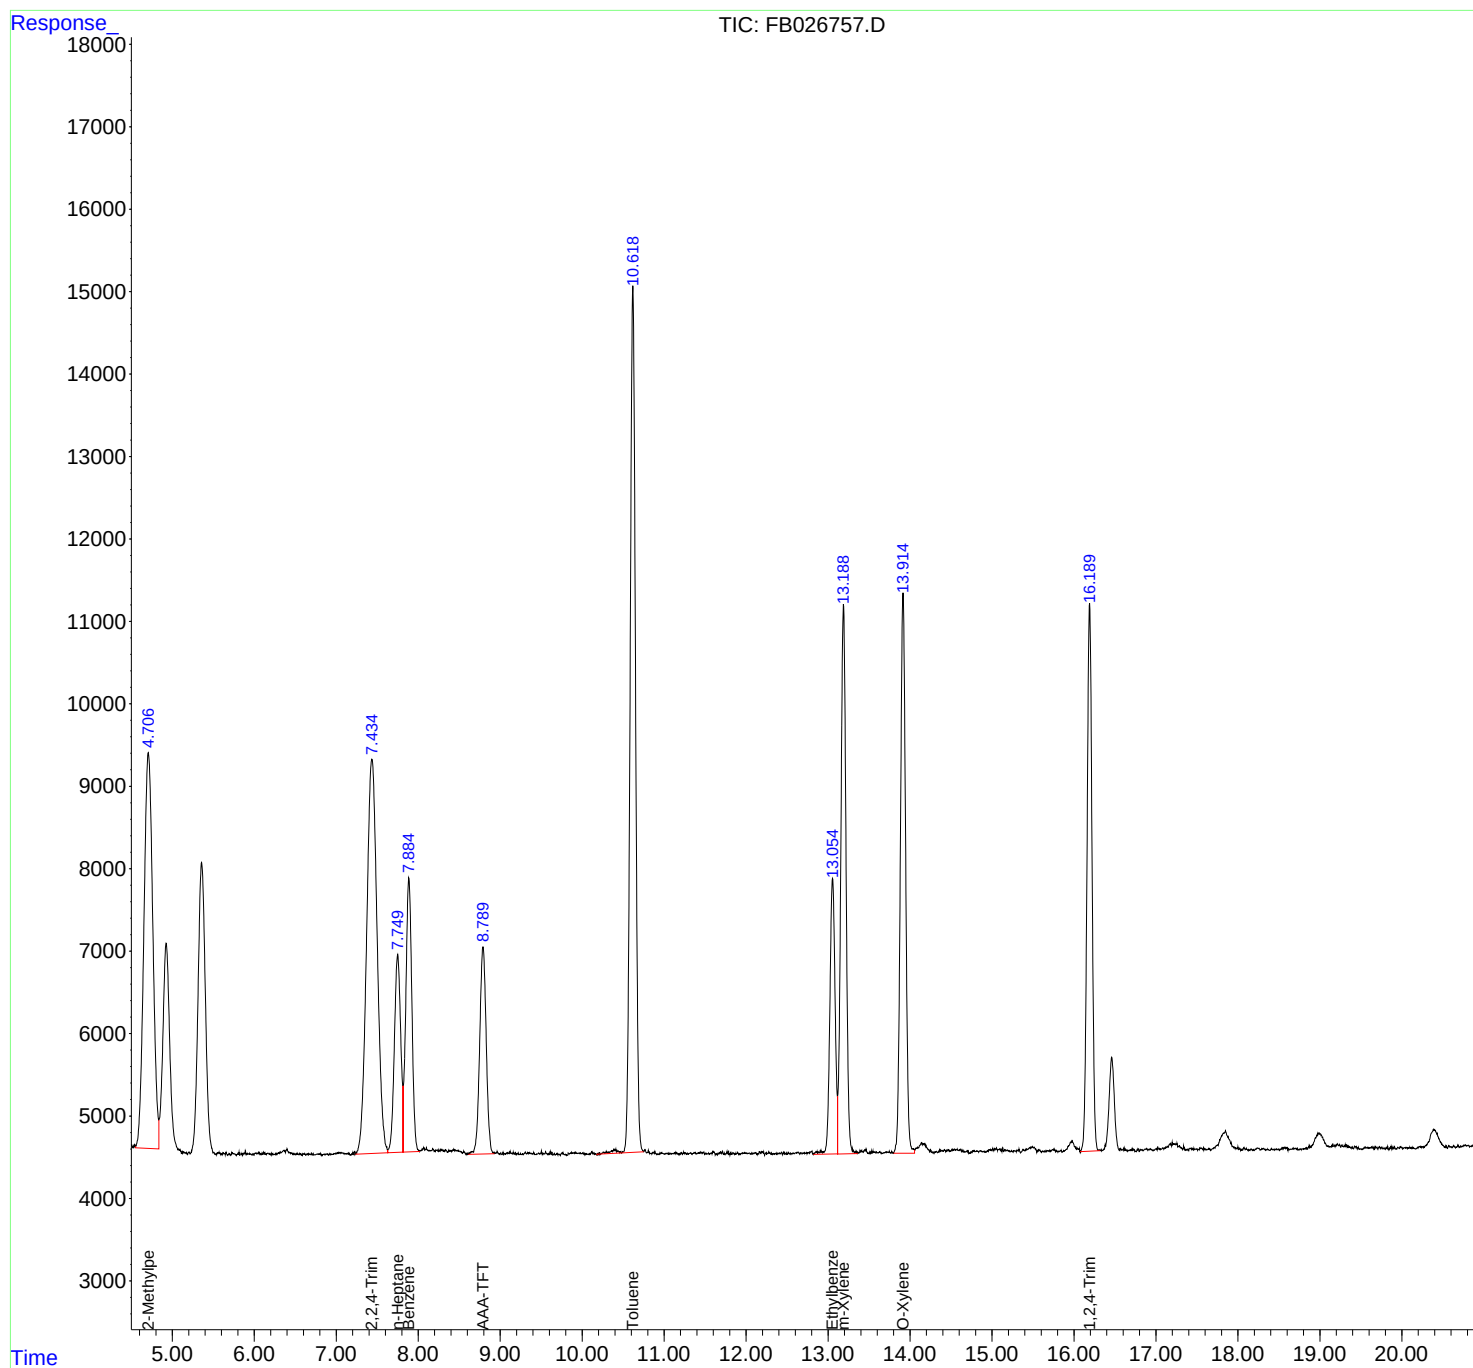

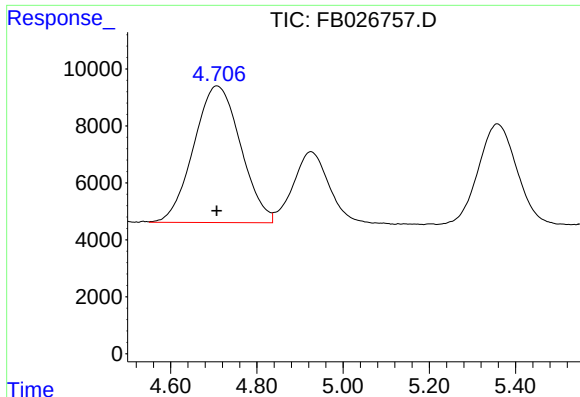


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 362790
Conc: 19.16 ng/ml

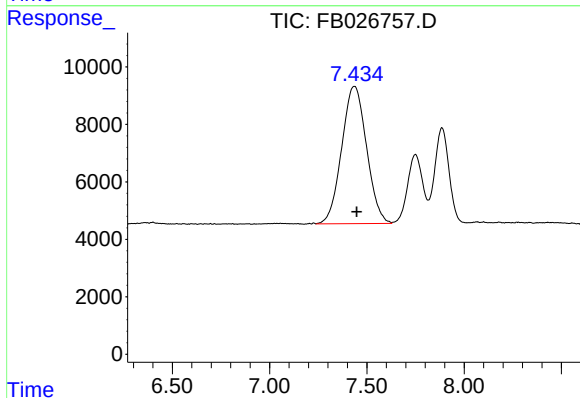


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: -0.011 min
Response: 424680
Conc: 20.49 ng/ml

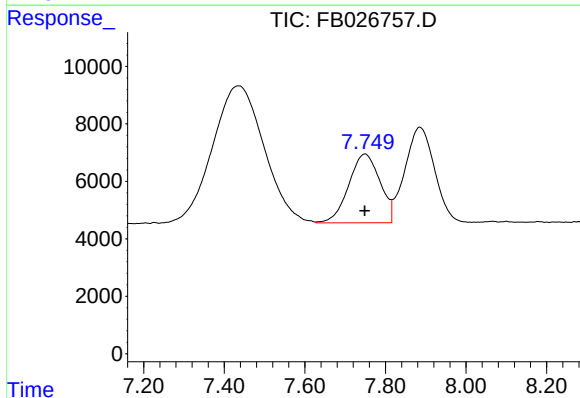


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 129031
Conc: 6.52 ng/ml

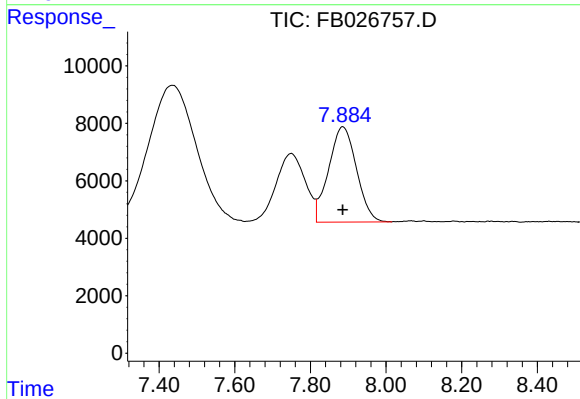


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 169915
Conc: 7.36 ng/ml

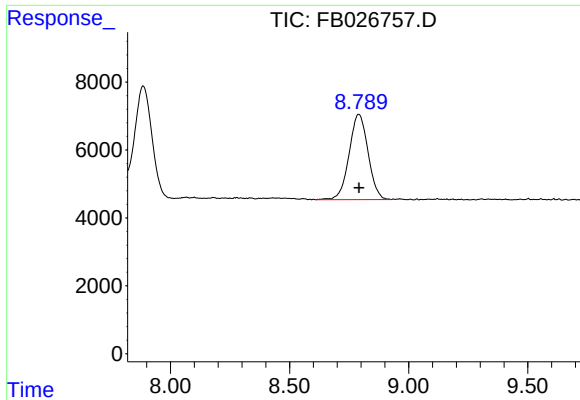


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 138931
Conc: 13.24 ng/ml

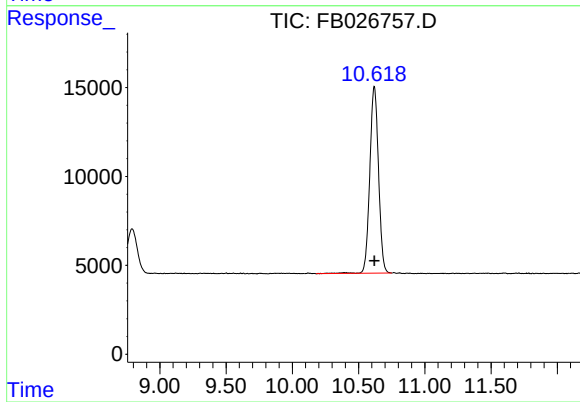


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 479901
Conc: 21.92 ng/ml

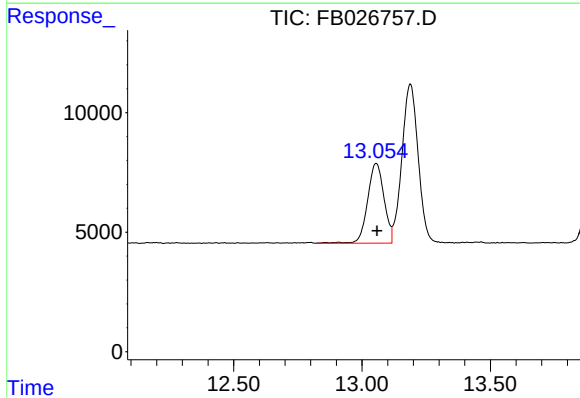


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 148254
Conc: 7.38 ng/ml

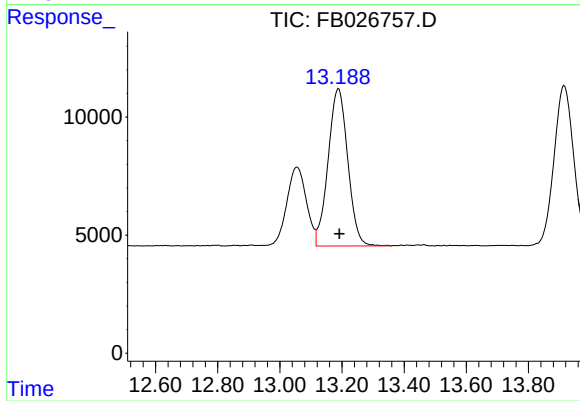


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.003 min
Response: 293025
Conc: 14.54 ng/ml

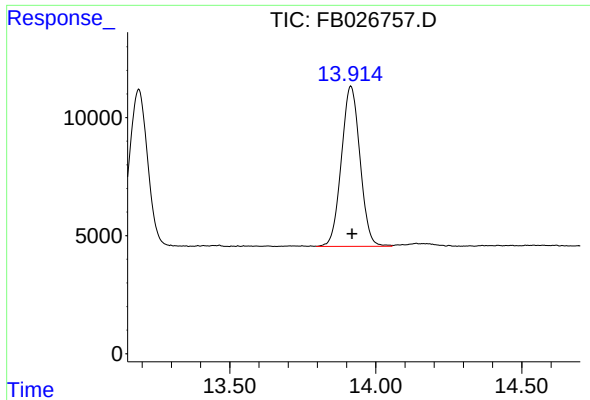

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.004 min
Response: 300251
Conc: 15.05 ng/ml

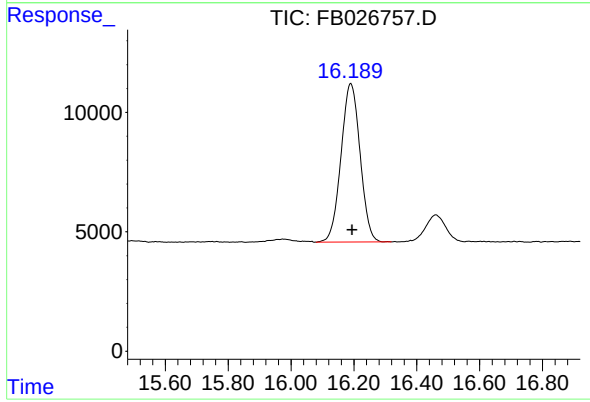

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.004 min
Response: 279071
Conc: 14.01 ng/ml