

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
Data File : FB029535.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2023 10:52
Operator : YP/AJ
Sample : 02021-03
Misc : 9.81G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 21 15:49:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	192846	15.917 ng/ml
Target Compounds			
6) t Toluene	10.617	21508	1.090 ng/ml
8) t m-Xylene	13.181	7974	0.429 ng/ml
9) t O-Xylene	13.919	4858	0.264 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	6587	0.354 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
Data File : FB029535.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2023 10:52
Operator : YP/AJ
Sample : 02021-03
Misc : 9.81G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 21 15:49:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

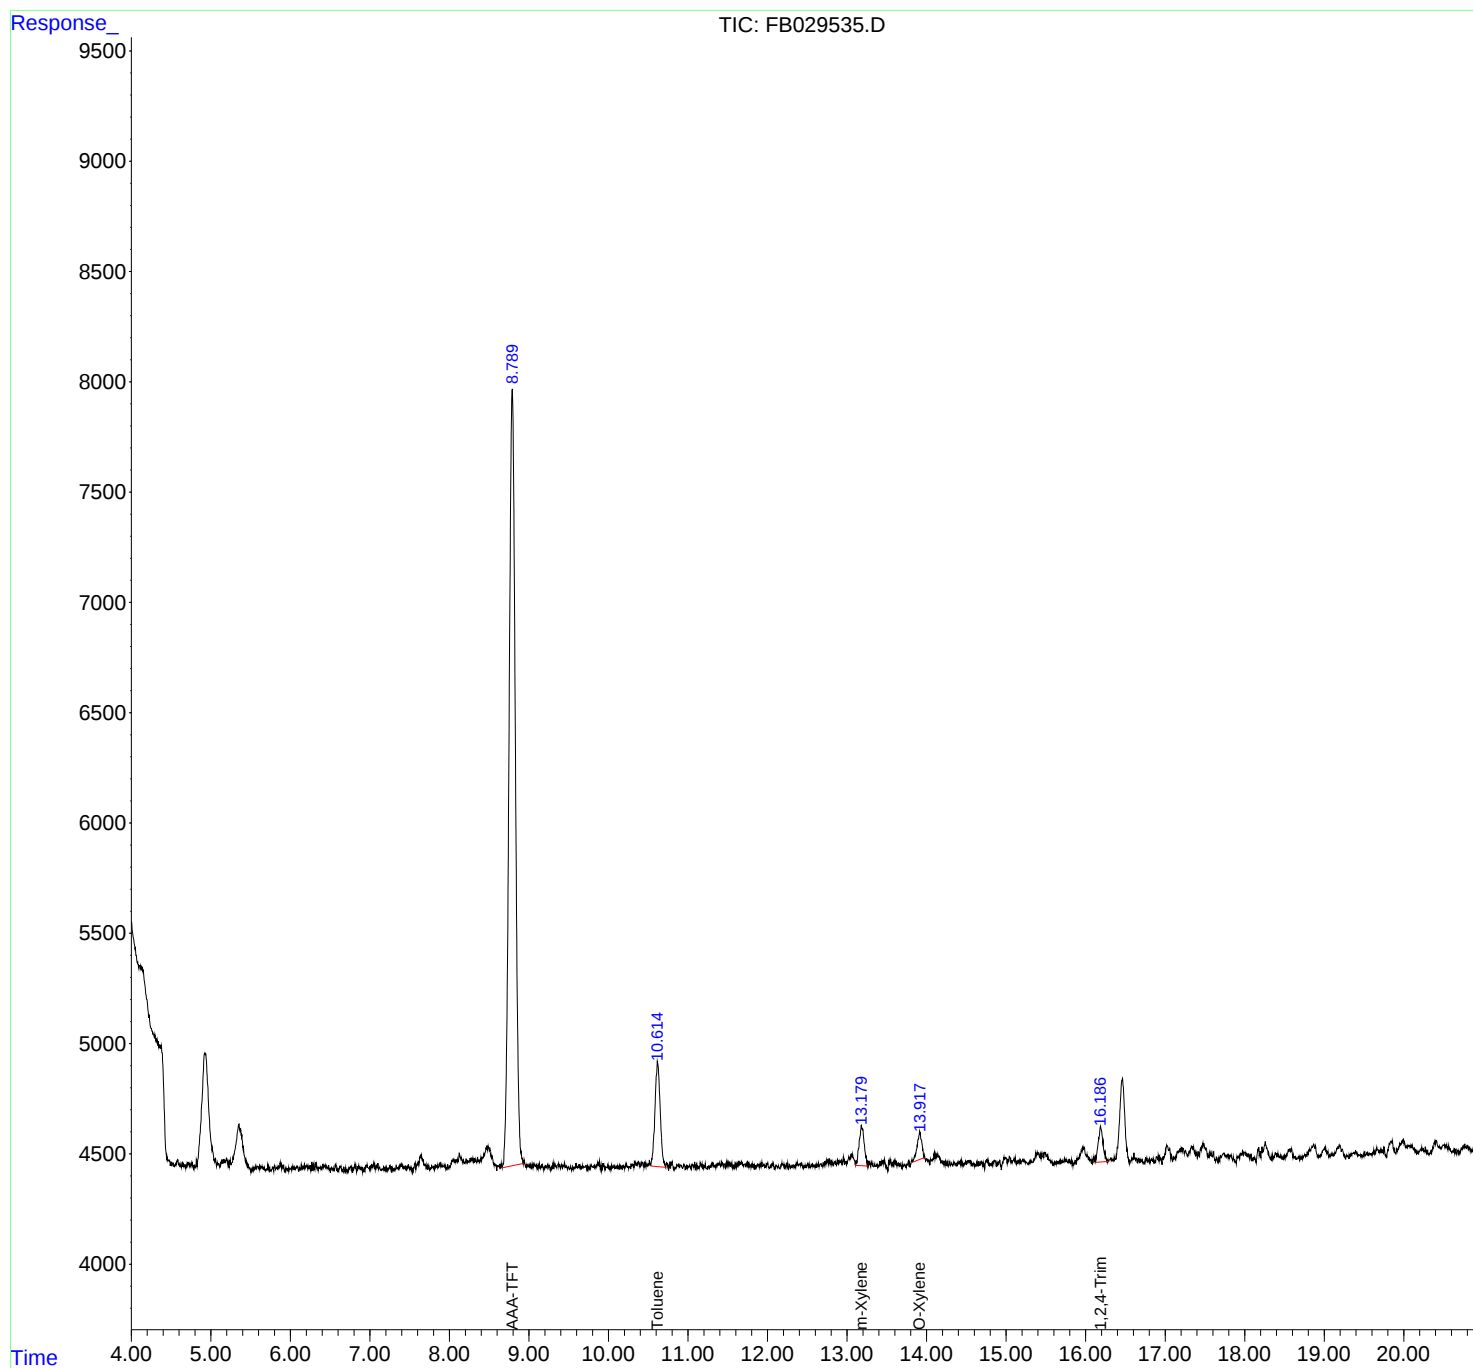


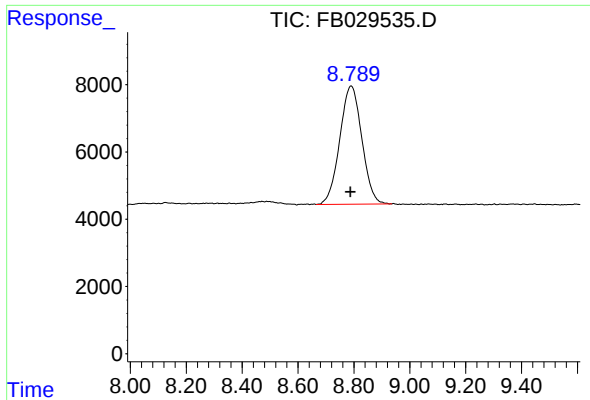

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.003 min
Response: 192846
Conc: 15.92 ng/ml

Instrument :
FID_B
ClientSampleId :

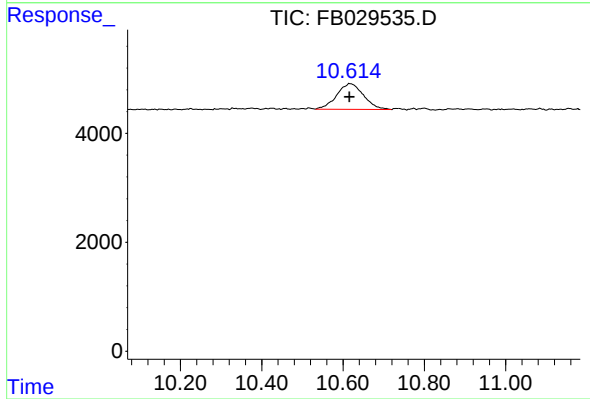


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 21508
Conc: 1.09 ng/ml

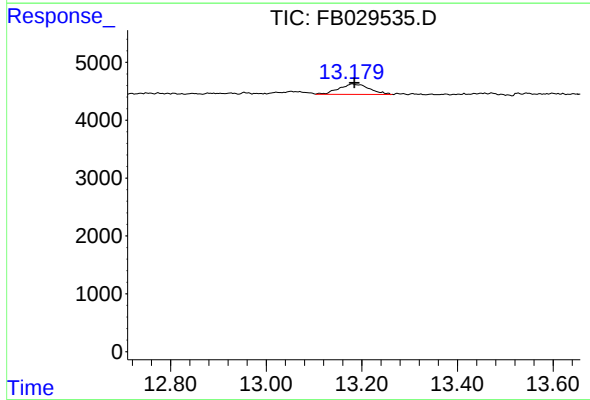


#8 m-Xylene

R.T.: 13.181 min
Delta R.T.: -0.004 min
Response: 7974
Conc: 0.43 ng/ml

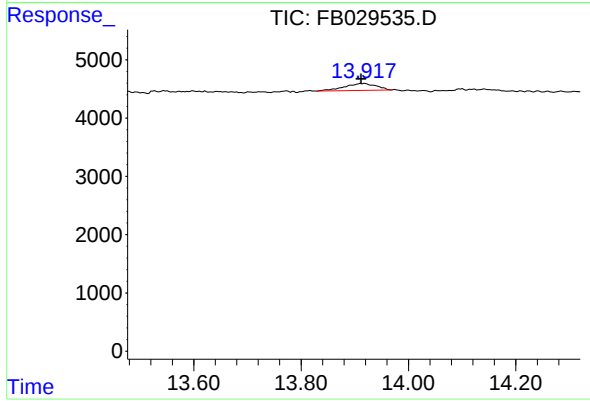

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.007 min
Response: 4858
Conc: 0.26 ng/ml

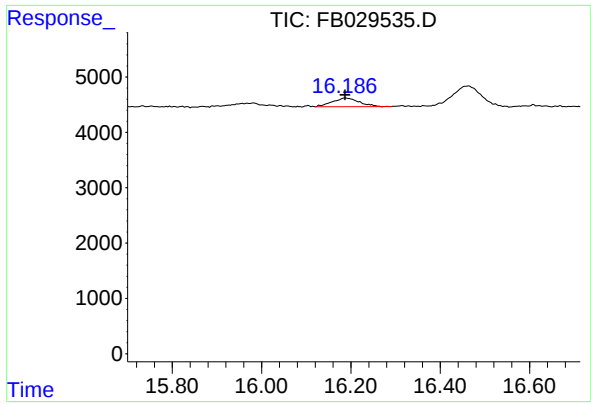

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.001 min
Response: 6587
Conc: 0.35 ng/ml

Instrument :
FID_B
ClientSampleId :