

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
 Data File : FB029536.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2023 11:30
 Operator : YP/AJ
 Sample : 02021-07
 Misc : 6.73G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 21 15:49:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	194129	16.023 ng/ml
Target Compounds			
6) t Toluene	10.619	36435	1.846 ng/ml
7) t Ethylbenzene	13.057	38942	2.092 ng/ml
8) t m-Xylene	13.185	93134	5.006 ng/ml
9) t O-Xylene	13.916	141295	7.674 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	21272	1.142 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
Data File : FB029536.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2023 11:30
Operator : YP/AJ
Sample : 02021-07
Misc : 6.73G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 21 15:49:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

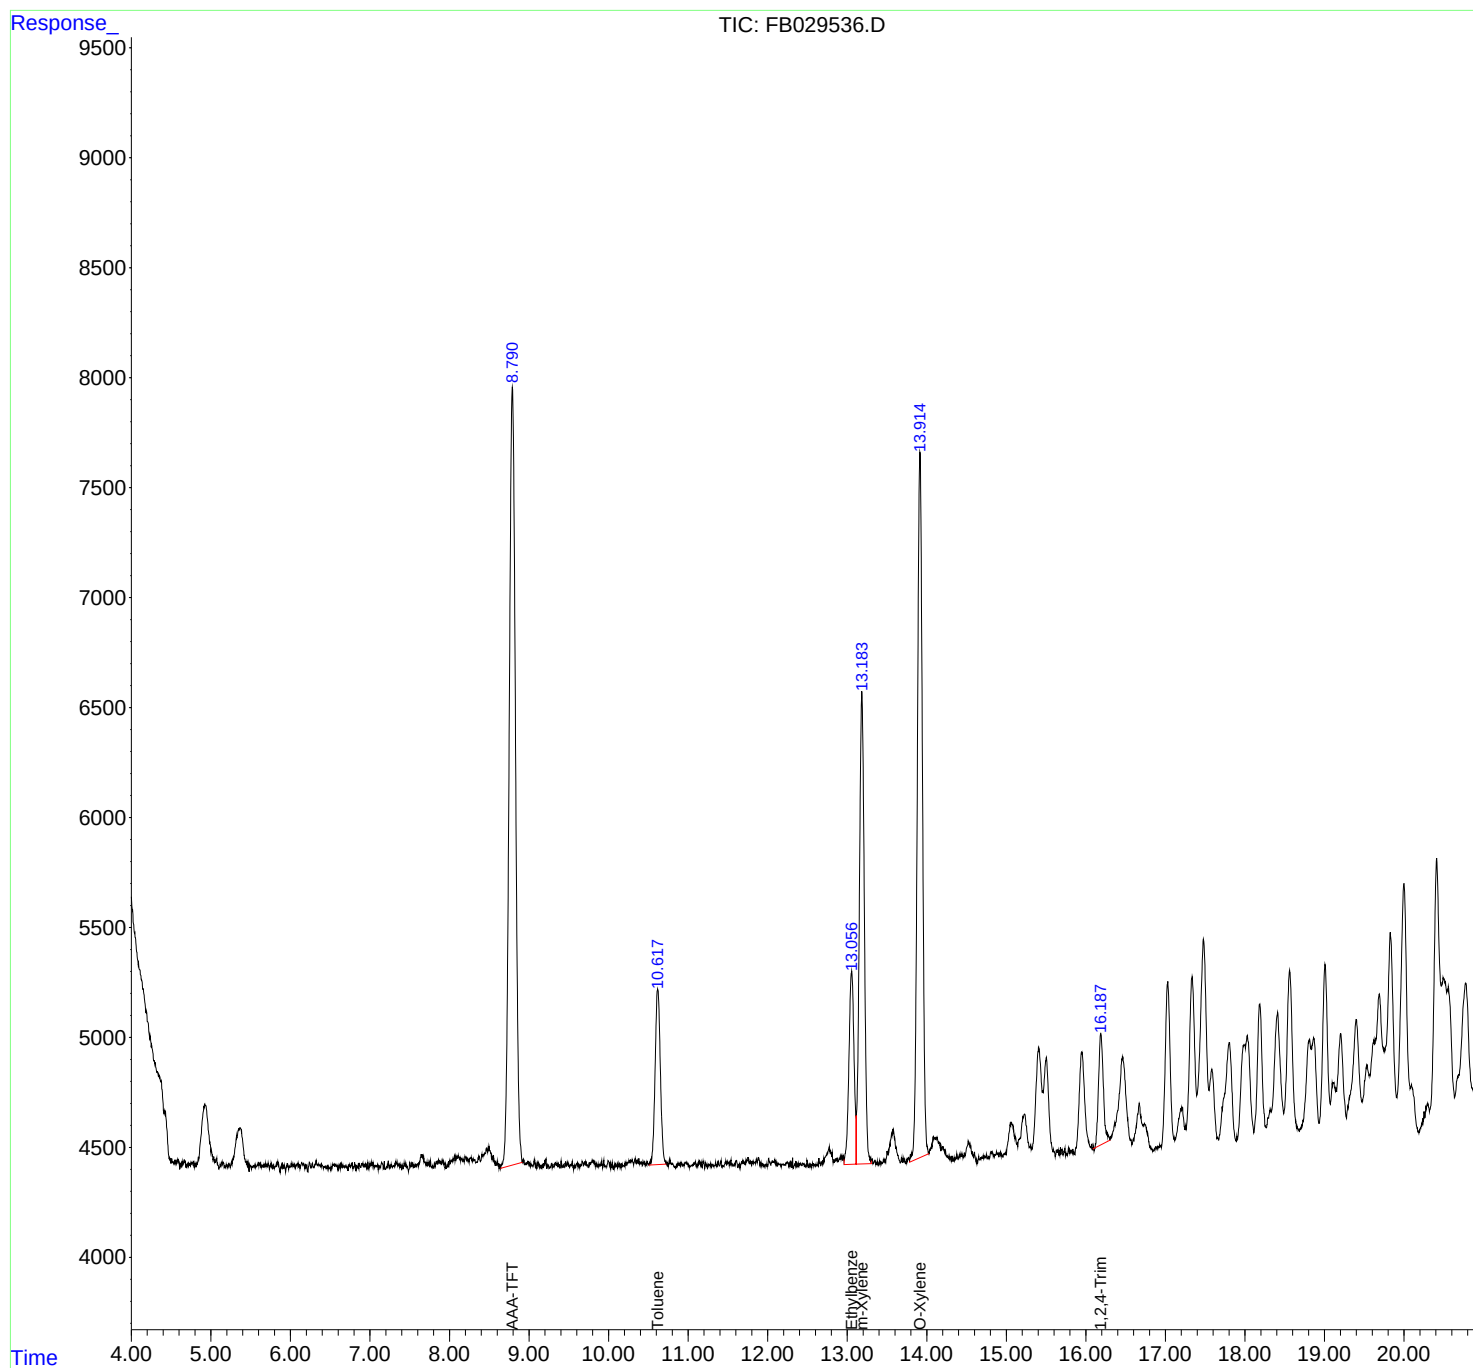


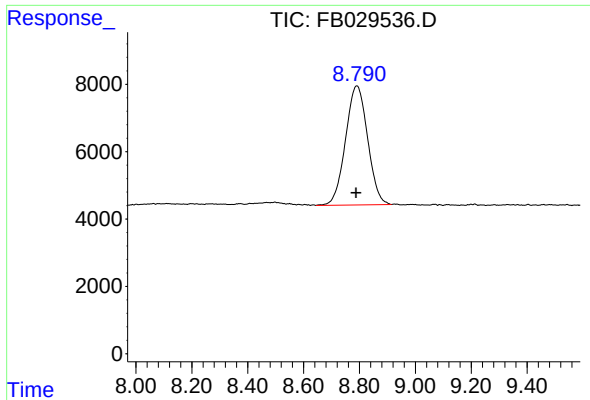

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.003 min
Response: 194129
Conc: 16.02 ng/ml

Instrument :
FID_B
ClientSampleId :

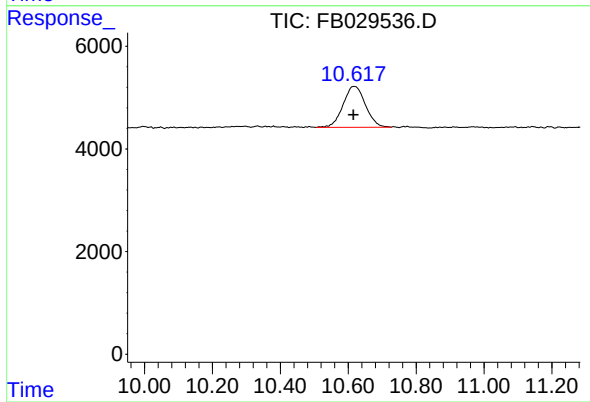


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.003 min
Response: 36435
Conc: 1.85 ng/ml

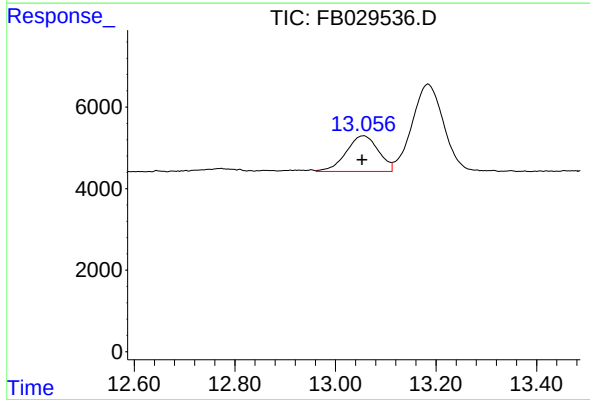


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.004 min
Response: 38942
Conc: 2.09 ng/ml

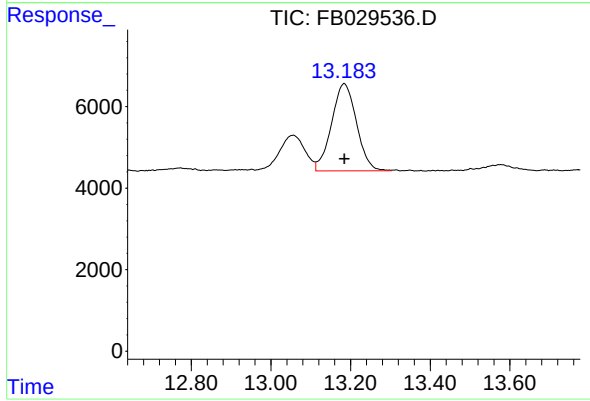

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 93134
Conc: 5.01 ng/ml

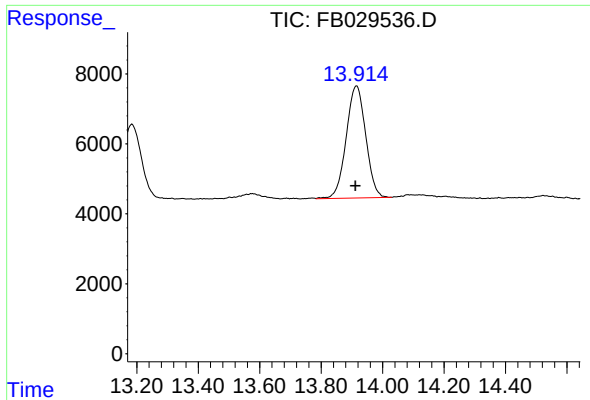

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.004 min
Response: 141295
Conc: 7.67 ng/ml

Instrument :
FID_B
ClientSampleId :

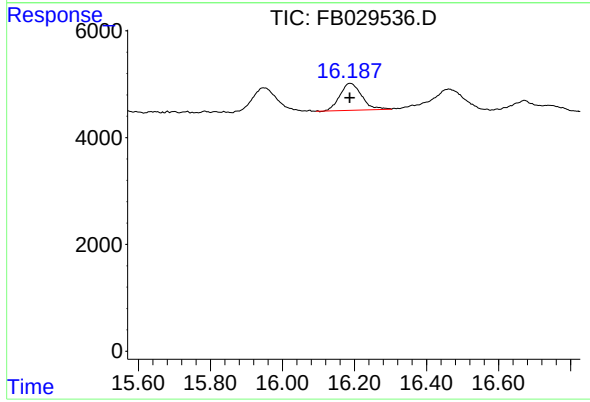

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.001 min
Response: 21272
Conc: 1.14 ng/ml