

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
 Data File : FB029534.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2023 10:13
 Operator : YP/AJ
 Sample : BSF0321S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0321S1

Integration File: Calibration.e
 Quant Time: Mar 21 15:48:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	275917	22.774 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	438623	28.586 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	511149	30.345 ng/ml
3) t n-Heptane	7.747	169220	9.784 ng/ml
4) t Benzene	7.883	213834	10.535 ng/ml
6) t Toluene	10.616	617770	31.297 ng/ml
7) t Ethylbenzene	13.053	196524	10.556 ng/ml
8) t m-Xylene	13.185	388468	20.881 ng/ml
9) t O-Xylene	13.912	373989	20.311 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	357249	19.180 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
Data File : FB029534.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2023 10:13
Operator : YP/AJ
Sample : BSF0321S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0321S1

Integration File: Calibration.e
Quant Time: Mar 21 15:48:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

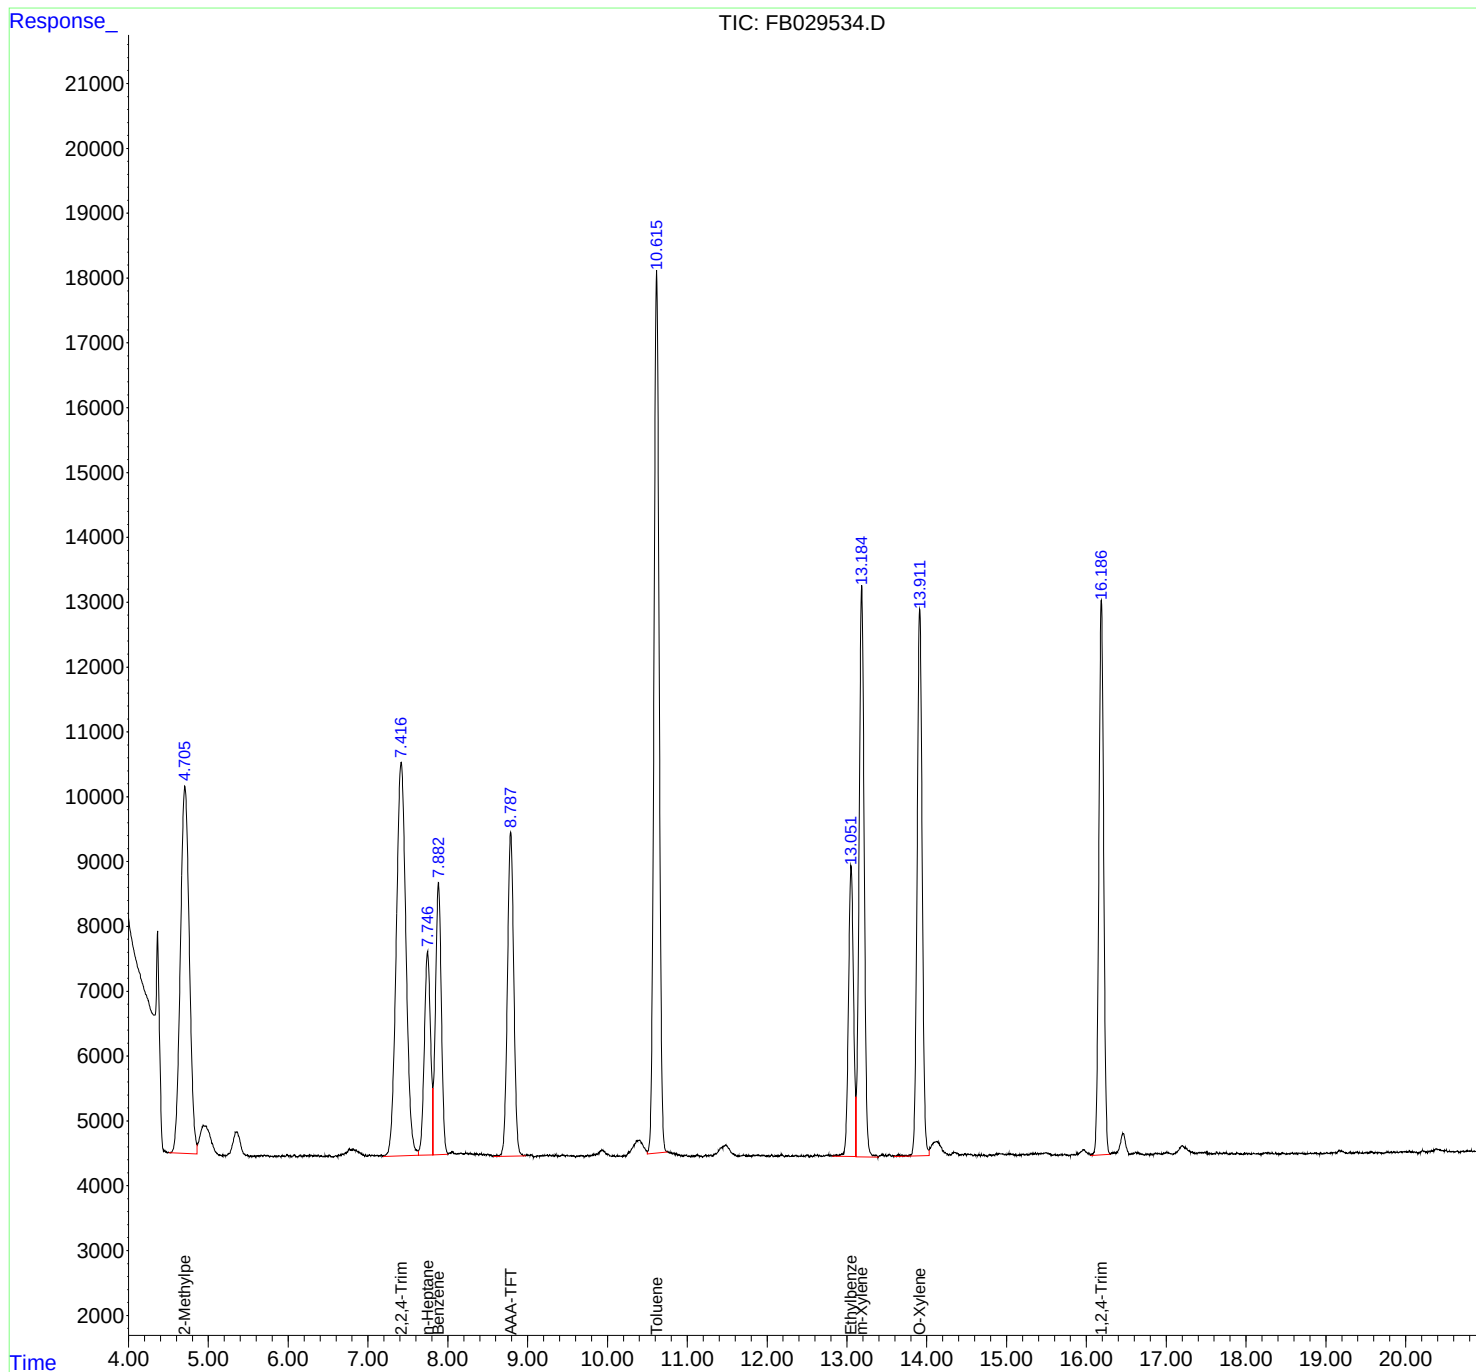


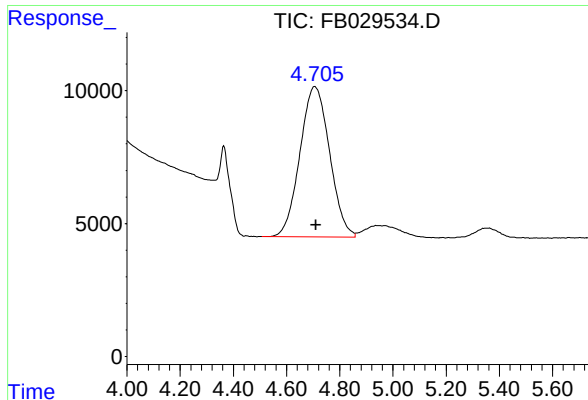

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.004 min
Response: 438623
Conc: 28.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0321S1

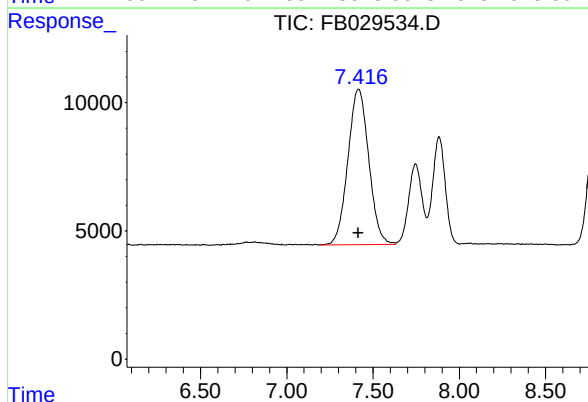


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.001 min
Response: 511149
Conc: 30.34 ng/ml

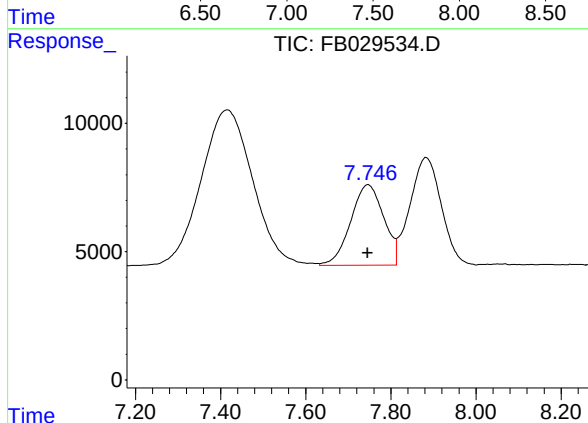


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.001 min
Response: 169220
Conc: 9.78 ng/ml

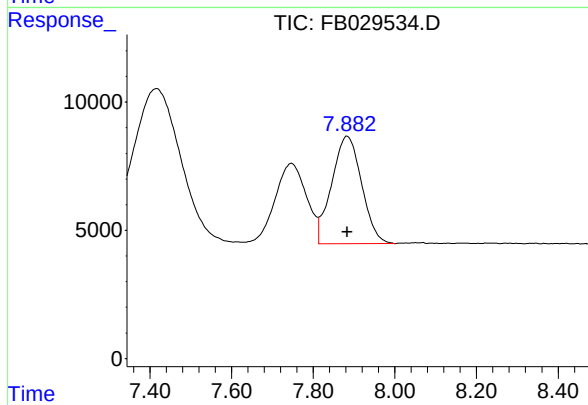

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.000 min
Response: 213834
Conc: 10.53 ng/ml

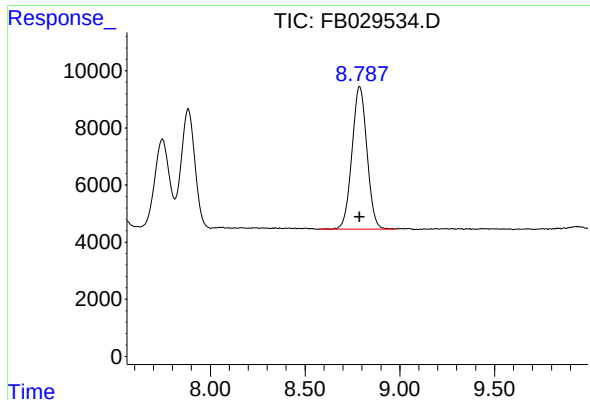

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 275917
Conc: 22.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0321S1

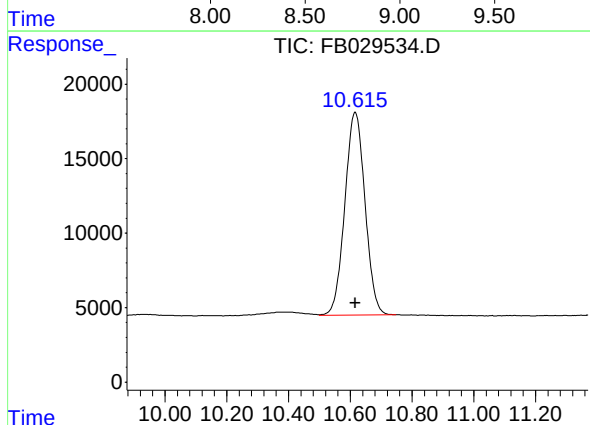


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.000 min
Response: 617770
Conc: 31.30 ng/ml

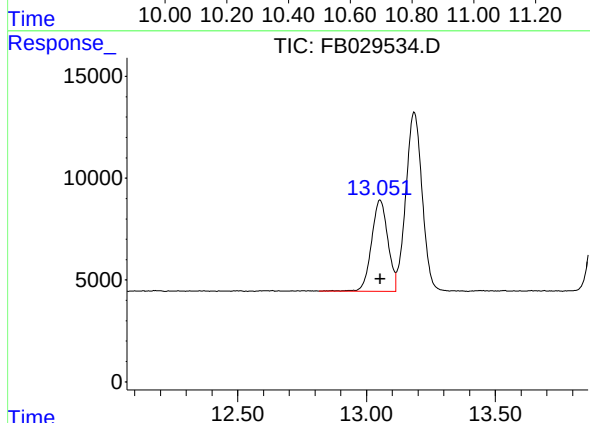


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.000 min
Response: 196524
Conc: 10.56 ng/ml

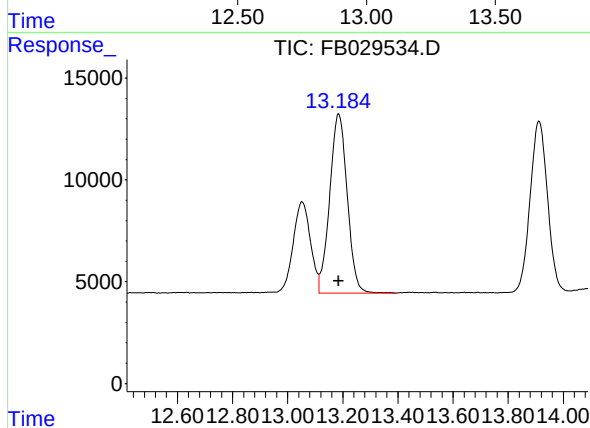

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 388468
Conc: 20.88 ng/ml

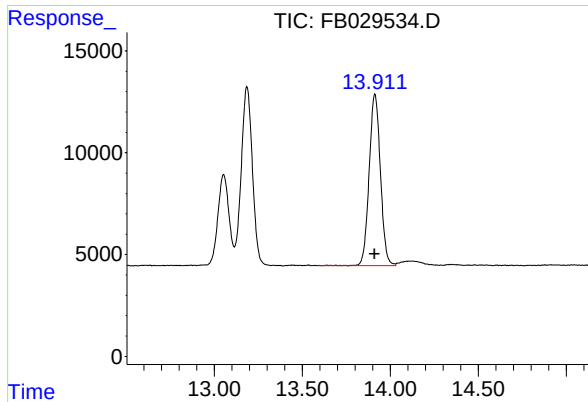

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.000 min
Response: 373989
Conc: 20.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0321S1

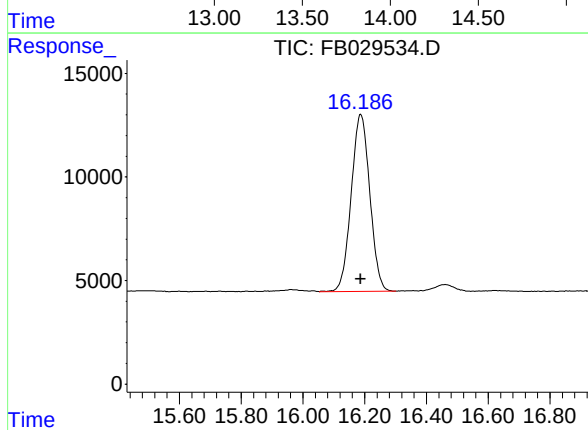

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 357249
Conc: 19.18 ng/ml