

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
 Data File : FB029539.D
 Signal(s) : FID2B.CH
 Acq On : 21 Mar 2023 13:24
 Operator : YP/AJ
 Sample : BSF0321S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0321S2

Integration File: Calibration.e
 Quant Time: Mar 21 15:49:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	228203	18.835 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	413302	26.936 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	488430	28.996 ng/ml
3) t n-Heptane	7.751	157135	9.085 ng/ml
4) t Benzene	7.888	200162	9.861 ng/ml
6) t Toluene	10.621	600511	30.423 ng/ml
7) t Ethylbenzene	13.057	190342	10.224 ng/ml
8) t m-Xylene	13.190	375233	20.170 ng/ml
9) t O-Xylene	13.917	359439	19.521 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	346469	18.602 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032123\
Data File : FB029539.D
Signal(s) : FID2B.CH
Acq On : 21 Mar 2023 13:24
Operator : YP/AJ
Sample : BSF0321S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0321S2

Integration File: Calibration.e
Quant Time: Mar 21 15:49:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

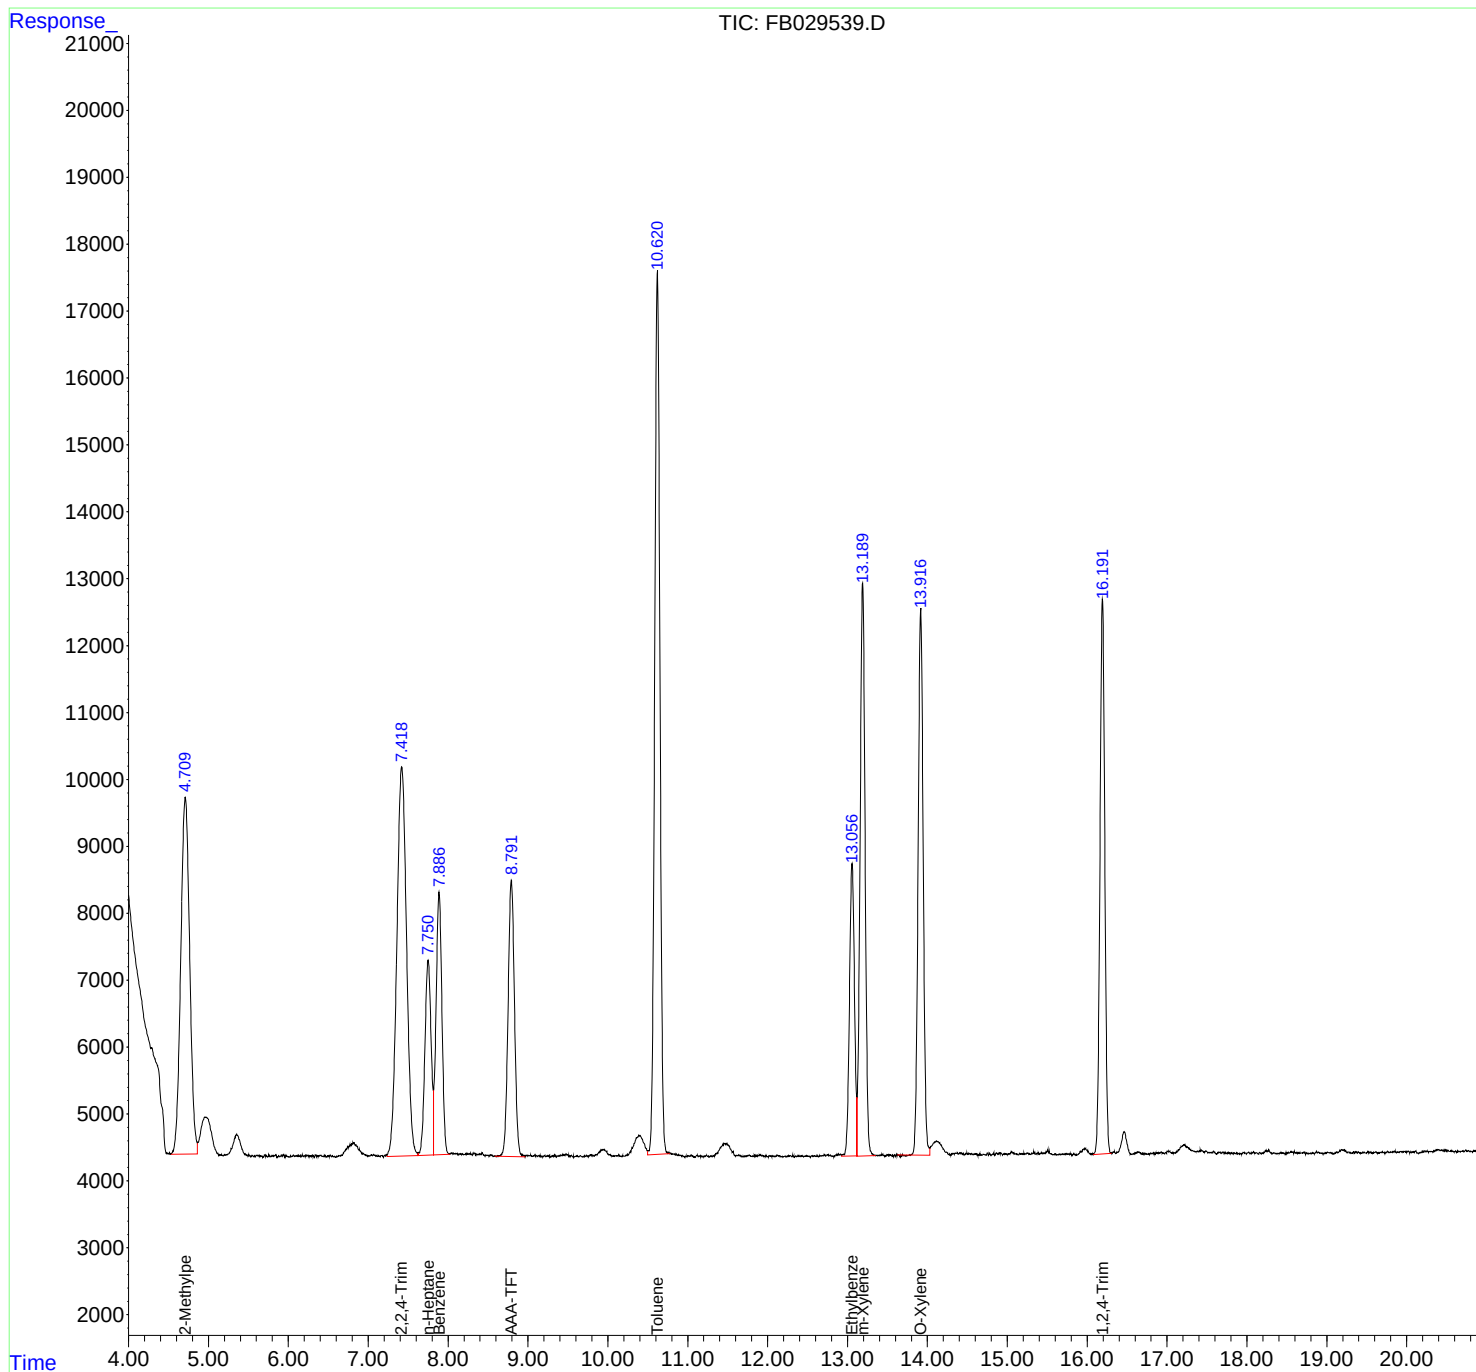


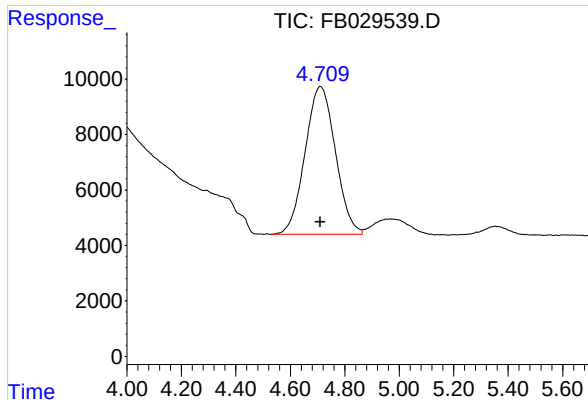

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 413302
Conc: 26.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0321S2

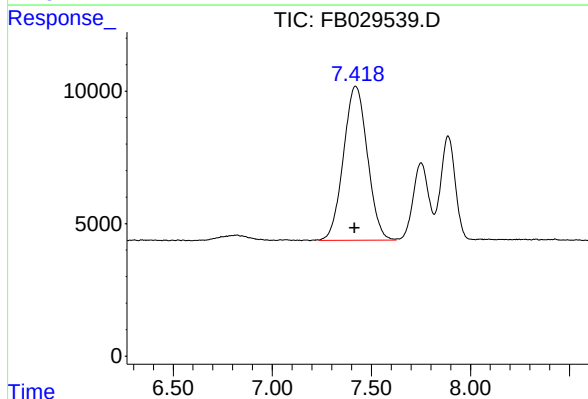


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.004 min
Response: 488430
Conc: 29.00 ng/ml

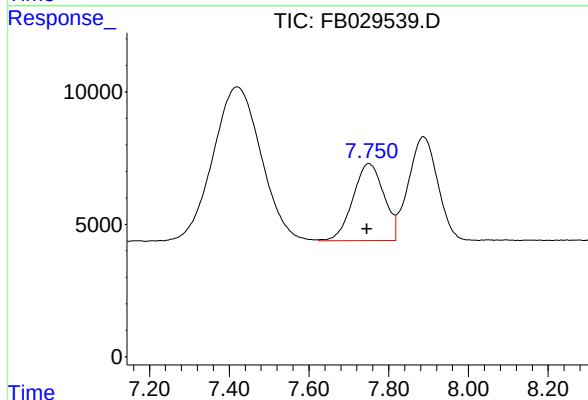


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.005 min
Response: 157135
Conc: 9.09 ng/ml

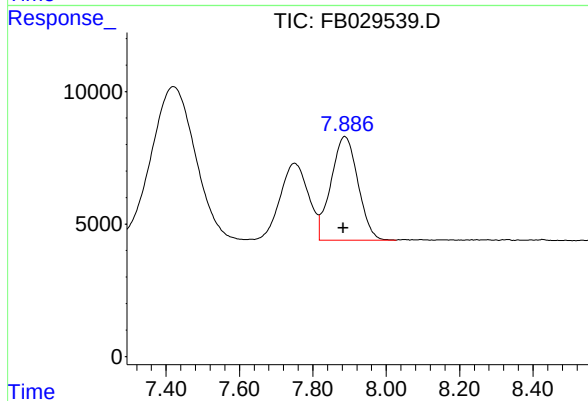

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.004 min
Response: 200162
Conc: 9.86 ng/ml

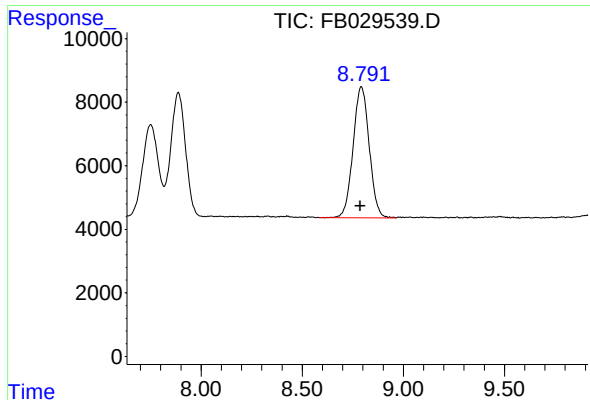

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.005 min
Response: 228203
Conc: 18.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0321S2

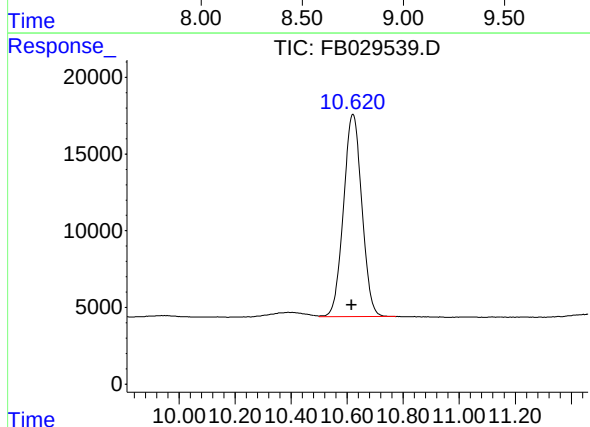


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.005 min
Response: 600511
Conc: 30.42 ng/ml

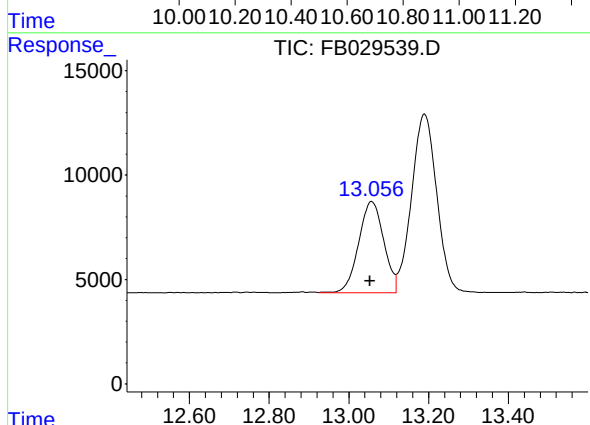


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.005 min
Response: 190342
Conc: 10.22 ng/ml

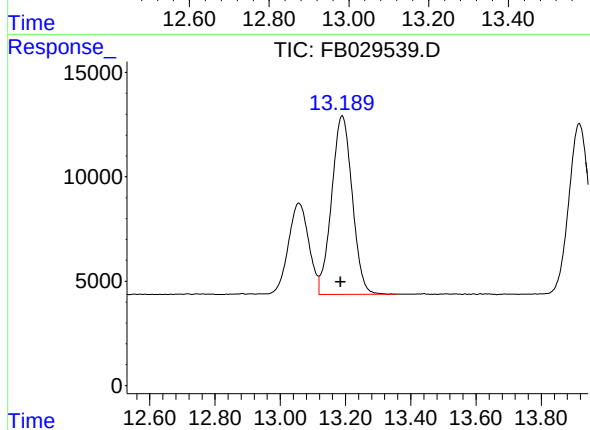

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.005 min
Response: 375233
Conc: 20.17 ng/ml

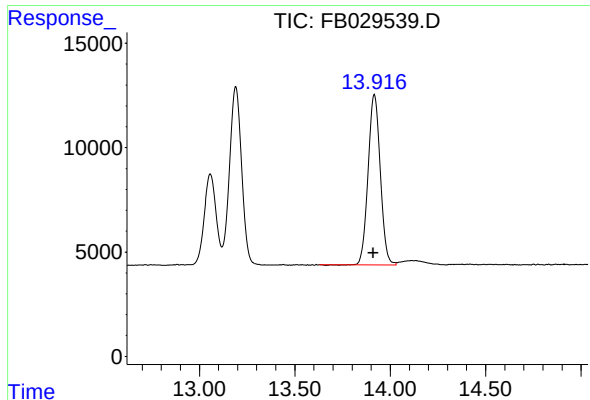

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.005 min
Response: 359439
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0321S2

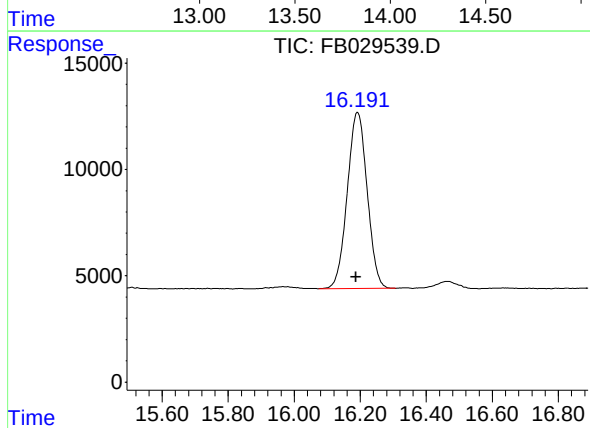

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.005 min
Response: 346469
Conc: 18.60 ng/ml