

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026759.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 14:53
Operator : AJ/MA
Sample : BSF0322S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 02:37:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	298196	28.417 ng/ml
Target Compounds			
6) t Toluene	10.616	4050	0.185 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026759.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 14:53
Operator : AJ/MA
Sample : BSF0322S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 02:37:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

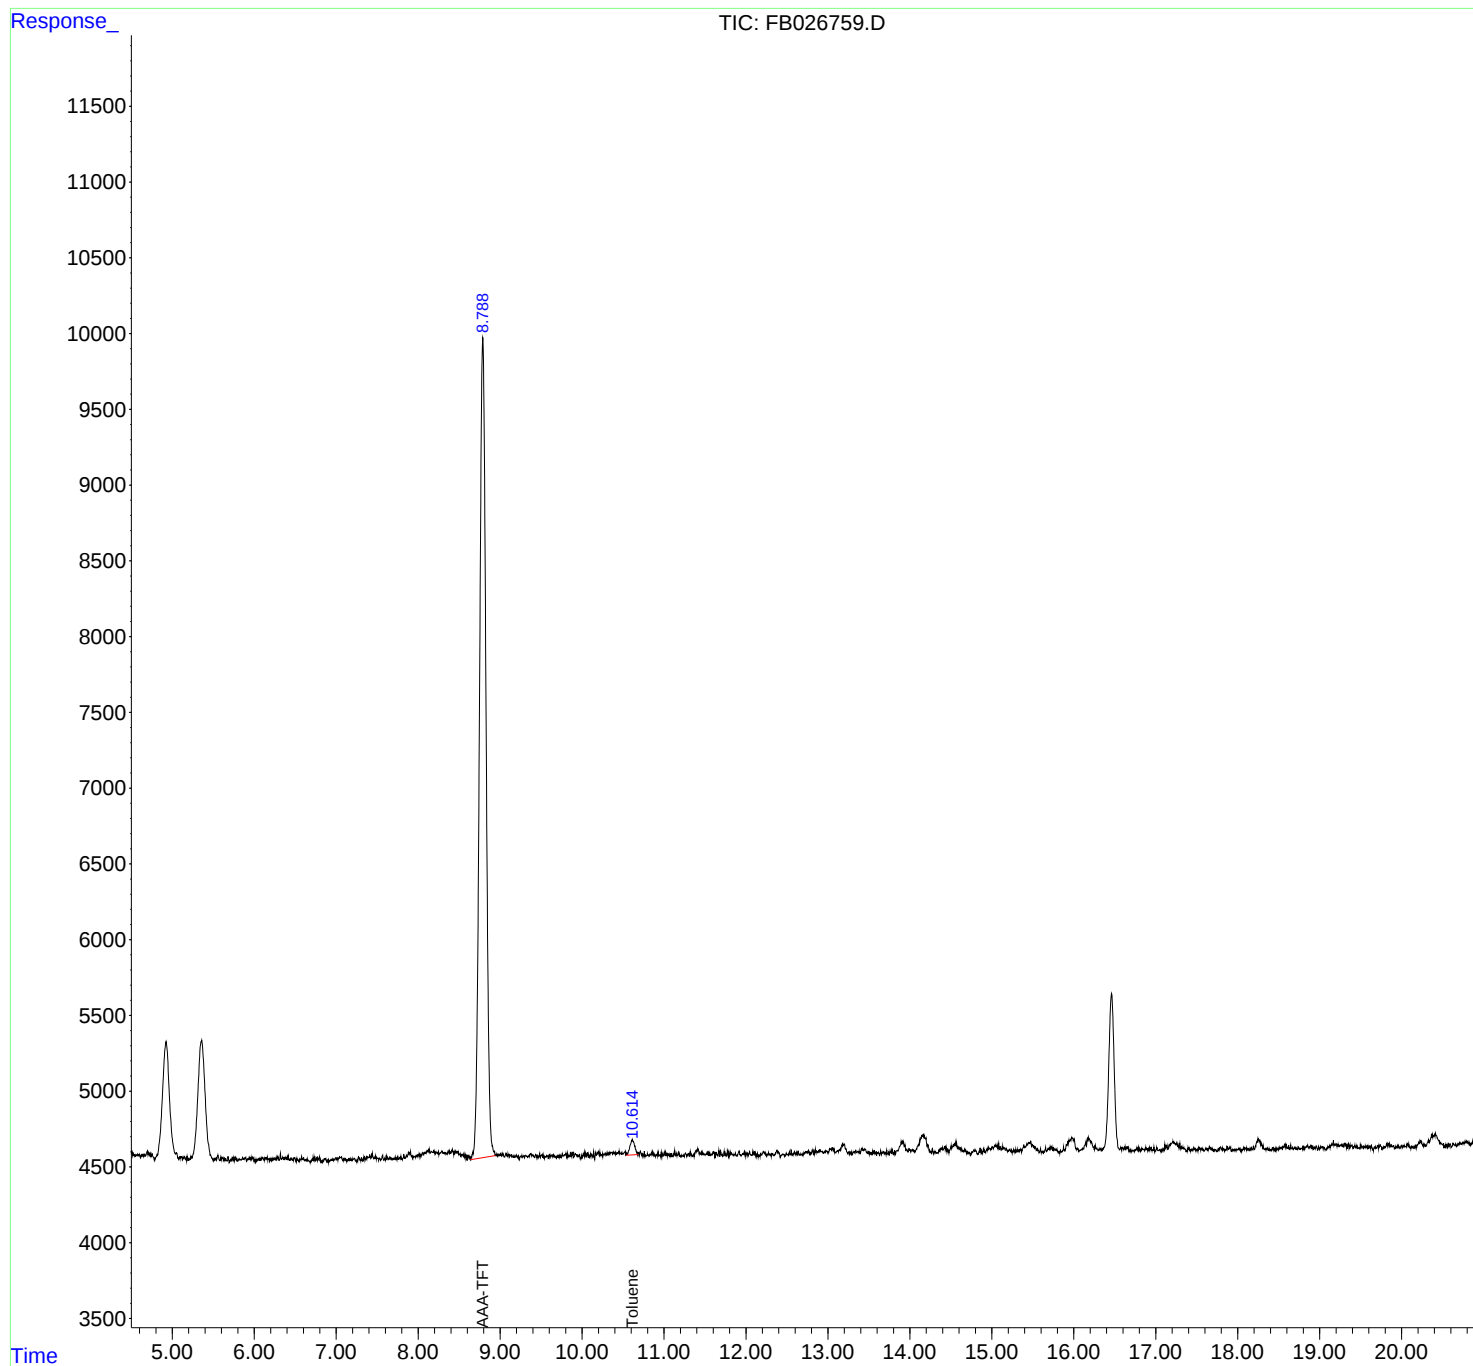

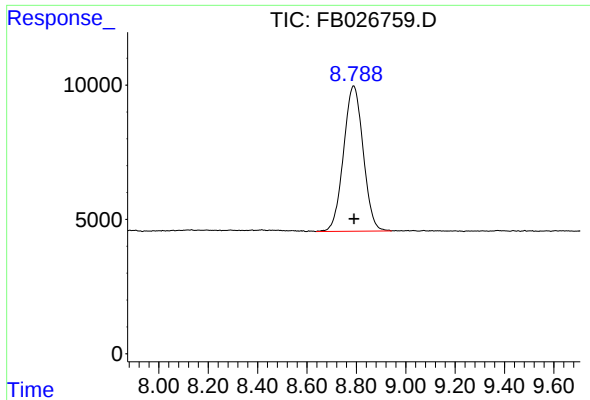


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 298196
Conc: 28.42 ng/ml

Instrument :

FID_B

ClientSampleId :

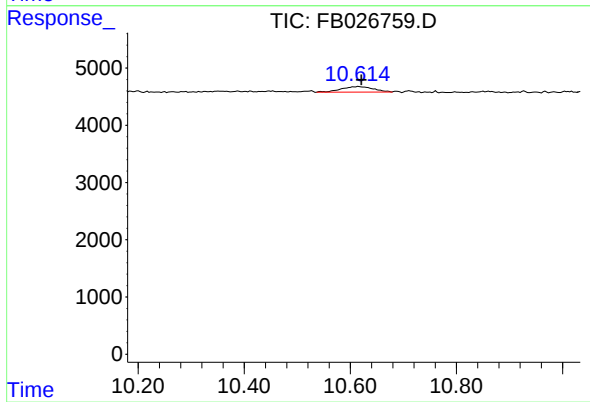

#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 4050
Conc: 0.18 ng/ml