

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB032222\  
 Data File : FB026767.D  
 Signal(s) : FID2B.CH  
 Acq On : 22 Mar 2022 20:03  
 Operator : AJ/MA  
 Sample : N1974-06MS  
 Misc : 5.01G/5.00 ML DI WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Mar 23 02:38:05 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030822.M  
 Quant Title :  
 QLast Update : Fri Mar 11 13:08:49 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.789  | 239341   | 22.809 ng/ml |
| Target Compounds             |        |          |              |
| 1) t 2-Methylpentane         | 4.705  | 438493   | 23.160 ng/ml |
| 2) t 2,2,4-Trimethylpentane  | 7.429  | 504444   | 24.337 ng/ml |
| 3) t n-Heptane               | 7.746  | 153200   | 7.740 ng/ml  |
| 4) t Benzene                 | 7.883  | 217109   | 9.409 ng/ml  |
| 6) t Toluene                 | 10.616 | 616817   | 28.174 ng/ml |
| 7) t Ethylbenzene            | 13.053 | 191616   | 9.534 ng/ml  |
| 8) t m-Xylene                | 13.186 | 381385   | 18.925 ng/ml |
| 9) t O-Xylene                | 13.913 | 374642   | 18.779 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.189 | 379138   | 19.029 ng/ml |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB032222\  
Data File : FB026767.D  
Signal(s) : FID2B.CH  
Acq On : 22 Mar 2022 20:03  
Operator : AJ/MA  
Sample : N1974-06MS  
Misc : 5.01G/5.00 ML DI WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Mar 23 02:38:05 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030822.M  
Quant Title :  
QLast Update : Fri Mar 11 13:08:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

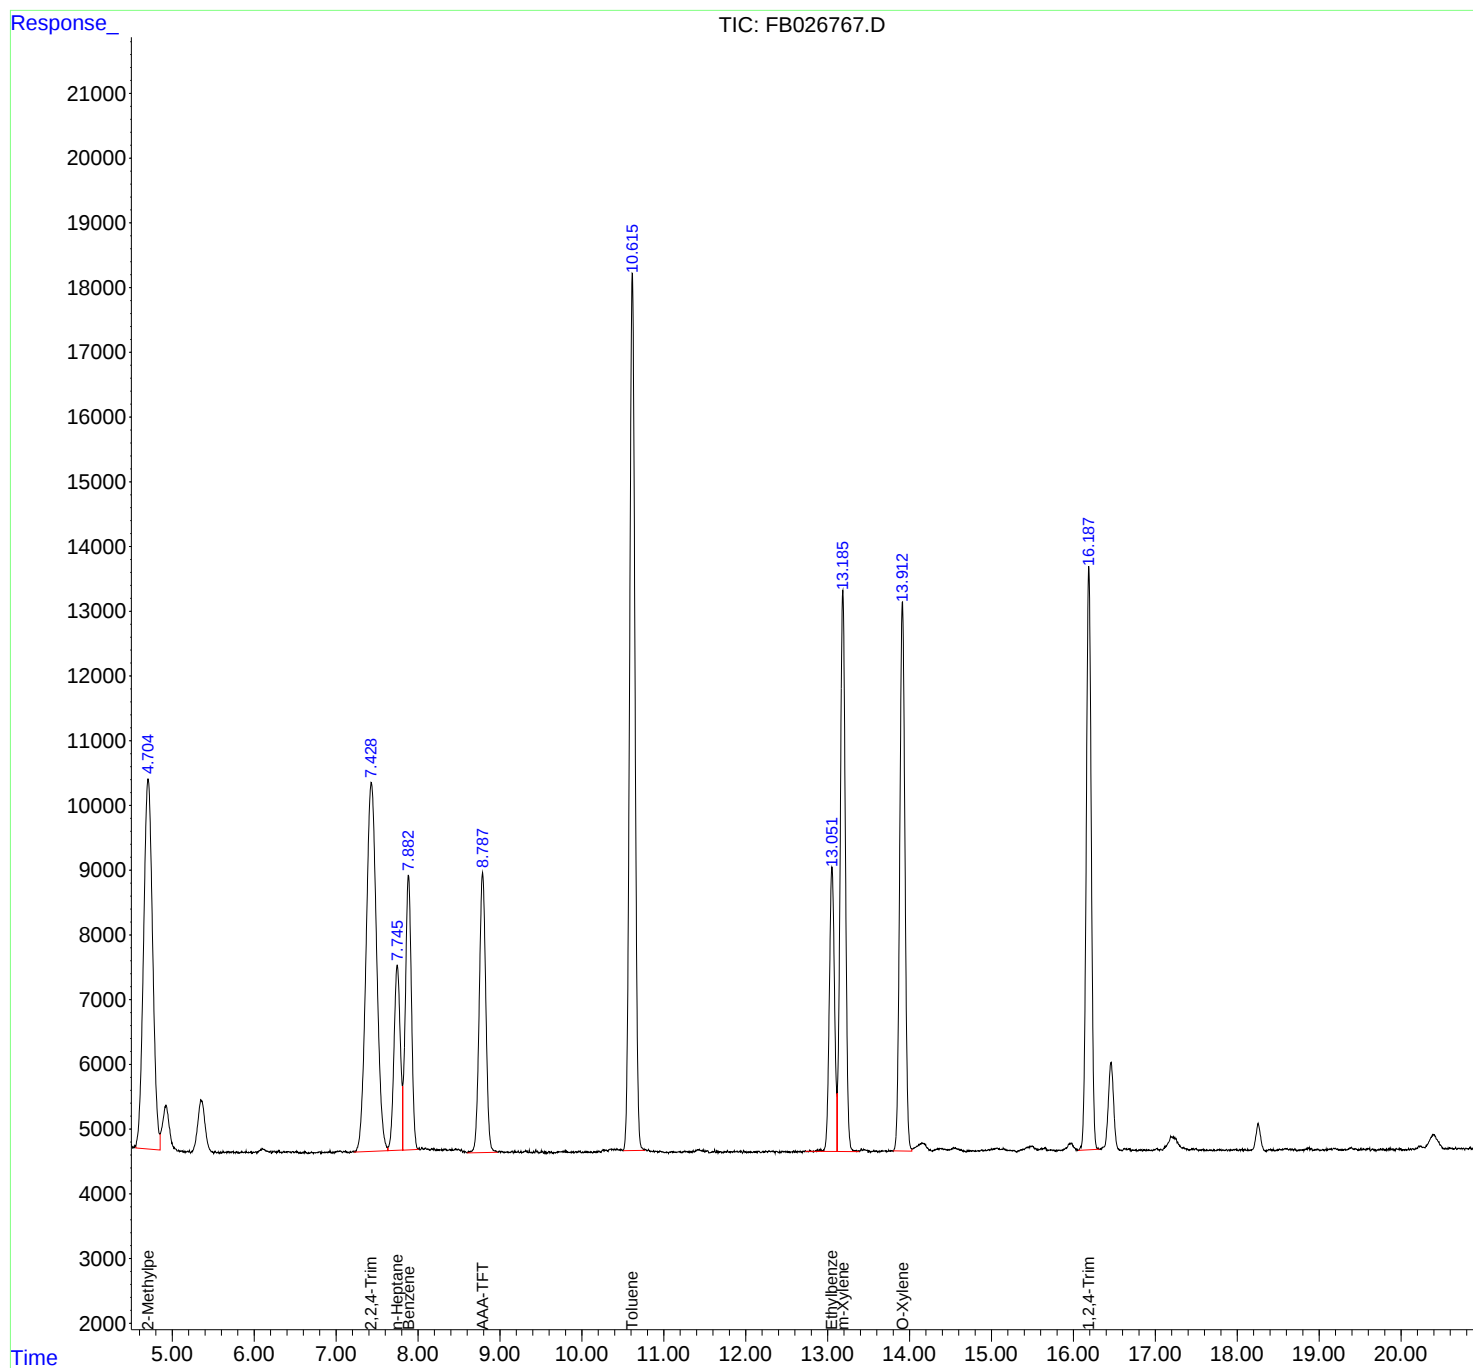


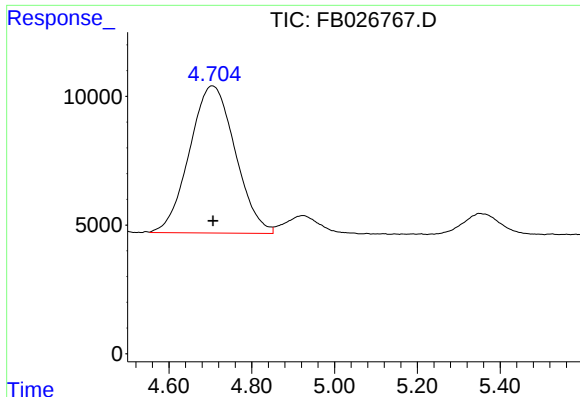

#1 2-Methylpentane


R.T.: 4.705 min  
Delta R.T.: -0.002 min  
Response: 438493  
Conc: 23.16 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

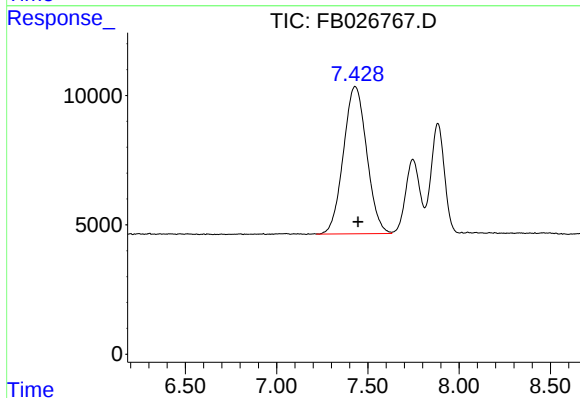


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min  
Delta R.T.: -0.018 min  
Response: 504444  
Conc: 24.34 ng/ml

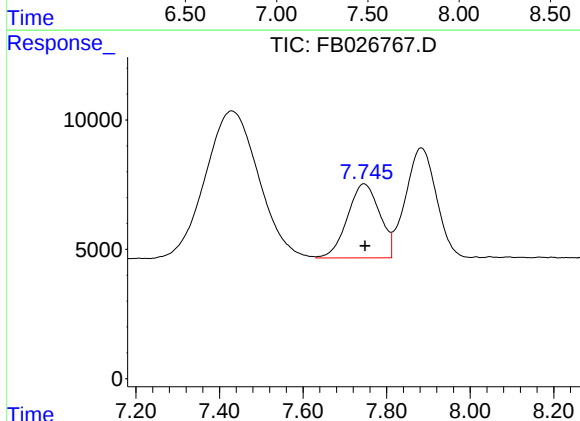


#3 n-Heptane

R.T.: 7.746 min  
Delta R.T.: -0.002 min  
Response: 153200  
Conc: 7.74 ng/ml

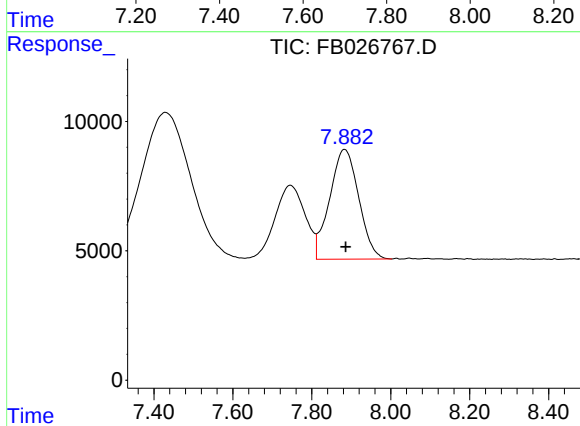

#4 Benzene


R.T.: 7.883 min  
Delta R.T.: -0.002 min  
Response: 217109  
Conc: 9.41 ng/ml

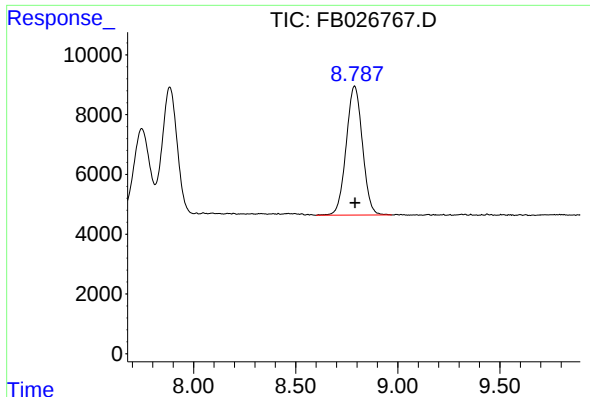

#5 AAA-TFT


R.T.: 8.789 min  
Delta R.T.: -0.003 min  
Response: 239341  
Conc: 22.81 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

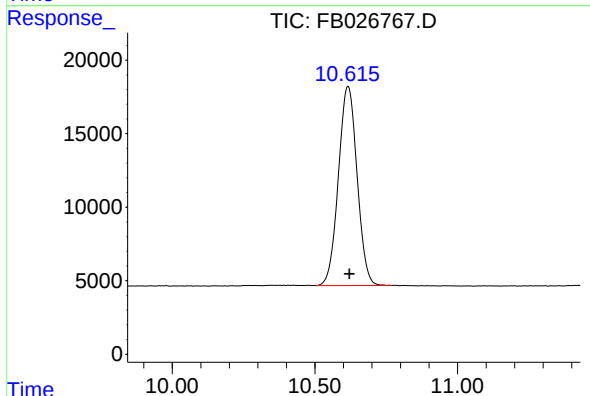


#6 Toluene

R.T.: 10.616 min  
Delta R.T.: -0.005 min  
Response: 616817  
Conc: 28.17 ng/ml

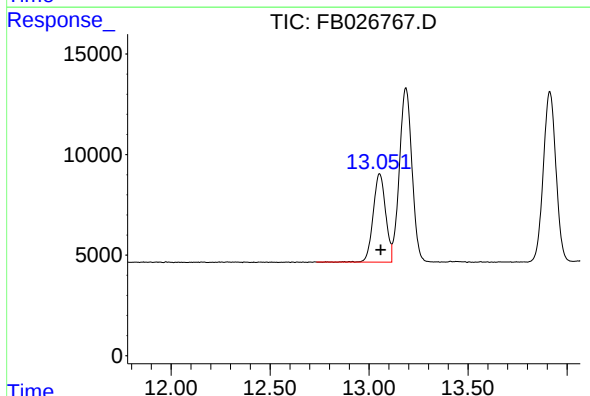


#7 Ethylbenzene

R.T.: 13.053 min  
Delta R.T.: -0.006 min  
Response: 191616  
Conc: 9.53 ng/ml

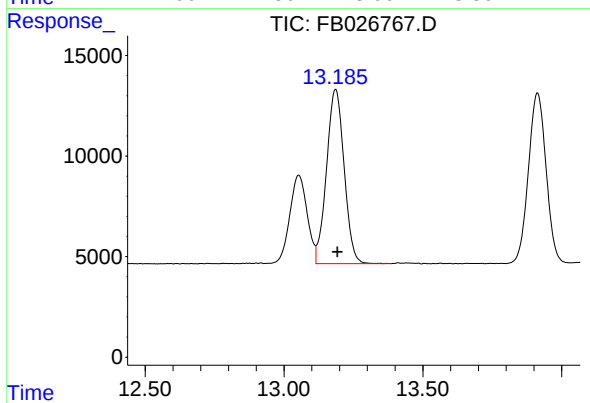

#8 m-Xylene


R.T.: 13.186 min  
Delta R.T.: -0.005 min  
Response: 381385  
Conc: 18.92 ng/ml

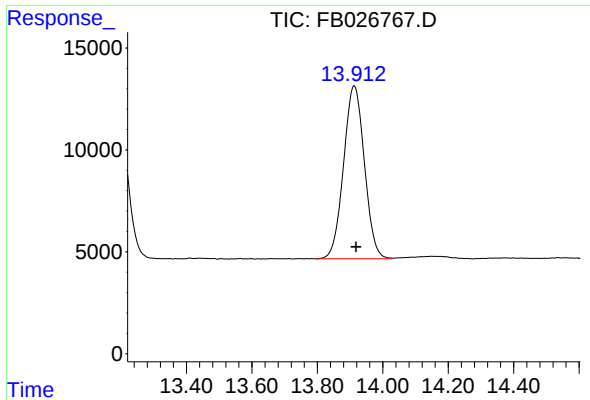

#9 O-Xylene

R.T.: 13.913 min  
Delta R.T.: -0.005 min  
Response: 374642  
Conc: 18.78 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

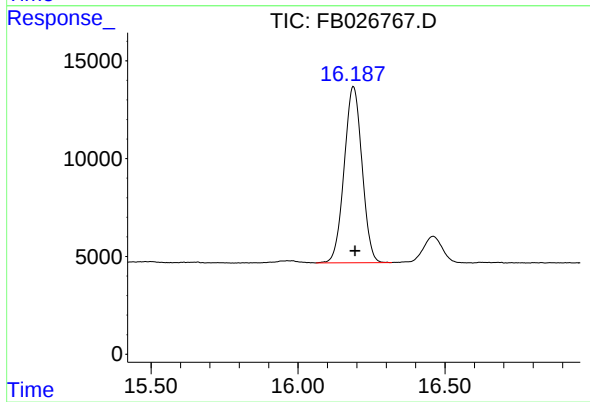

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min  
Delta R.T.: -0.006 min  
Response: 379138  
Conc: 19.03 ng/ml