

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
 Data File : FB026776.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 2:44
 Operator : AJ/MA
 Sample : N1996-12 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 23 03:23:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	208802	19.898 ng/ml
Target Compounds			
4) t Benzene	7.882	213346	9.246 ng/ml
6) t Toluene	10.614	13395	0.612 ng/ml
7) t Ethylbenzene	13.058	5312	0.264 ng/ml
8) t m-Xylene	13.183	9897	0.491 ng/ml
9) t O-Xylene	13.922	10990	0.551 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	7006	0.352 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026776.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 2:44
Operator : AJ/MA
Sample : N1996-12 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 03:23:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

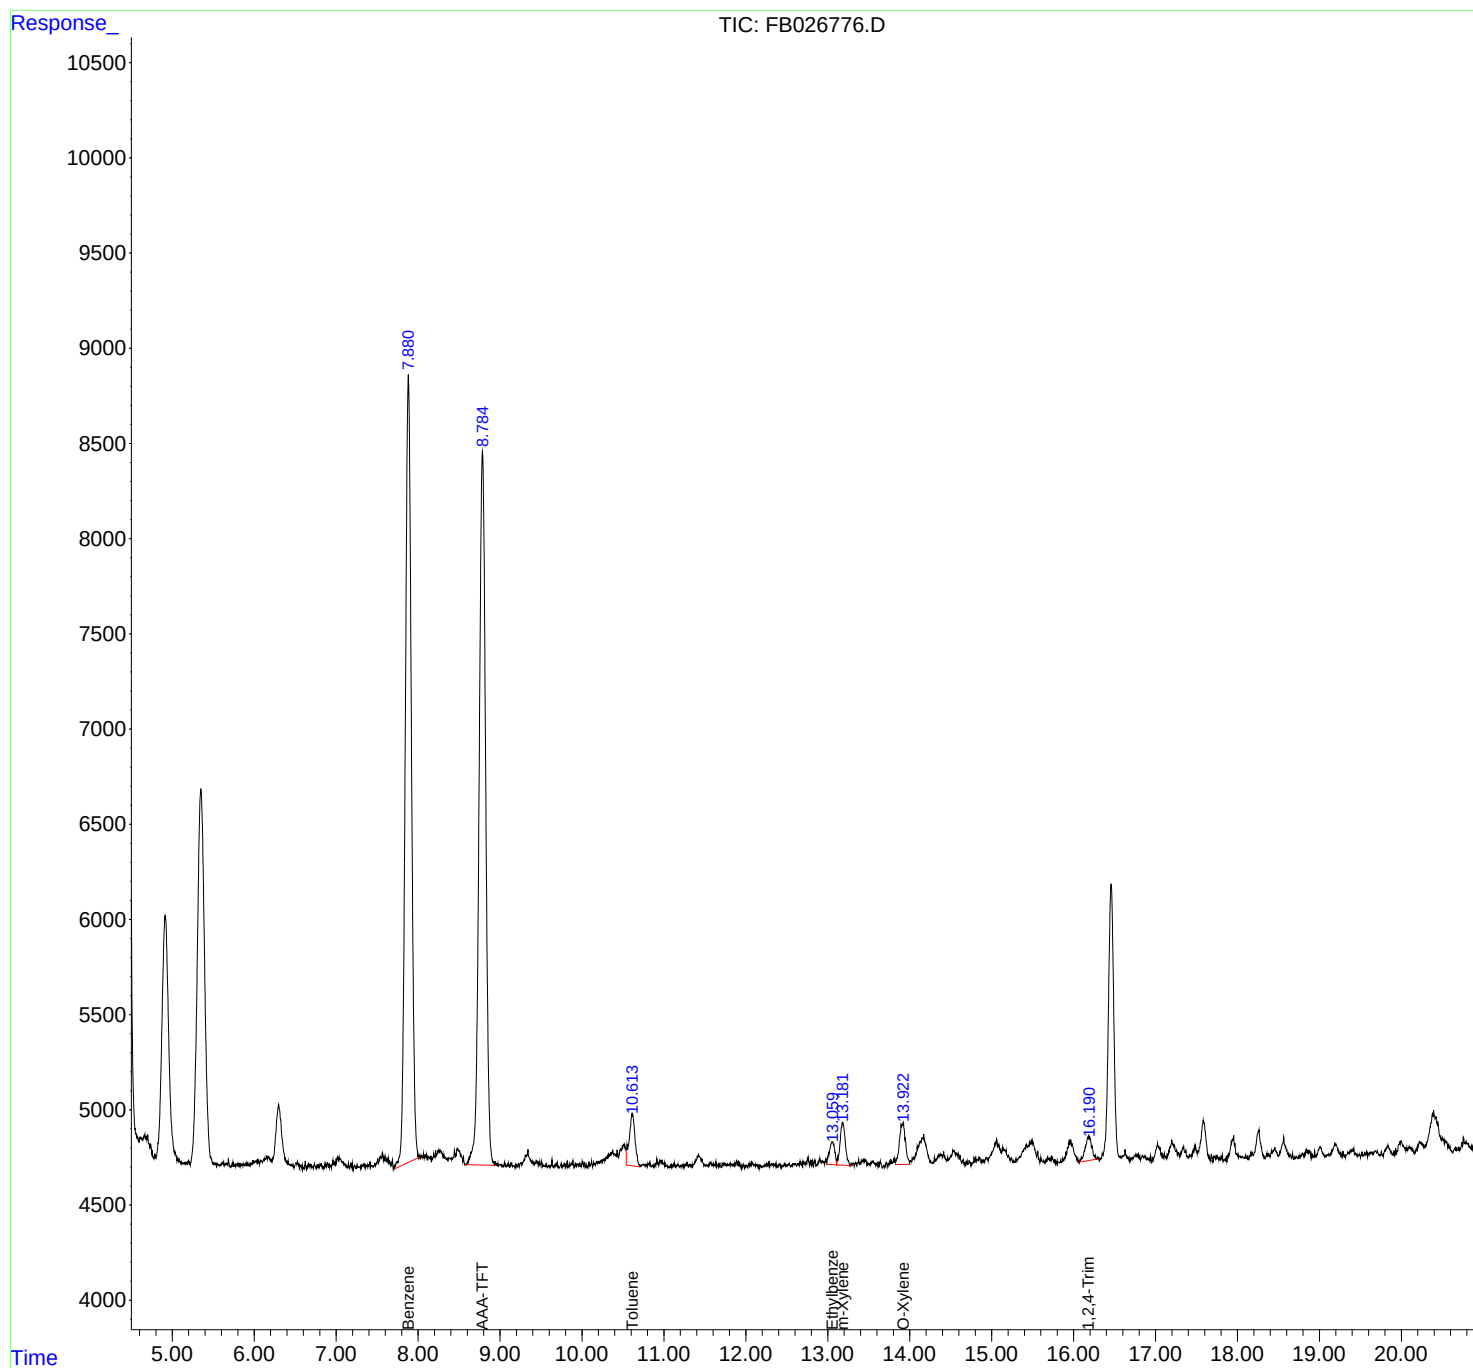


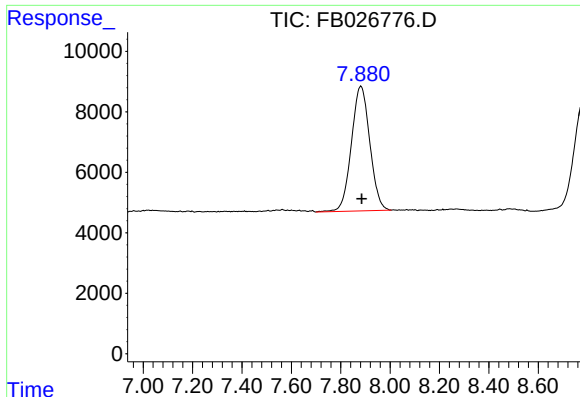

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.004 min
Response: 213346
Conc: 9.25 ng/ml

Instrument :
FID_B
ClientSampleId :

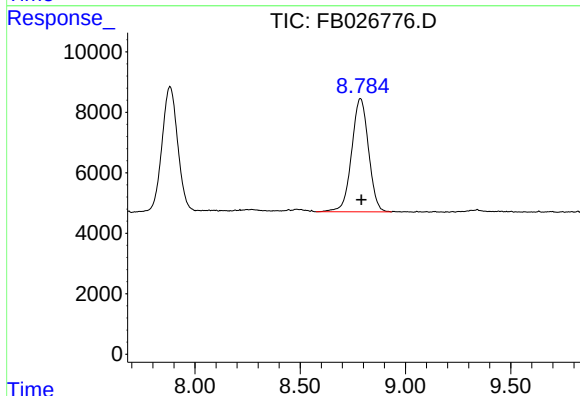


#5 AAA-TFT

R.T.: 8.786 min
Delta R.T.: -0.006 min
Response: 208802
Conc: 19.90 ng/ml

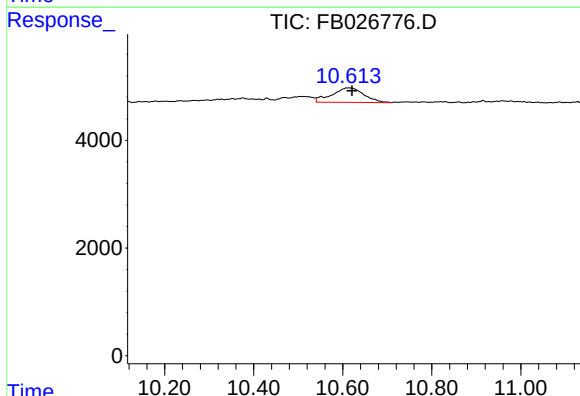


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.007 min
Response: 13395
Conc: 0.61 ng/ml

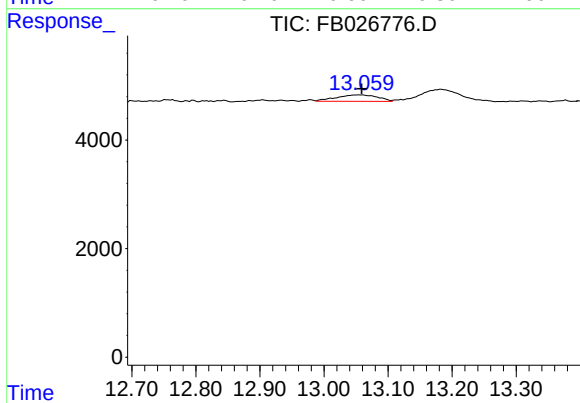

#7 Ethylbenzene


R.T.: 13.058 min
Delta R.T.: -0.001 min
Response: 5312
Conc: 0.26 ng/ml

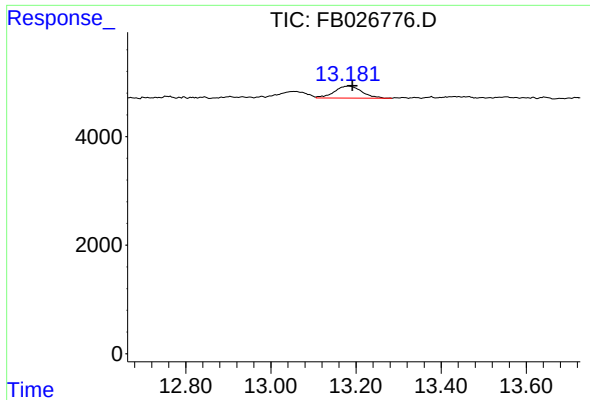

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.008 min
Response: 9897
Conc: 0.49 ng/ml

Instrument :
FID_B
ClientSampleId :

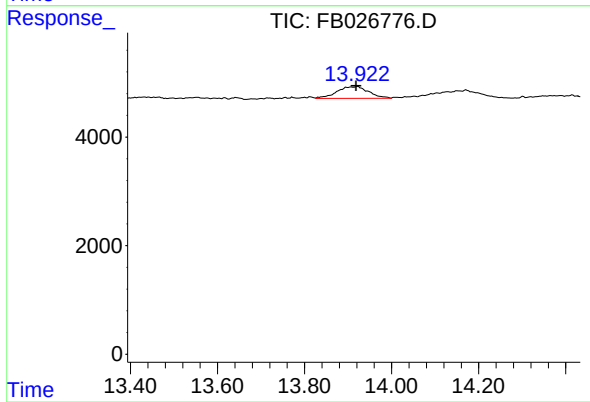

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.003 min
Response: 10990
Conc: 0.55 ng/ml

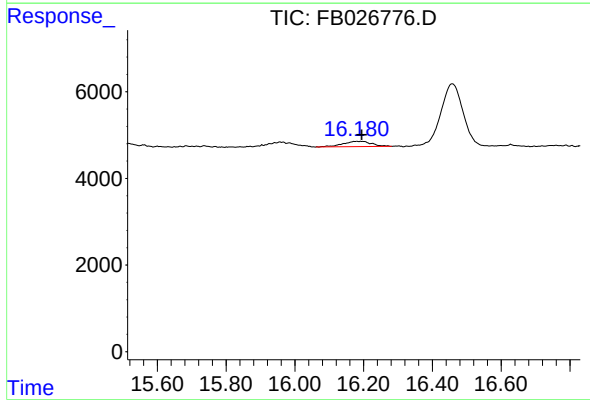

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: -0.013 min
Response: 7006
Conc: 0.35 ng/ml