

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
 Data File : FBCCCC70.D
 Signal(s) : FID2B.CH
 Acq On : 22 Mar 2022 21:58
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 23 02:38:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	220839	21.045 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	491866	25.979 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	569309	27.467 ng/ml
3) t n-Heptane	7.747	171089	8.644 ng/ml
4) t Benzene	7.883	232049	10.056 ng/ml
6) t Toluene	10.616	653577	29.854 ng/ml
7) t Ethylbenzene	13.053	200536	9.978 ng/ml
8) t m-Xylene	13.185	401318	19.914 ng/ml
9) t O-Xylene	13.912	398829	19.991 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	400807	20.116 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FBCCCC70.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 21:58
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 02:38:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

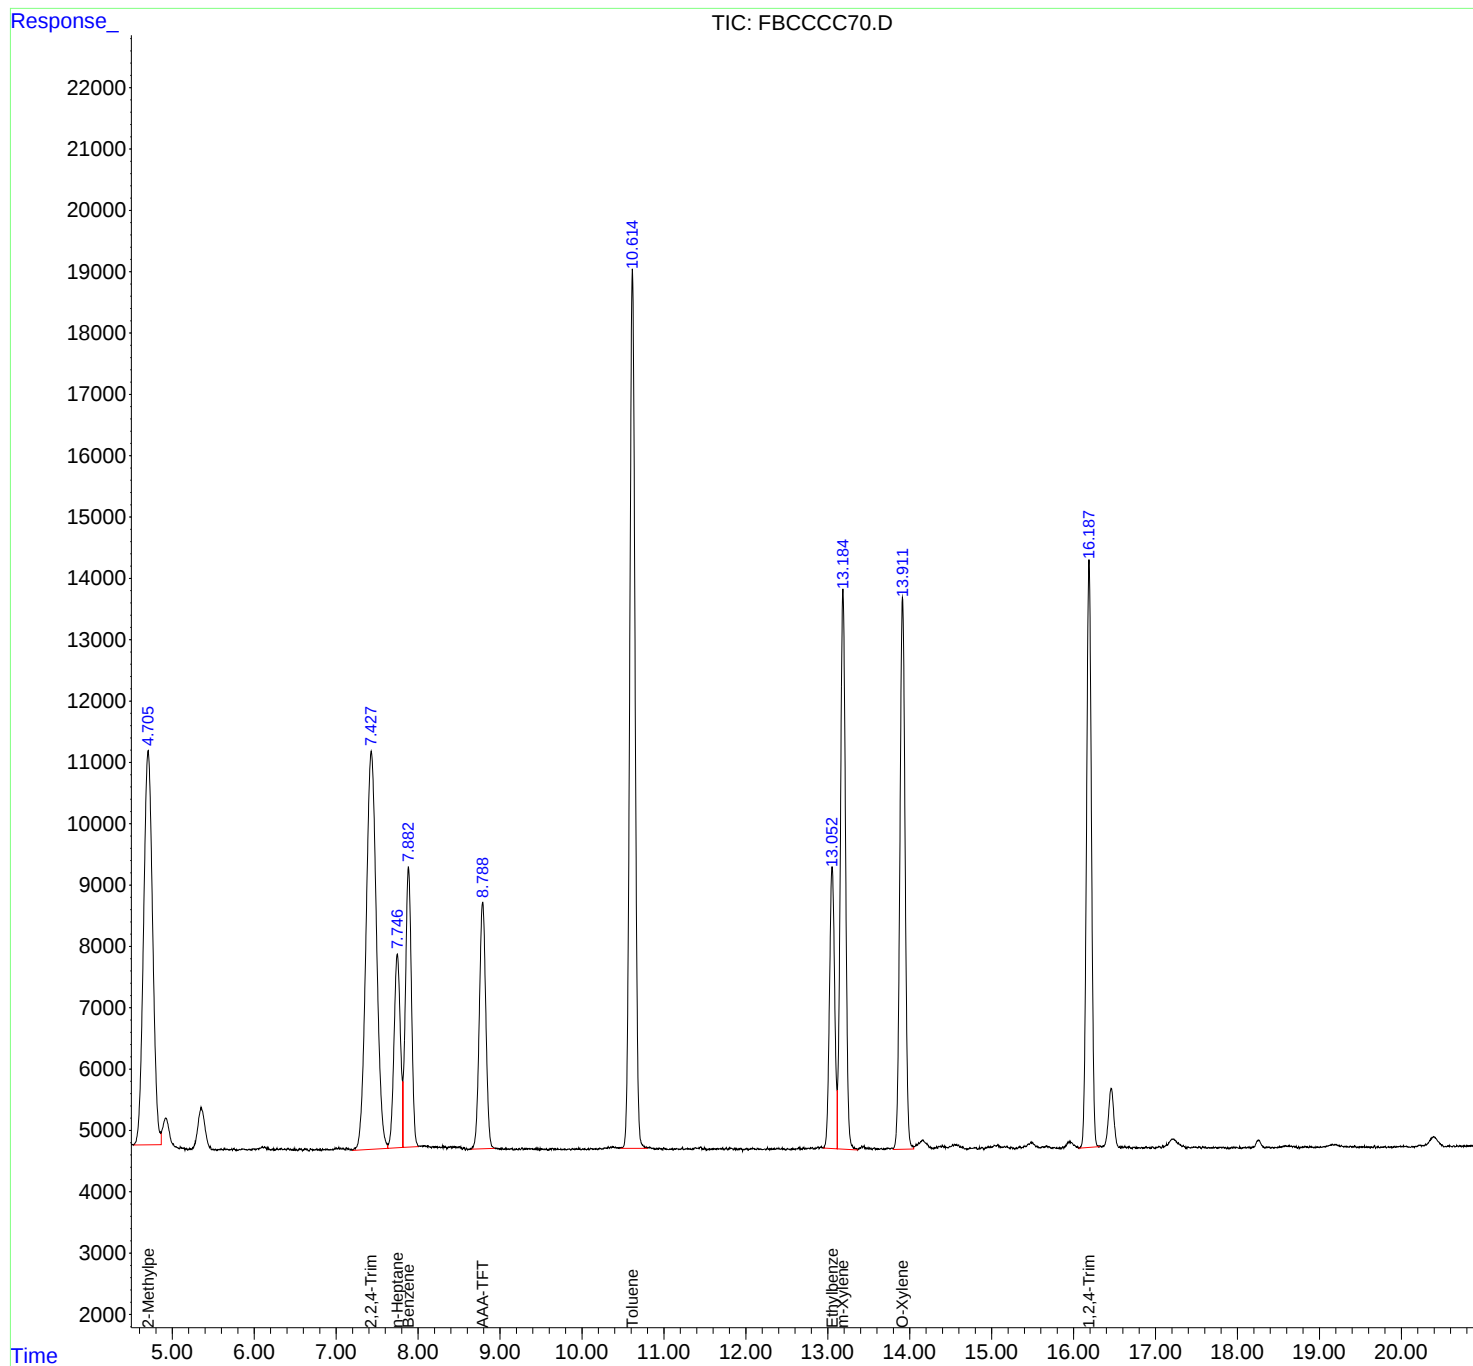


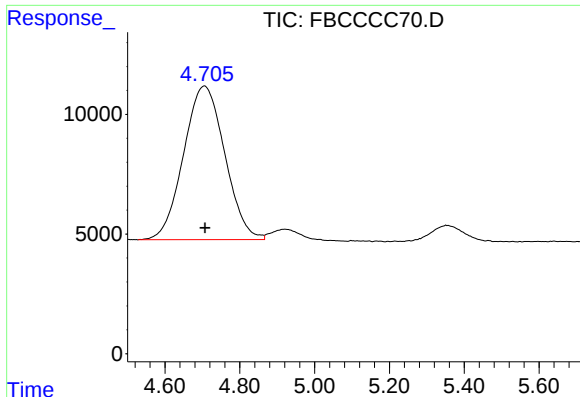

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 491866
Conc: 25.98 ng/ml

Instrument :
FID_B
ClientSampleId :

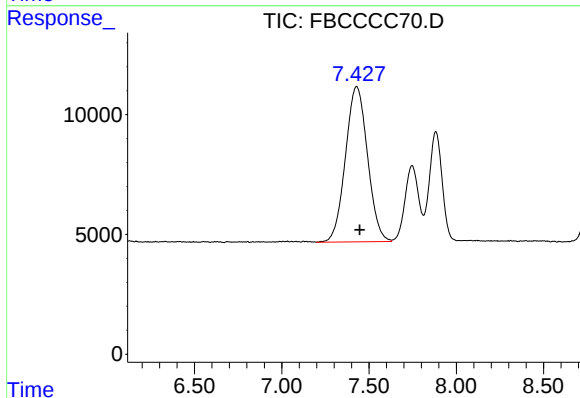


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.018 min
Response: 569309
Conc: 27.47 ng/ml

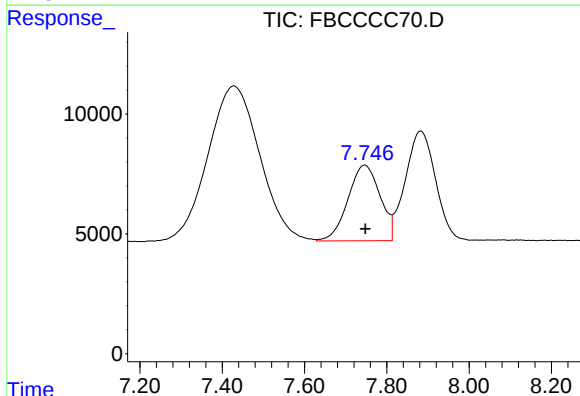


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.001 min
Response: 171089
Conc: 8.64 ng/ml

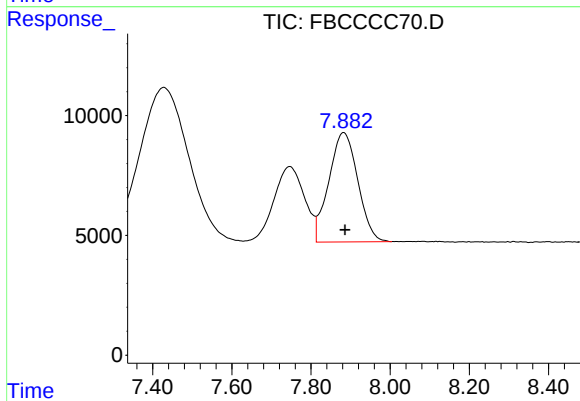

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 232049
Conc: 10.06 ng/ml

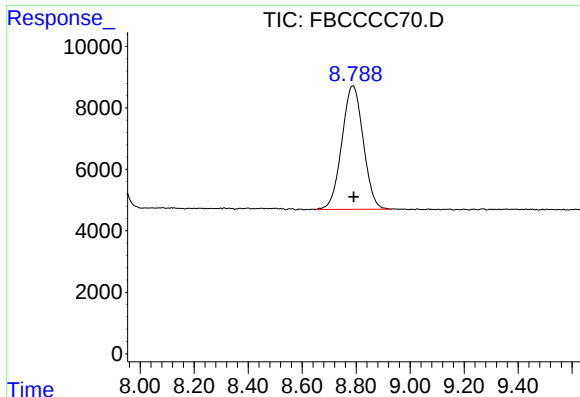

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 220839
Conc: 21.05 ng/ml

Instrument :
FID_B
ClientSampleId :

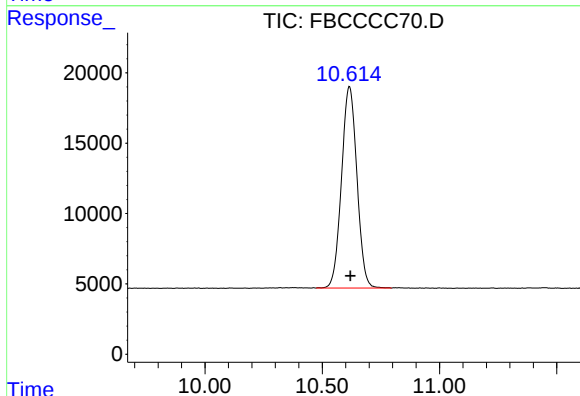


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 653577
Conc: 29.85 ng/ml

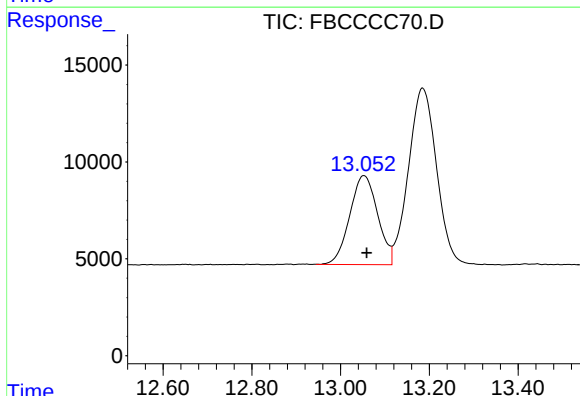


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 200536
Conc: 9.98 ng/ml

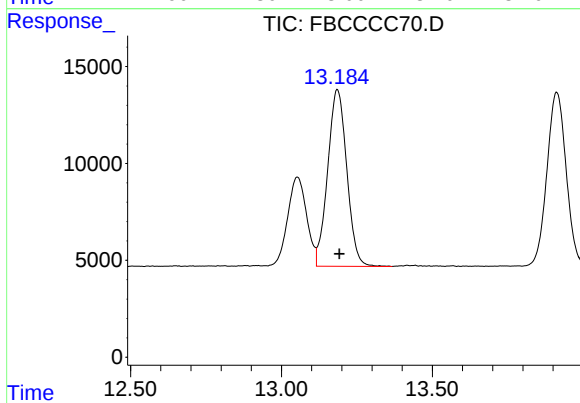

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 401318
Conc: 19.91 ng/ml

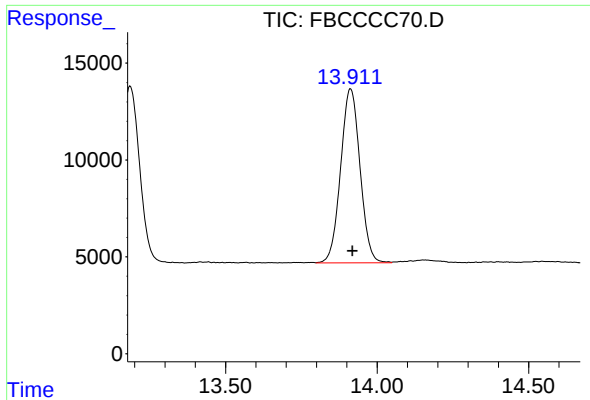

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.006 min
Response: 398829
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :

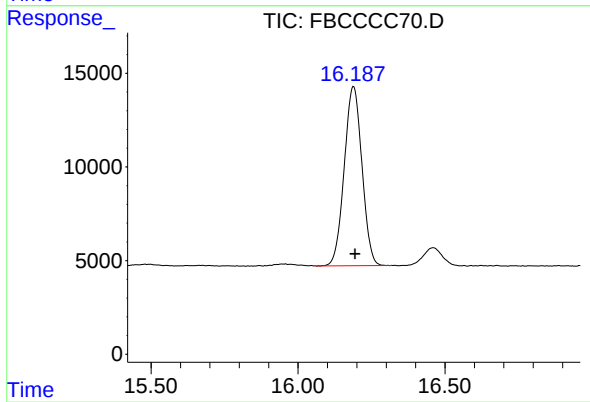

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 400807
Conc: 20.12 ng/ml