

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
 Data File : FB026760.D
 Signal(s) : FID2B.CH
 Acq On : 22 Mar 2022 15:35
 Operator : AJ/MA
 Sample : BSF0322S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0322S1

Integration File: Calibration.e
 Quant Time: Mar 23 02:37:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	209914	20.004 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	482519	25.485 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	562373	27.132 ng/ml
3) t n-Heptane	7.747	162261	8.198 ng/ml
4) t Benzene	7.884	215140	9.324 ng/ml
6) t Toluene	10.617	608722	27.805 ng/ml
7) t Ethylbenzene	13.054	191880	9.547 ng/ml
8) t m-Xylene	13.187	378277	18.771 ng/ml
9) t O-Xylene	13.913	376289	18.862 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	392740	19.711 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026760.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 15:35
Operator : AJ/MA
Sample : BSF0322S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0322S1

Integration File: Calibration.e
Quant Time: Mar 23 02:37:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

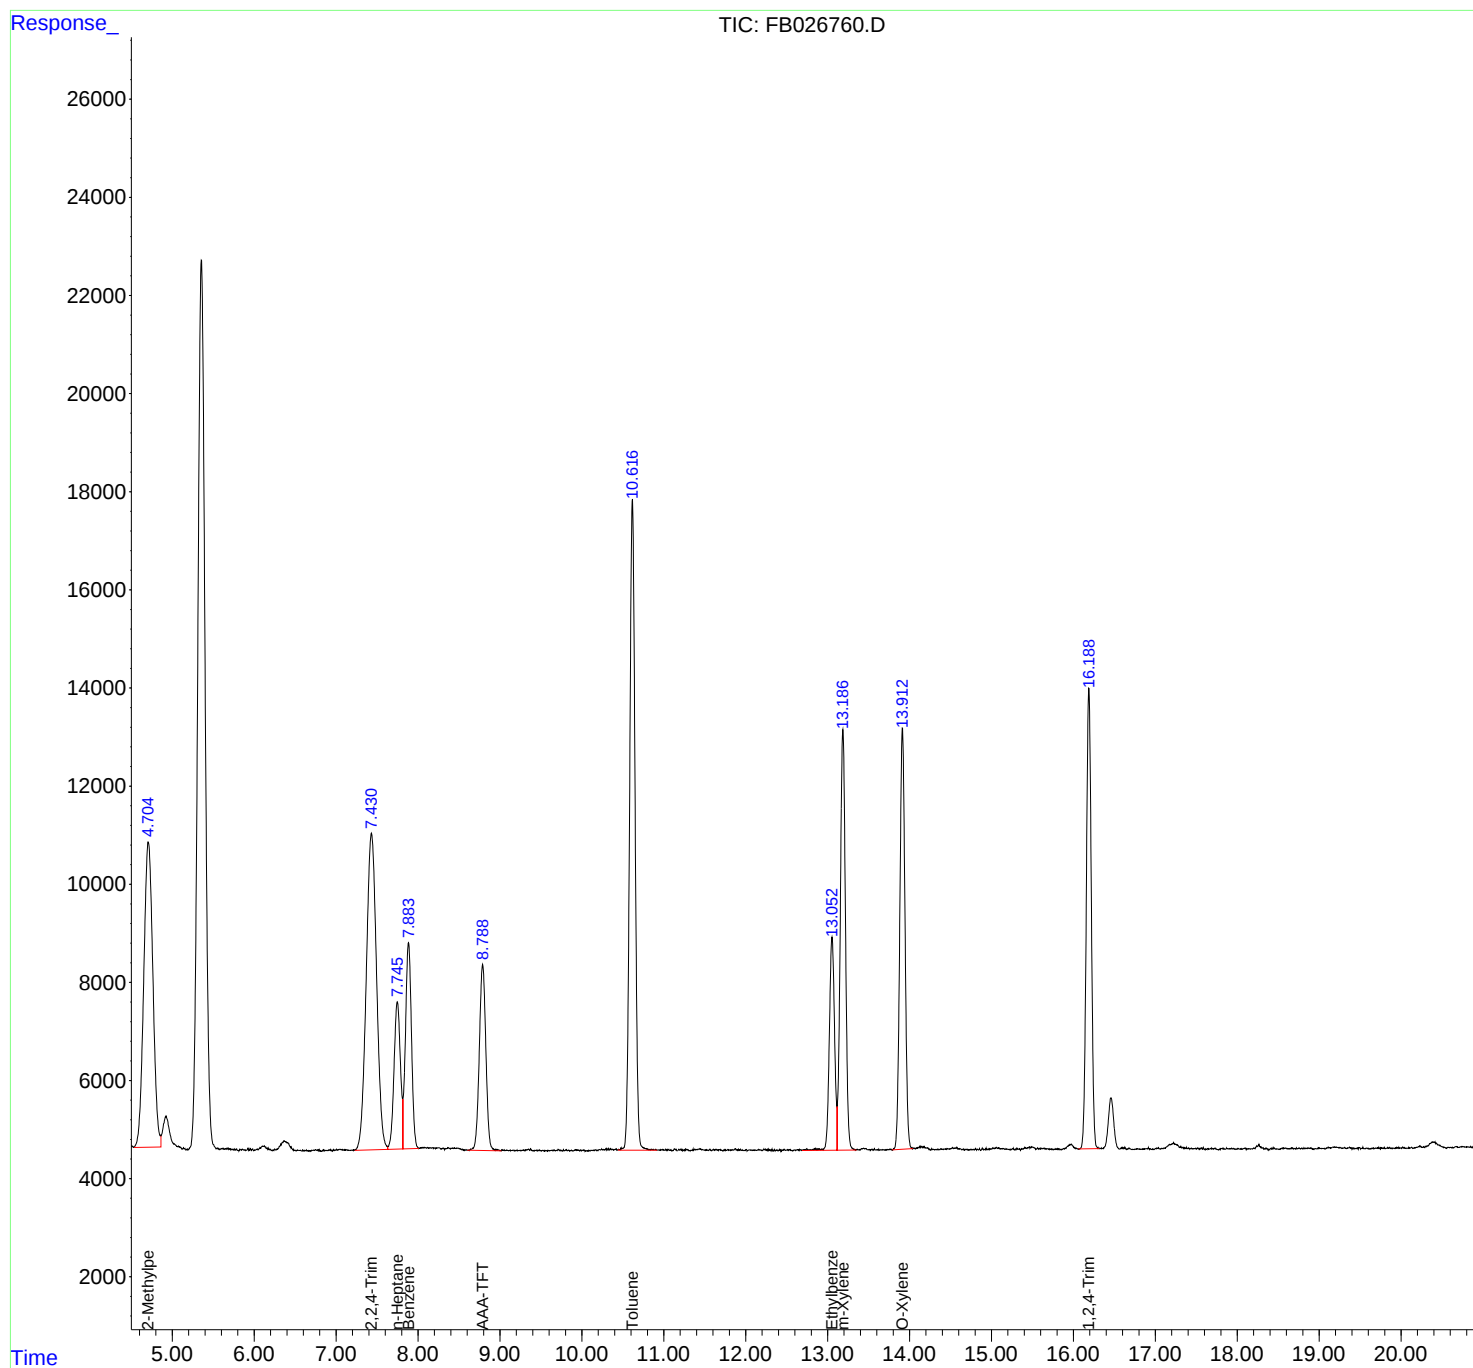


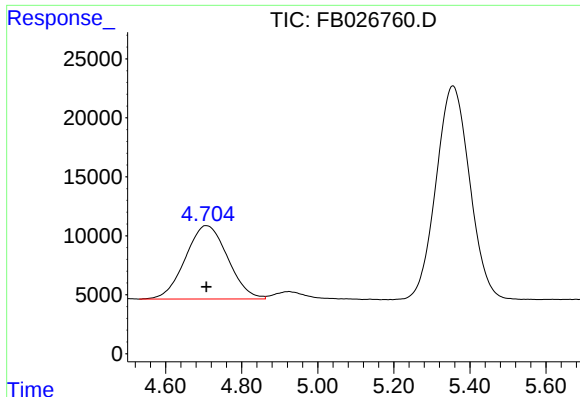

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 482519
Conc: 25.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0322S1

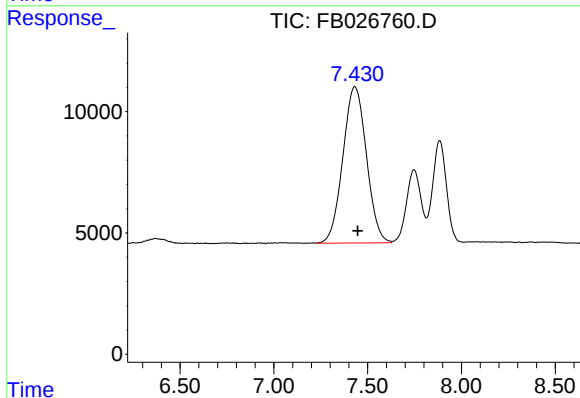


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: -0.015 min
Response: 562373
Conc: 27.13 ng/ml

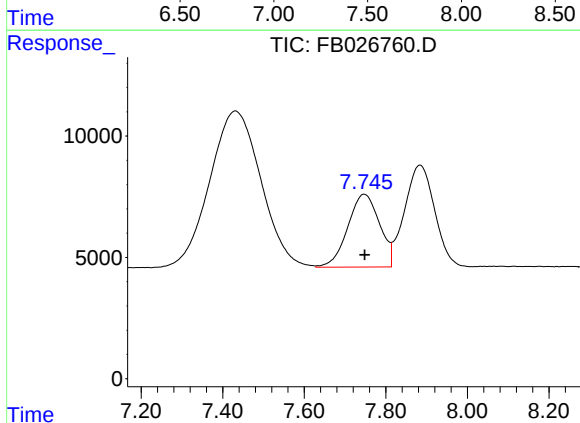


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 162261
Conc: 8.20 ng/ml

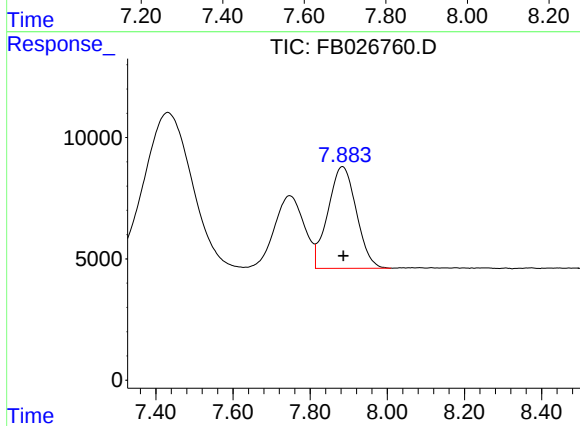

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.001 min
Response: 215140
Conc: 9.32 ng/ml

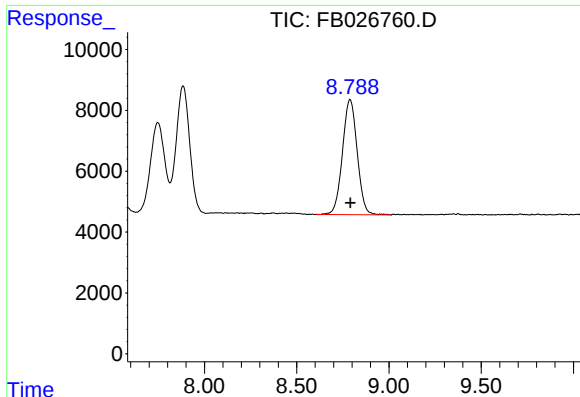

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 209914
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0322S1

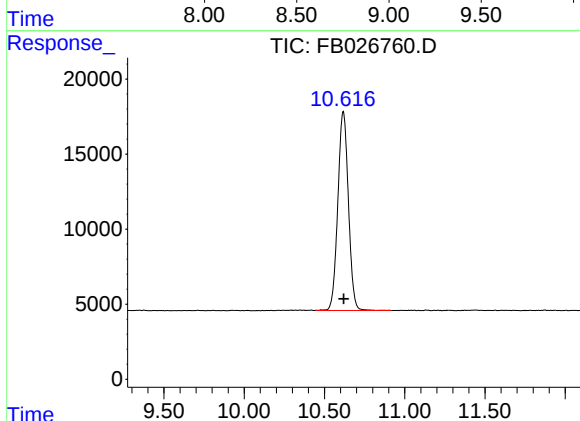


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 608722
Conc: 27.80 ng/ml

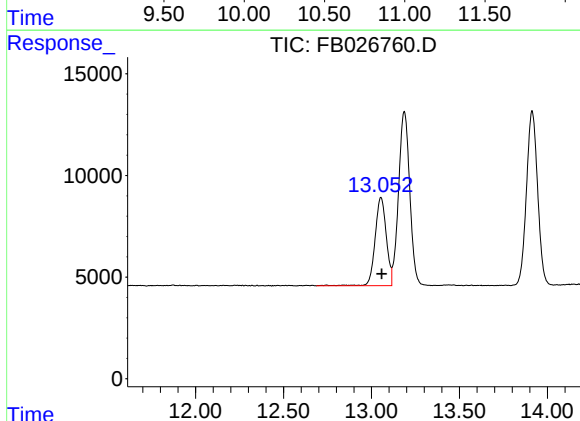


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 191880
Conc: 9.55 ng/ml

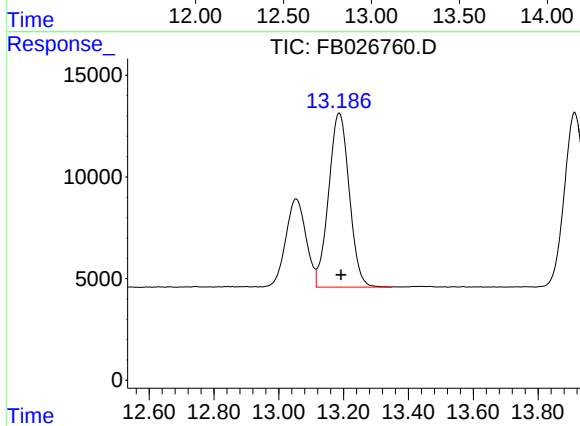

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 378277
Conc: 18.77 ng/ml

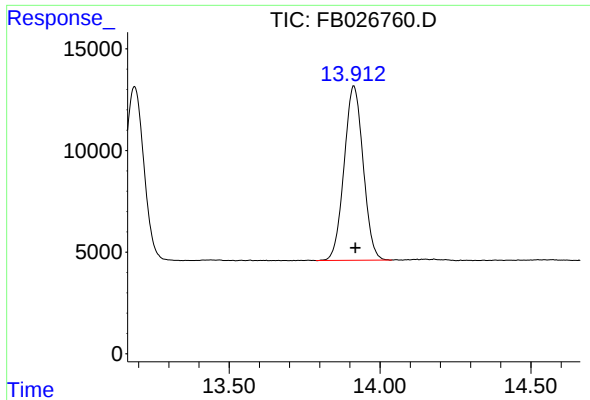

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 376289
Conc: 18.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0322S1

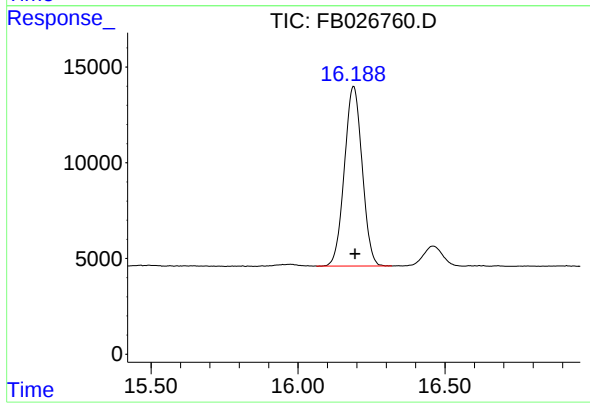

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 392740
Conc: 19.71 ng/ml