

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026763.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 17:29
Operator : AJ/MA
Sample : N1974-06
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-6-4-6-7

Integration File: Calibration.e
Quant Time: Mar 23 02:37:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	197674	18.838 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026763.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 17:29
Operator : AJ/MA
Sample : N1974-06
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-6-4-6-7

Integration File: Calibration.e
Quant Time: Mar 23 02:37:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

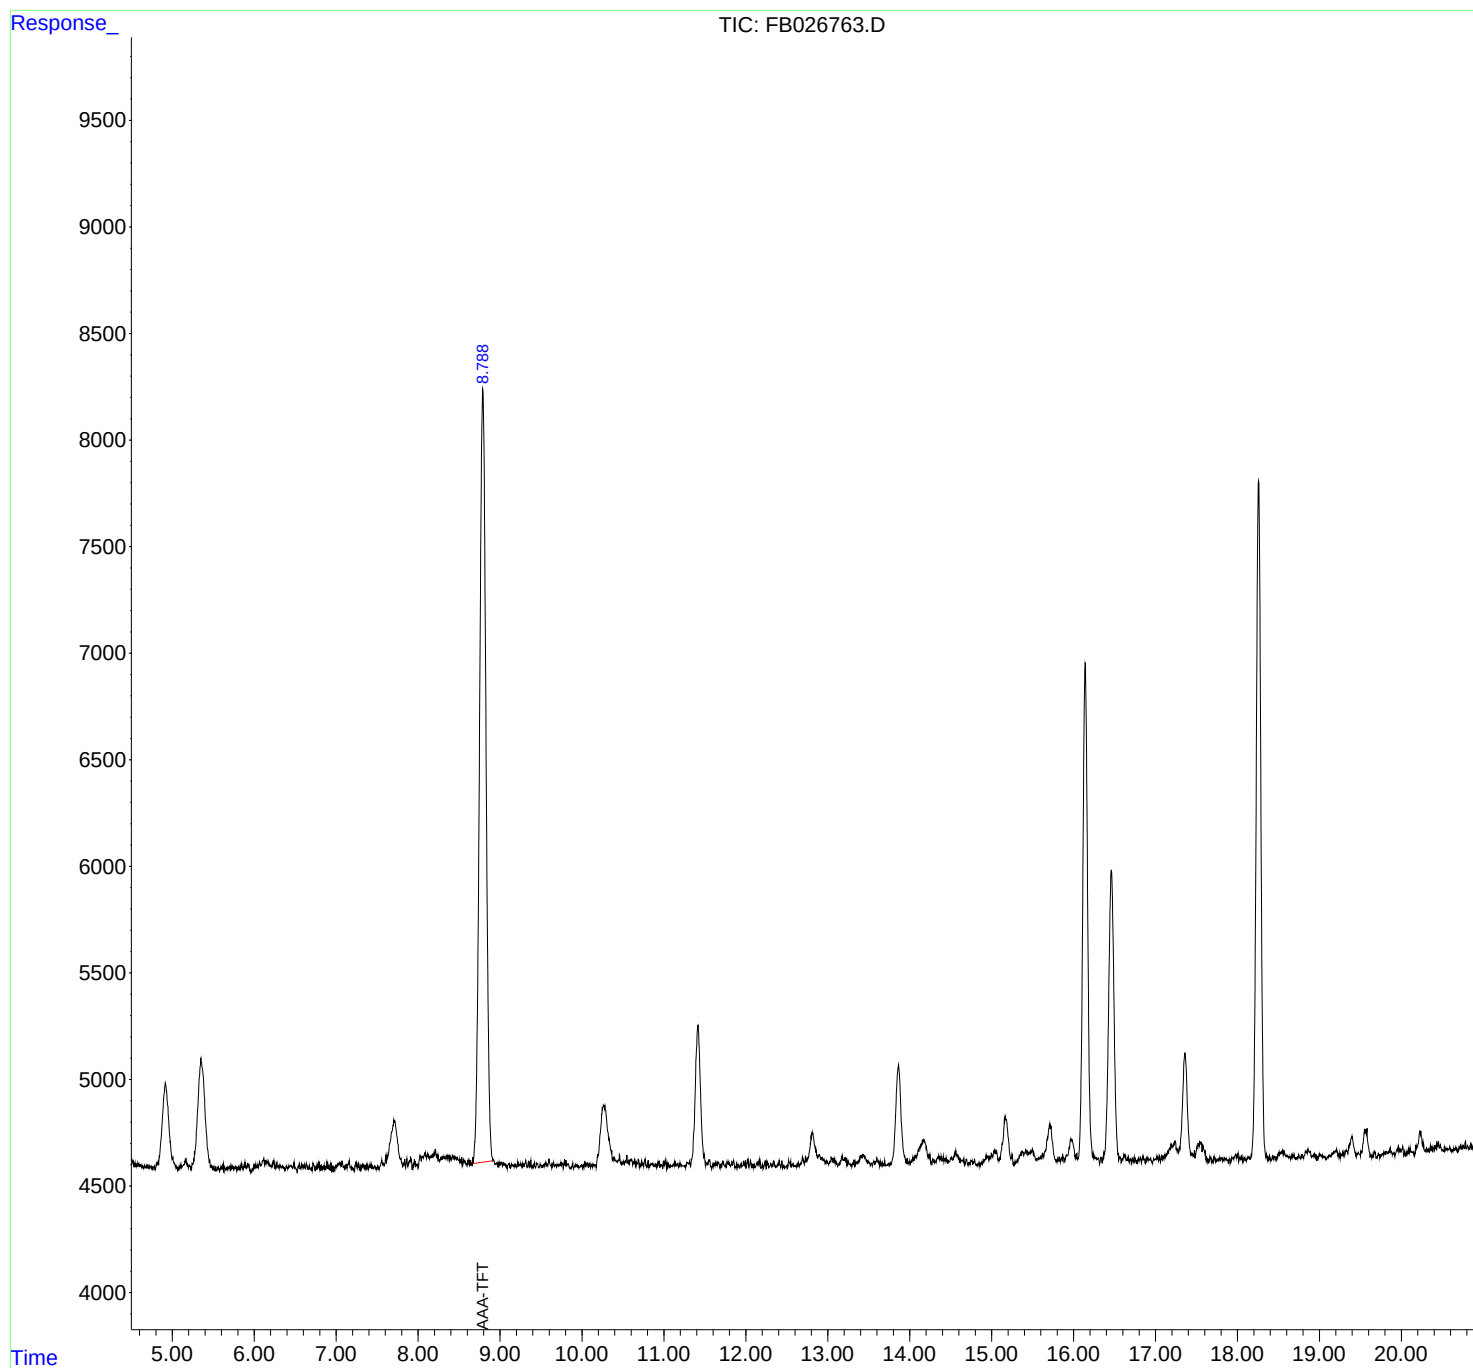

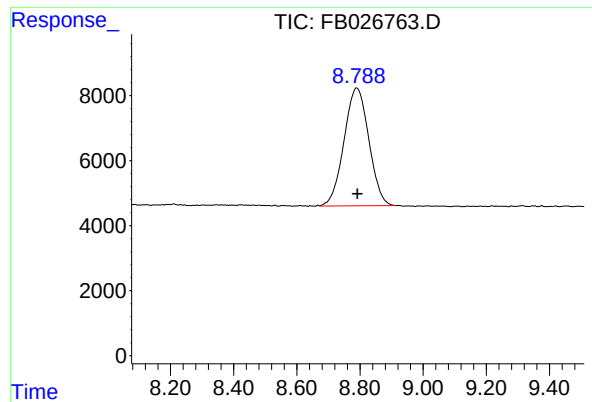

#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 197674
Conc: 18.84 ng/ml

Instrument :

FID_B

ClientSampleId :

G-6-4-6-7