

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB032222\  
Data File : FB026766.D  
Signal(s) : FID2B.CH  
Acq On : 22 Mar 2022 19:25  
Operator : AJ/MA  
Sample : N1994-11  
Misc : 5.06G/5.00 ML DI WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-04-COMP

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/23/2022  
Supervised By :Sohil Jodhani 03/23/2022

Integration File: Calibration.e  
Quant Time: Mar 23 02:37:59 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030822.M  
Quant Title :  
QLast Update : Fri Mar 11 13:08:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.794 | 18324    | 1.746 ng/mlm |
| Target Compounds            |       |          |              |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB032222\  
Data File : FB026766.D  
Signal(s) : FID2B.CH  
Acq On : 22 Mar 2022 19:25  
Operator : AJ/MA  
Sample : N1994-11  
Misc : 5.06G/5.00 ML DI WATER  
ALS Vial : 10 Sample Multiplier: 1


Instrument :  
FID\_B  
ClientSampleId :  
SB-04-COMP


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/23/2022  
Supervised By :Sohil Jodhani 03/23/2022

Integration File: Calibration.e  
Quant Time: Mar 23 02:37:59 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030822.M  
Quant Title :  
QLast Update : Fri Mar 11 13:08:49 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

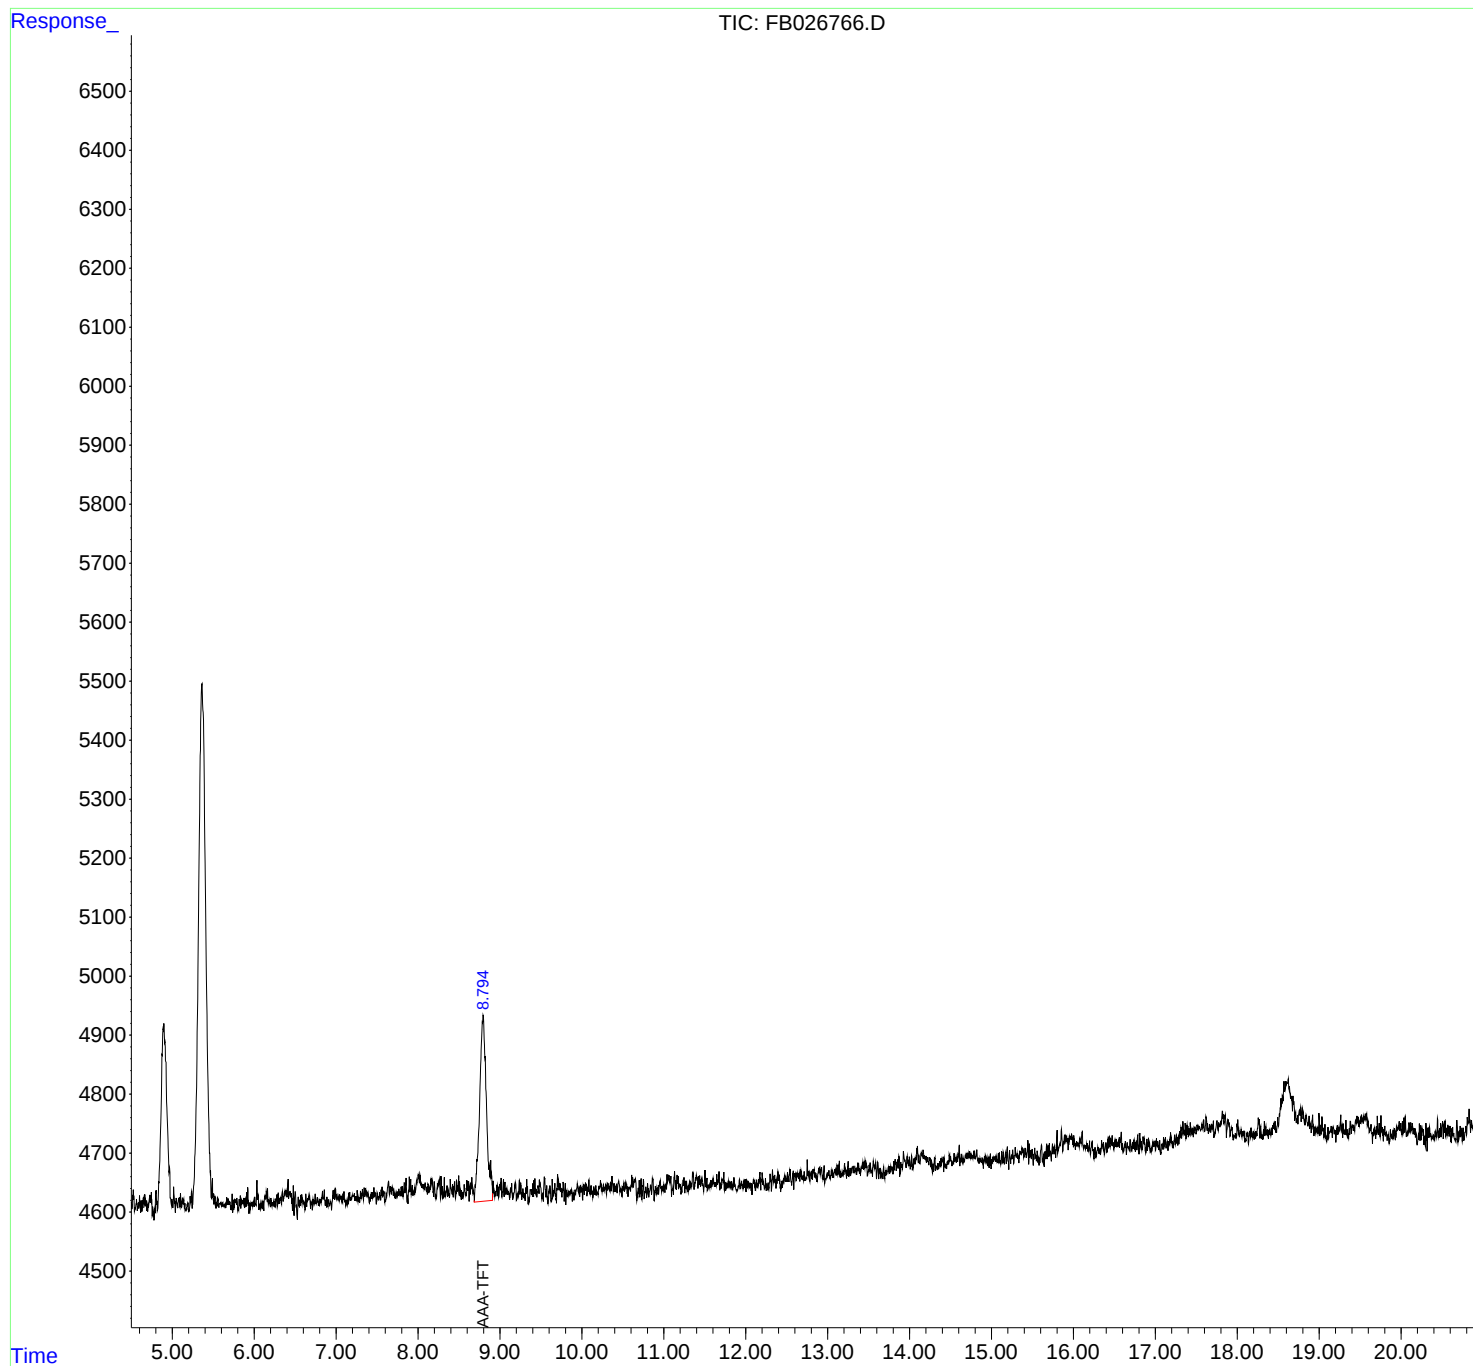

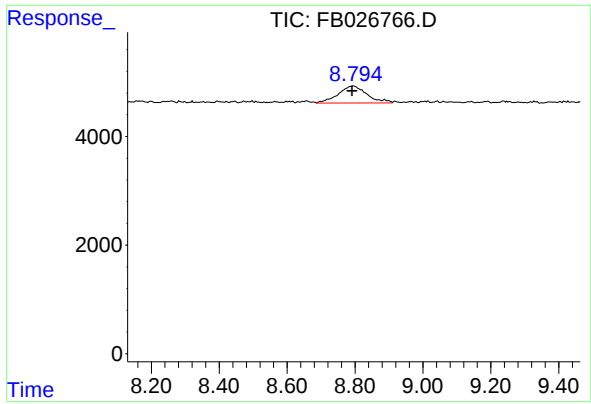

#5 AAA-TFT

R.T.: 8.794 min  
Delta R.T.: 0.003 min  
Response: 18324  
Conc: 1.75 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
SB-04-COMP

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/23/2022  
Supervised By :Sohil Jodhani 03/23/2022