

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
 Data File : FB026768.D
 Signal(s) : FID2B.CH
 Acq On : 22 Mar 2022 20:41
 Operator : AJ/MA
 Sample : N1974-06MSD
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G-6-4-6-7MSD

Integration File: Calibration.e
 Quant Time: Mar 23 02:38:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	241661	23.030 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	440916	23.288 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	517487	24.966 ng/ml
3) t n-Heptane	7.747	155113	7.837 ng/ml
4) t Benzene	7.884	217834	9.440 ng/ml
6) t Toluene	10.616	624739	28.536 ng/ml
7) t Ethylbenzene	13.053	190959	9.502 ng/ml
8) t m-Xylene	13.186	381099	18.911 ng/ml
9) t O-Xylene	13.913	376848	18.890 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	375349	18.839 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032222\
Data File : FB026768.D
Signal(s) : FID2B.CH
Acq On : 22 Mar 2022 20:41
Operator : AJ/MA
Sample : N1974-06MSD
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-6-4-6-7MSD

Integration File: Calibration.e
Quant Time: Mar 23 02:38:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

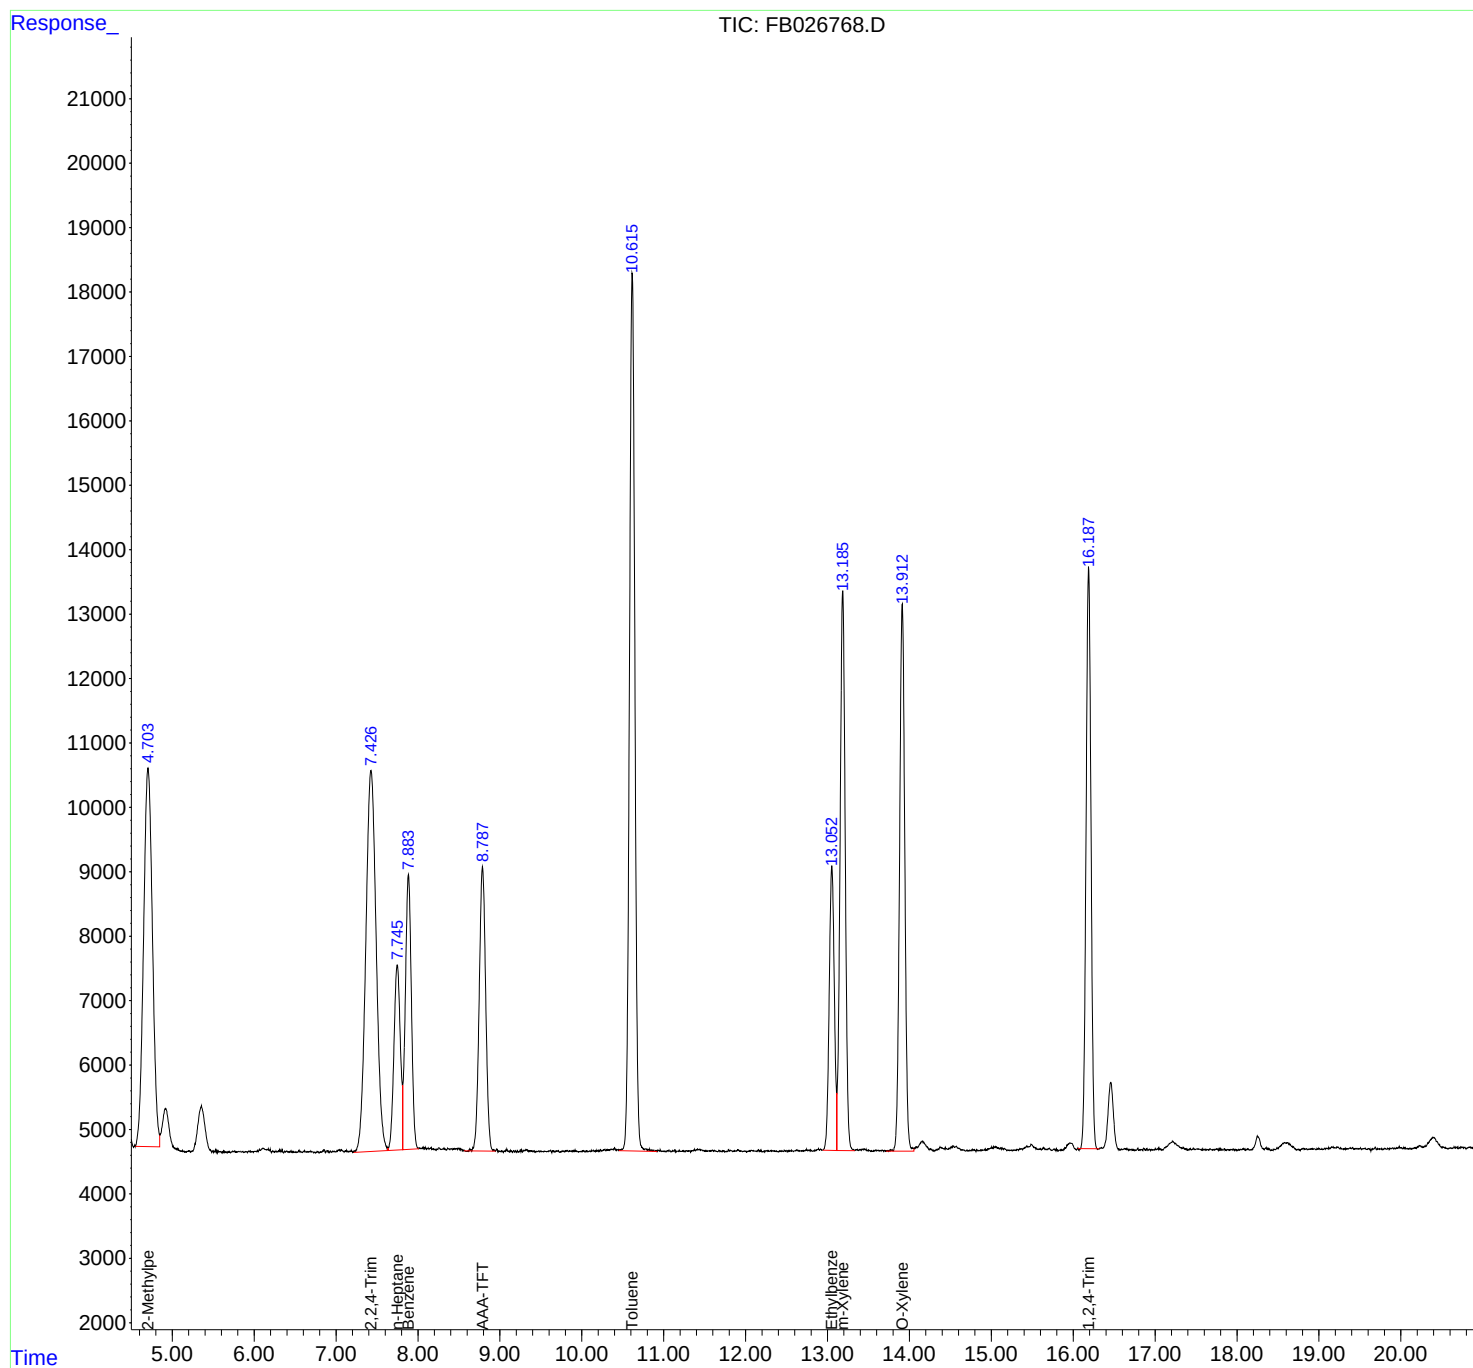


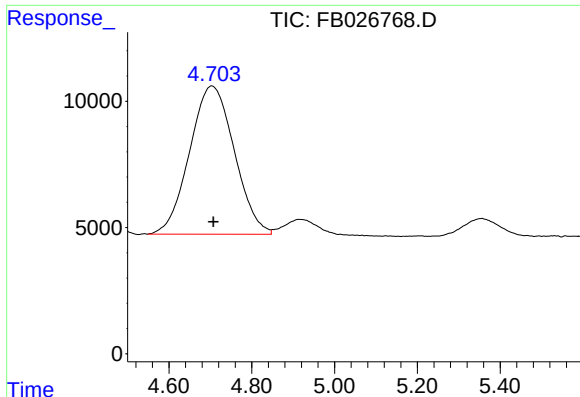

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 440916
Conc: 23.29 ng/ml

Instrument :
FID_B
ClientSampleId :
G-6-4-6-7MSD

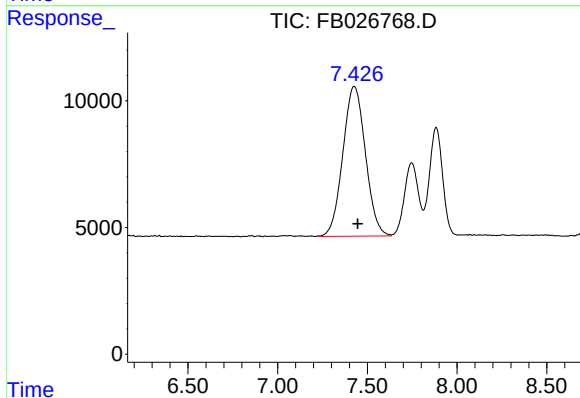


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.020 min
Response: 517487
Conc: 24.97 ng/ml

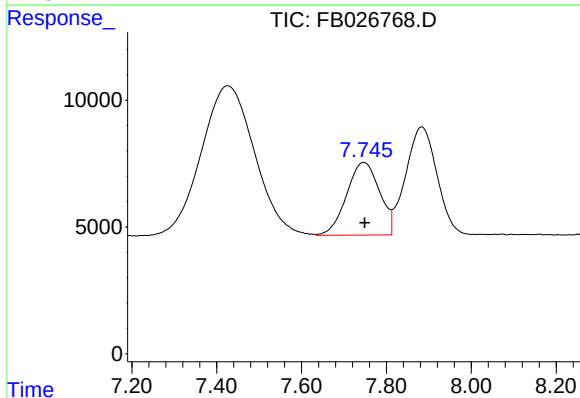


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 155113
Conc: 7.84 ng/ml

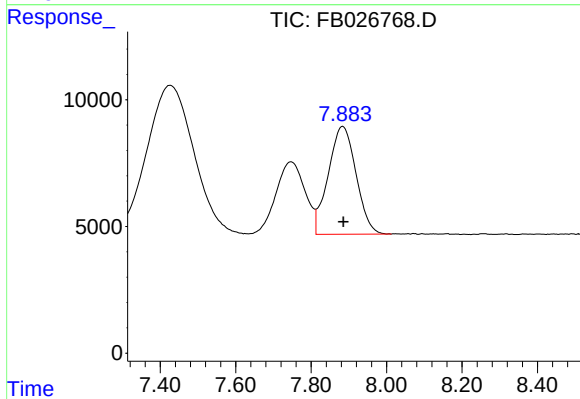

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 217834
Conc: 9.44 ng/ml

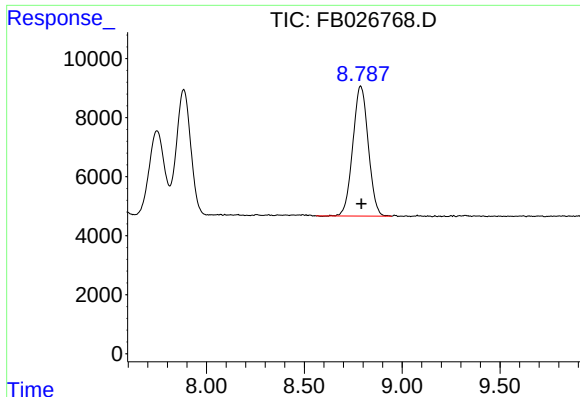

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 241661
Conc: 23.03 ng/ml

Instrument :
FID_B
ClientSampleId :
G-6-4-6-7MSD

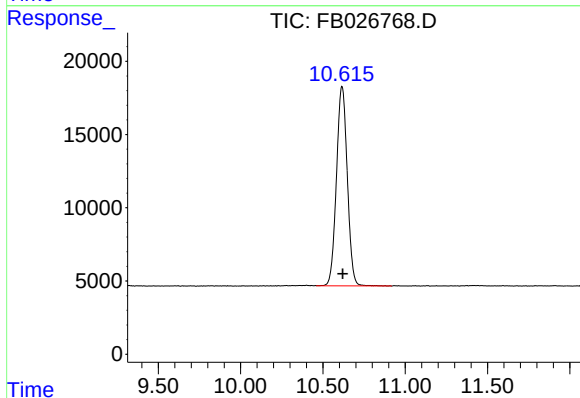


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 624739
Conc: 28.54 ng/ml

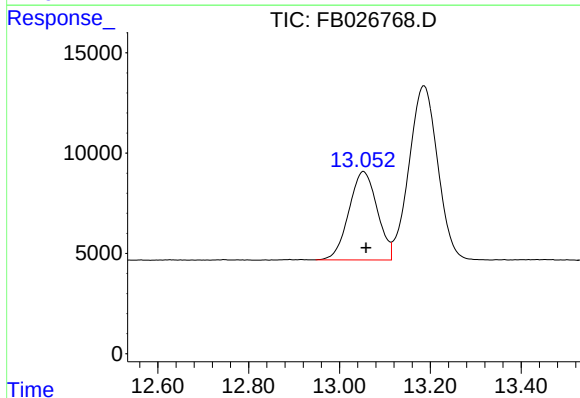


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 190959
Conc: 9.50 ng/ml

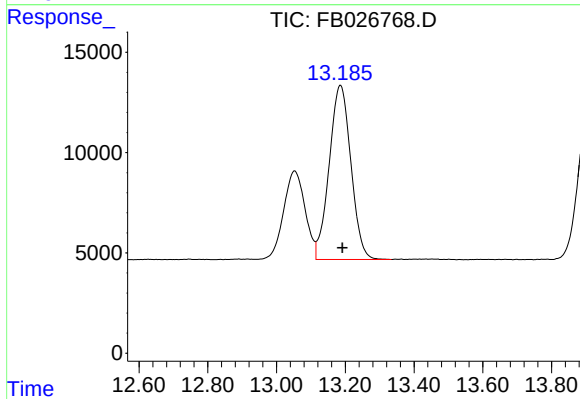

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 381099
Conc: 18.91 ng/ml

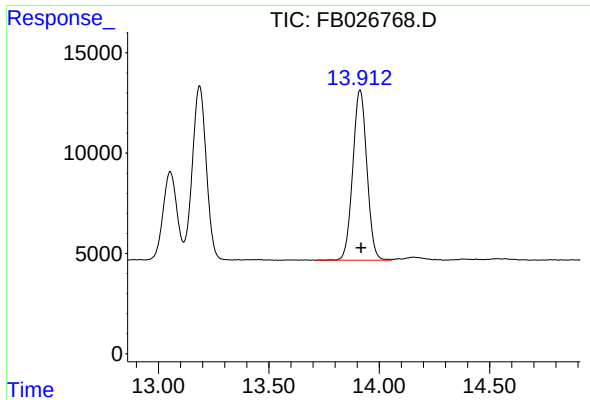

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 376848
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :
G-6-4-6-7MSD

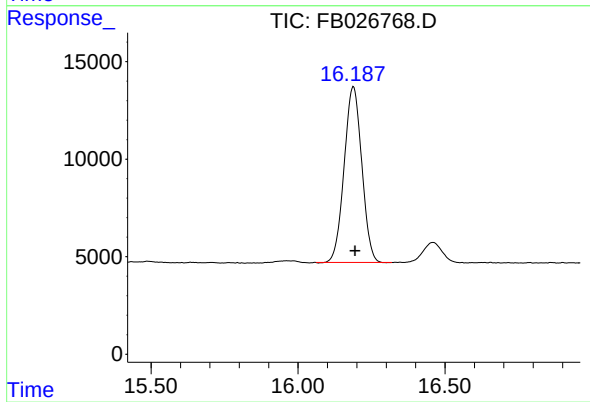

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.006 min
Response: 375349
Conc: 18.84 ng/ml