

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB032223\  
 Data File : FB029544.D  
 Signal(s) : FID2B.CH  
 Acq On : 22 Mar 2023 9:16  
 Operator : YP/AJ  
 Sample : BSF0322S1  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Mar 22 15:52:31 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030123.M  
 Quant Title :  
 QLast Update : Wed Mar 01 12:30:24 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
5) s AAA-TFT	8.790	222440	18.360 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	432352	28.177 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	516814	30.681 ng/ml
3) t n-Heptane	7.748	164100	9.488 ng/ml
4) t Benzene	7.885	215803	10.632 ng/ml
6) t Toluene	10.618	627606	31.795 ng/ml
7) t Ethylbenzene	13.054	197374	10.602 ng/ml
8) t m-Xylene	13.187	390424	20.987 ng/ml
9) t O-Xylene	13.913	380564	20.668 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	370239	19.878 ng/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB032223\  
 Data File : FB029544.D  
 Signal(s) : FID2B.CH  
 Acq On : 22 Mar 2023 9:16  
 Operator : YP/AJ  
 Sample : BSF0322S1  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Mar 22 15:52:31 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030123.M  
 Quant Title :  
 QLast Update : Wed Mar 01 12:30:24 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

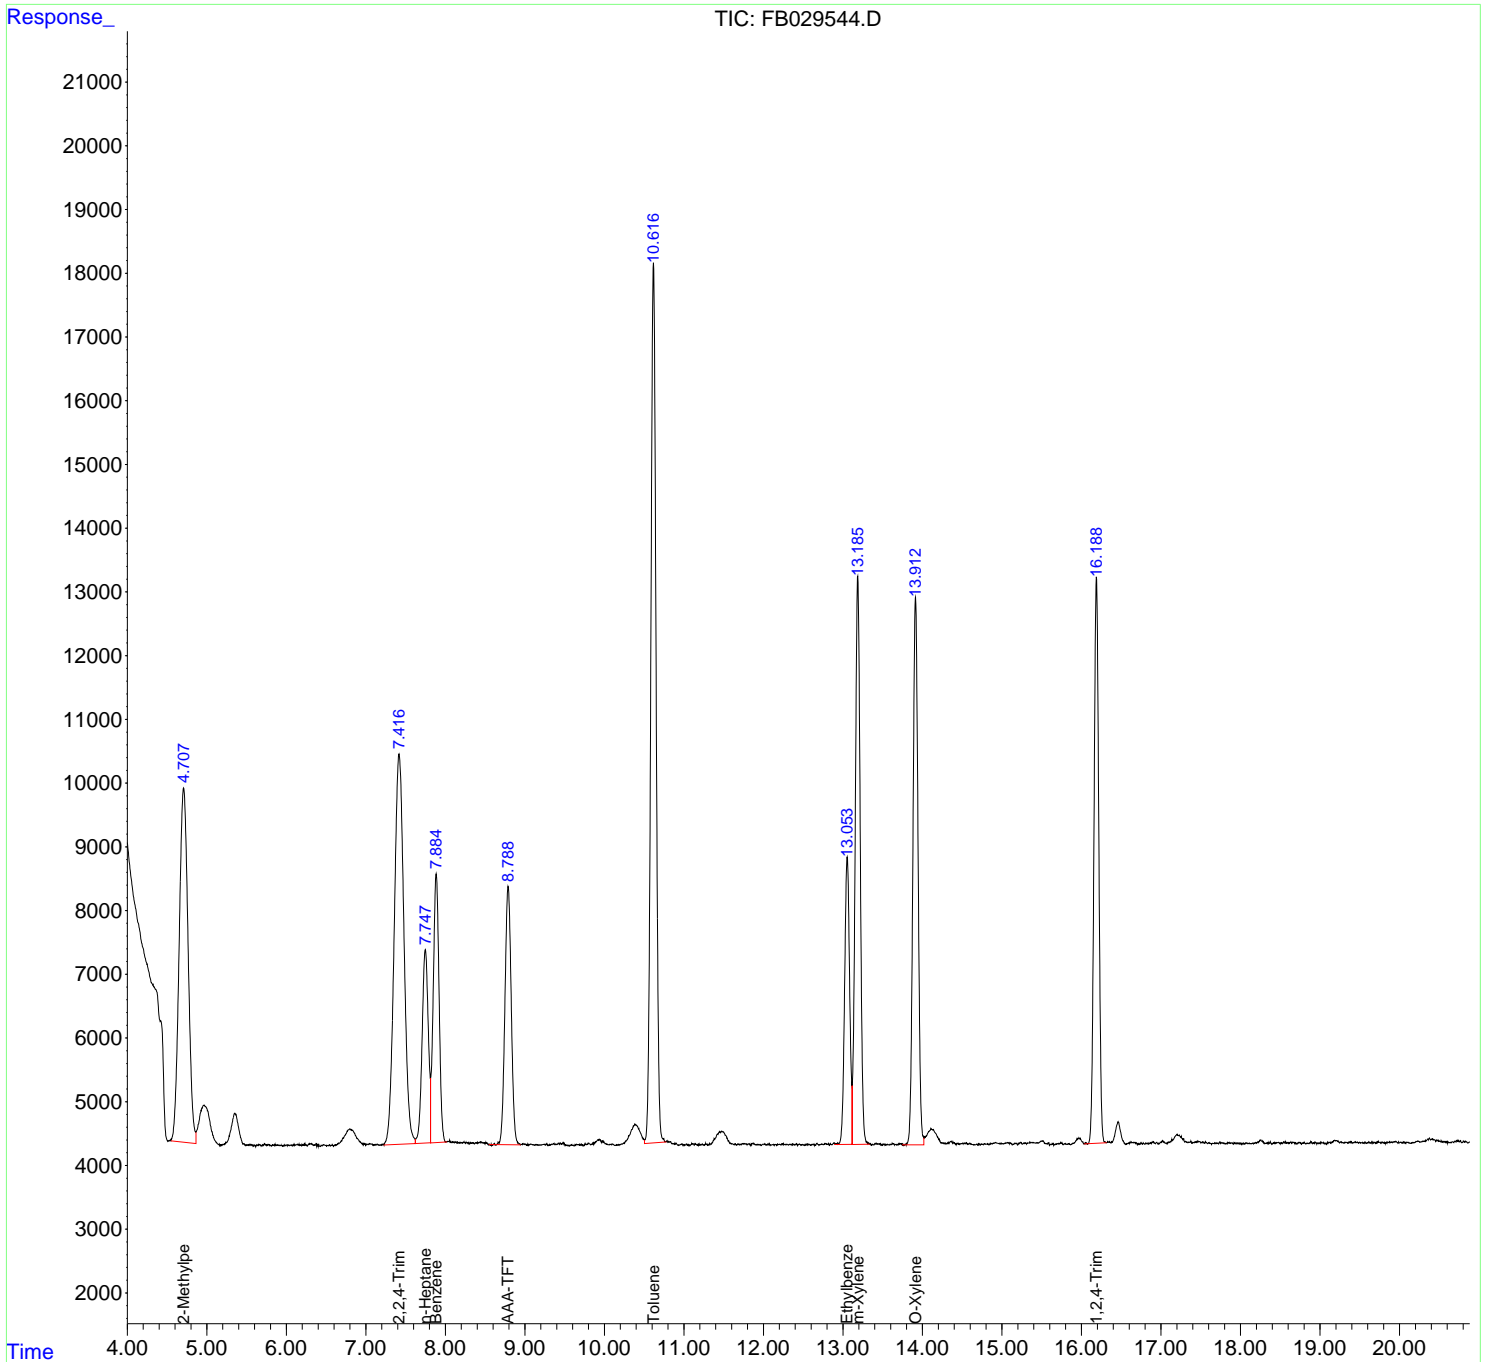


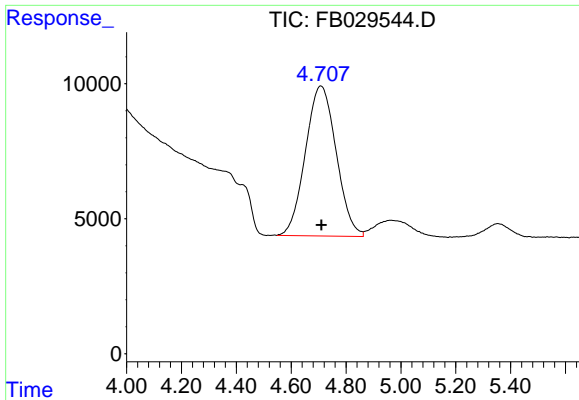

#1 2-Methylpentane


R.T.: 4.709 min  
 Delta R.T.: -0.001 min  
 Response: 432352  
 Conc: 28.18 ng/ml

Instrument :  
 FID\_B  
 ClientSampleId :

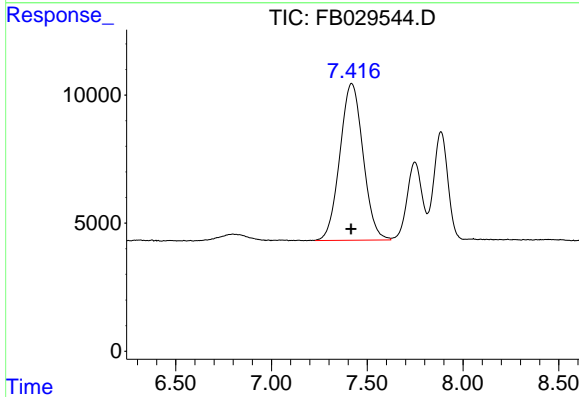


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min  
 Delta R.T.: 0.002 min  
 Response: 516814  
 Conc: 30.68 ng/ml

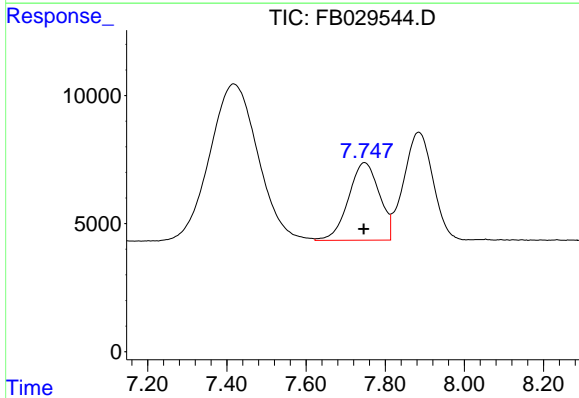


#3 n-Heptane

R.T.: 7.748 min  
 Delta R.T.: 0.002 min  
 Response: 164100  
 Conc: 9.49 ng/ml

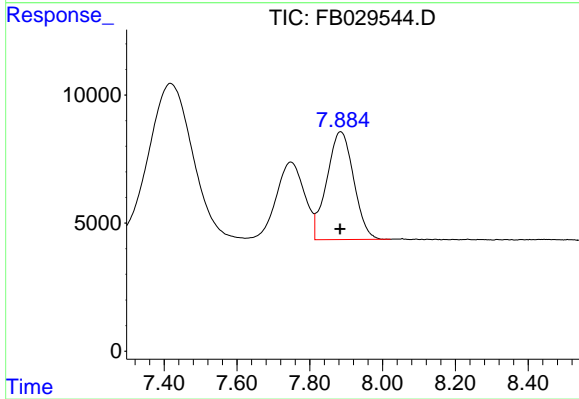

#4 Benzene


R.T.: 7.885 min  
 Delta R.T.: 0.002 min  
 Response: 215803  
 Conc: 10.63 ng/ml

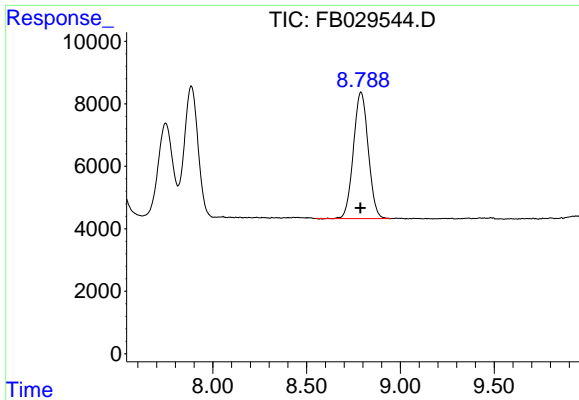

#5 AAA-TFT


R.T.: 8.790 min  
 Delta R.T.: 0.002 min  
 Response: 222440  
 Conc: 18.36 ng/ml

Instrument : FID\_B  
 ClientSampleId :

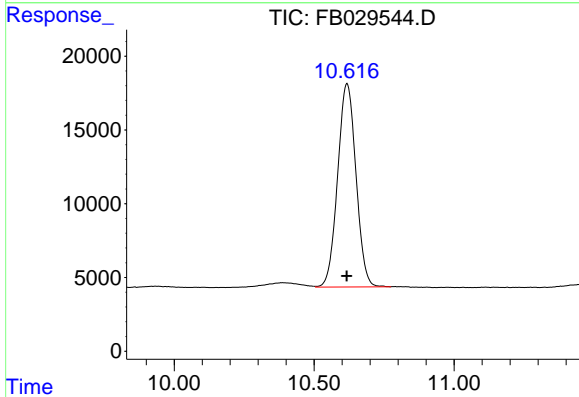


#6 Toluene

R.T.: 10.618 min  
 Delta R.T.: 0.002 min  
 Response: 627606  
 Conc: 31.80 ng/ml

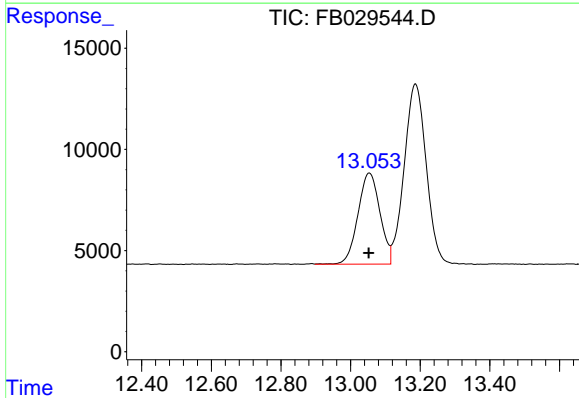


#7 Ethylbenzene

R.T.: 13.054 min  
 Delta R.T.: 0.001 min  
 Response: 197374  
 Conc: 10.60 ng/ml

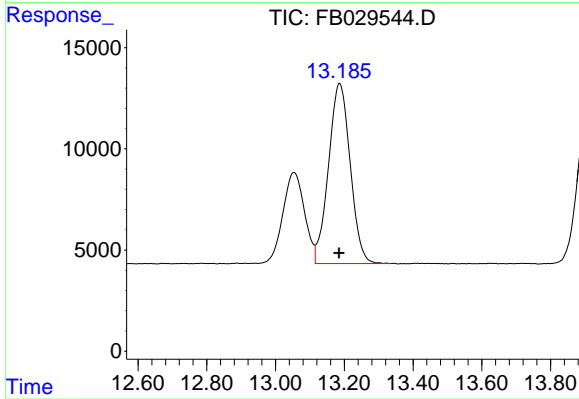

#8 m-Xylene


R.T.: 13.187 min  
 Delta R.T.: 0.002 min  
 Response: 390424  
 Conc: 20.99 ng/ml

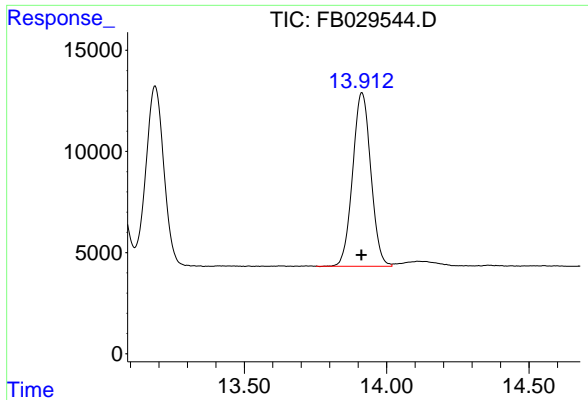

#9 O-Xylene

R.T.: 13.913 min  
Delta R.T.: 0.001 min  
Response: 380564  
Conc: 20.67 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

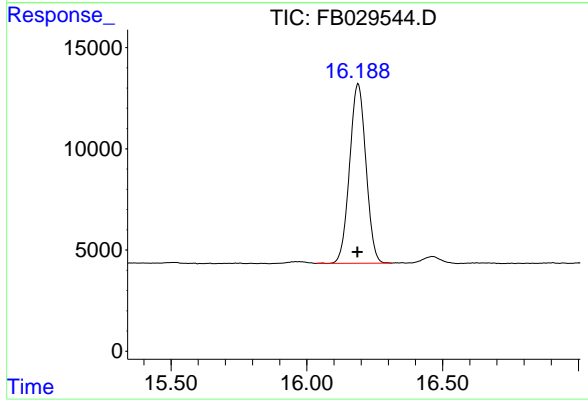

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min  
Delta R.T.: 0.002 min  
Response: 370239  
Conc: 19.88 ng/ml