

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032321\
 Data File : FB025549.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2021 9:15
 Operator : DD/AJ
 Sample : BSF0323S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 24 01:17:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
 Quant Title :
 QLast Update : Wed Mar 17 08:44:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.799	435519	20.805 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.686	972793	32.648 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	1067703	33.660 ng/ml
3) t	n-Heptane	7.758	346063	11.148 ng/ml
4) t	Benzene	7.892	422572	10.875 ng/ml
6) t	Toluene	10.630	1221340	32.345 ng/ml
7) t	Ethylbenzene	13.071	370663	10.729 ng/ml
8) t	m-Xylene	13.204	745392	21.730 ng/ml
9) t	O-Xylene	13.931	710961	21.469 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	617415	21.395 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032321\
Data File : FB025549.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2021 9:15
Operator : DD/AJ
Sample : BSF0323S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 24 01:17:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
Quant Title :
QLast Update : Wed Mar 17 08:44:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

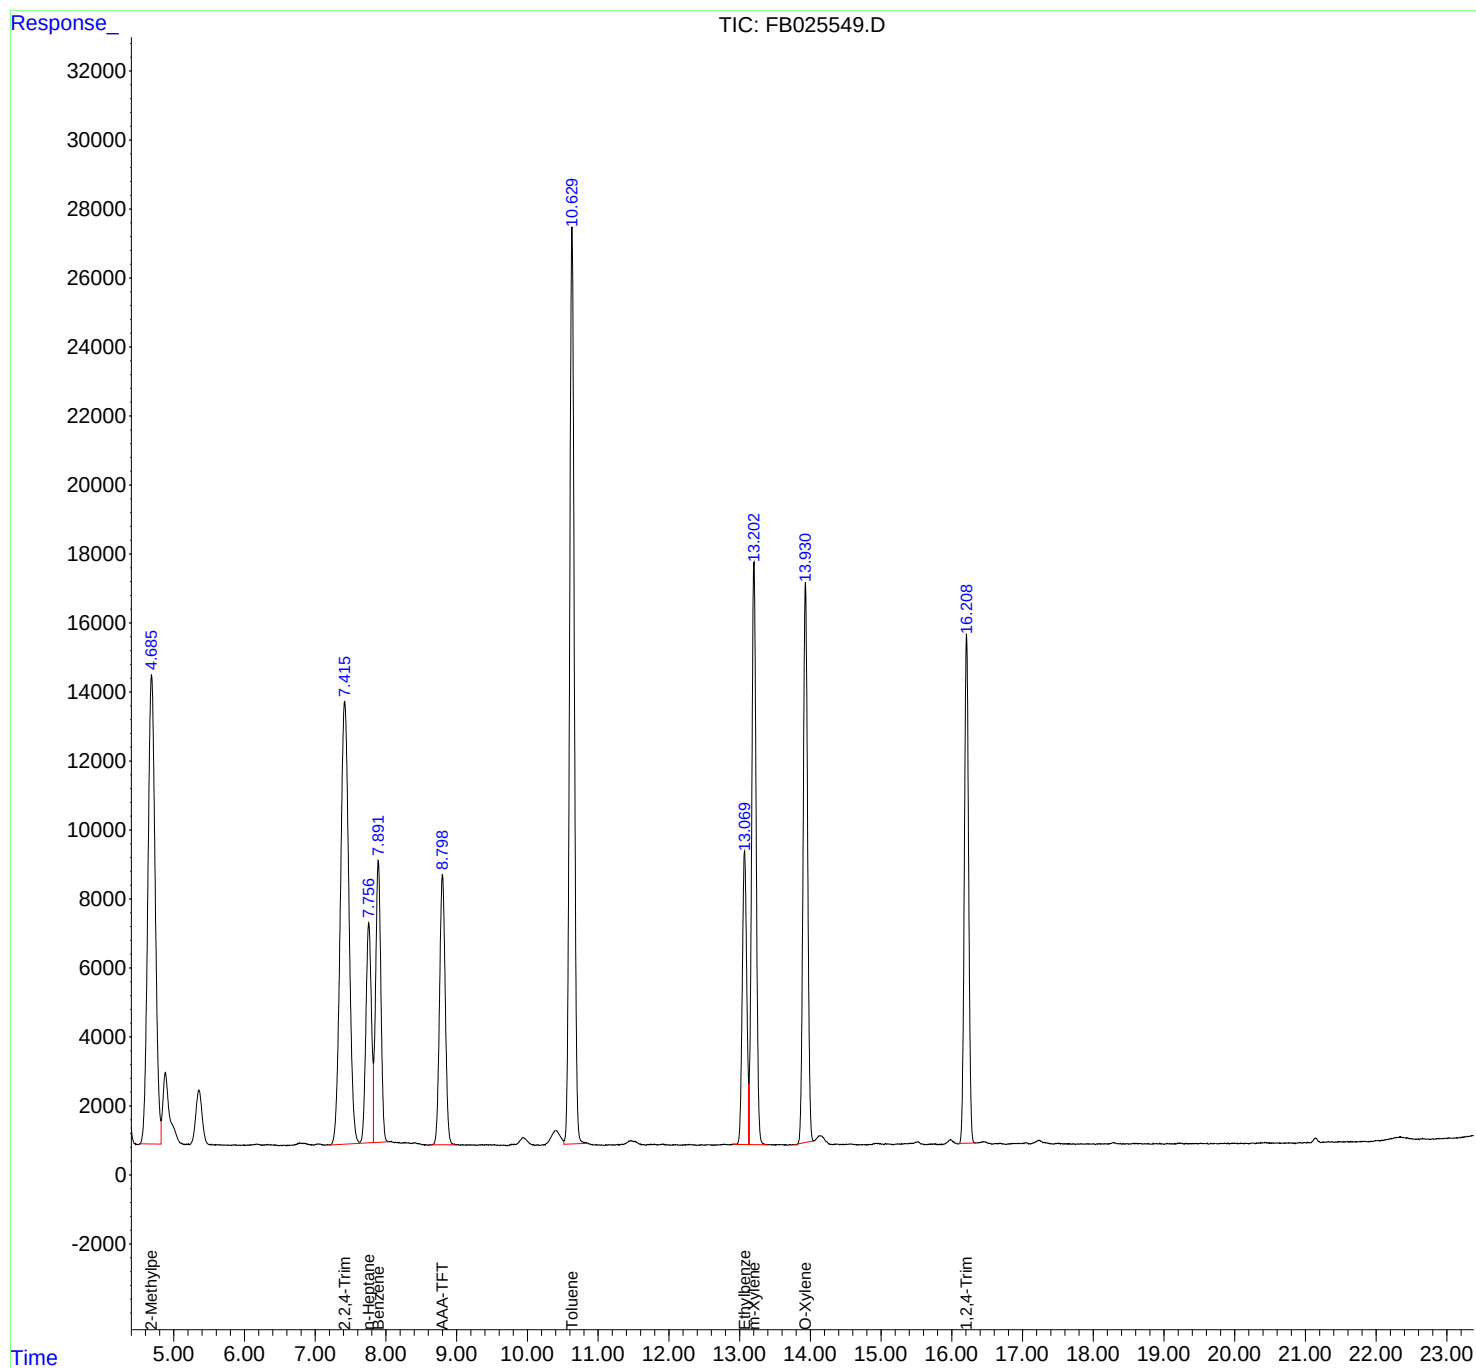

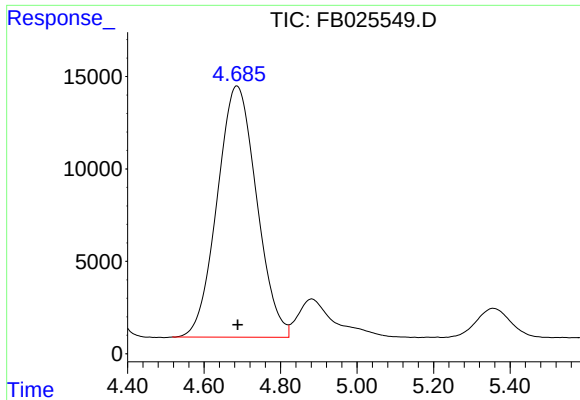


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.002 min
Response: 972793
Conc: 32.65 ng/ml

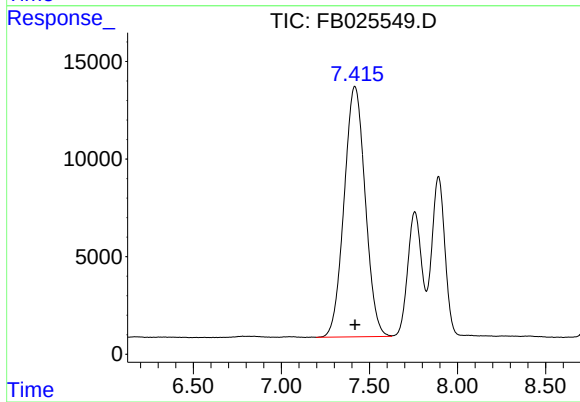


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 1067703
Conc: 33.66 ng/ml

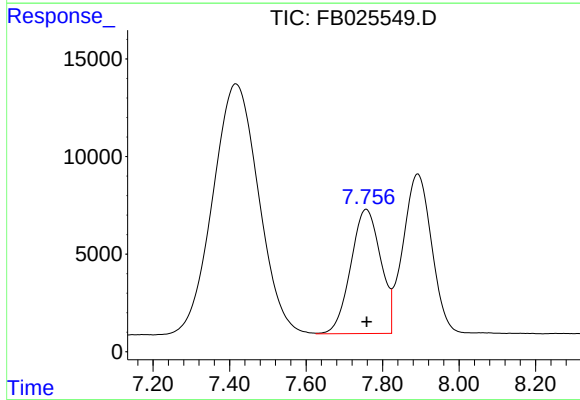


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 346063
Conc: 11.15 ng/ml

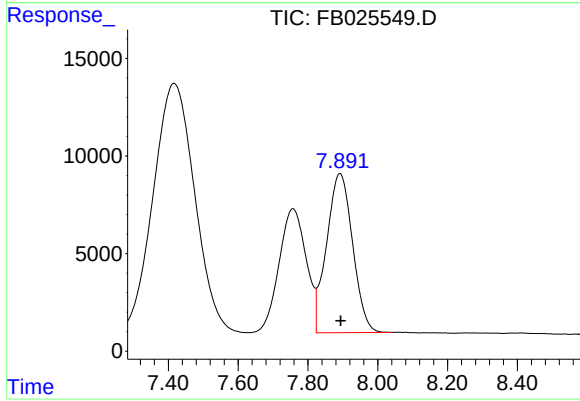


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 422572
Conc: 10.87 ng/ml

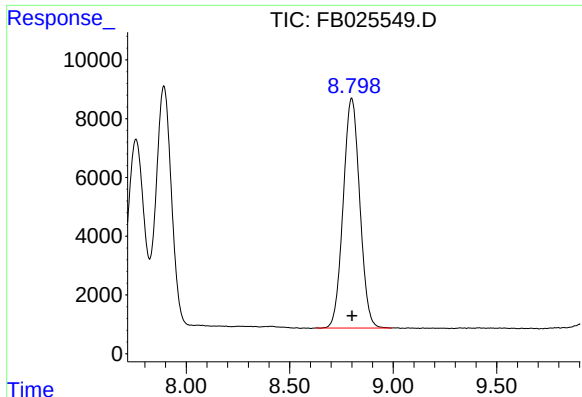


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.001 min
Response: 435519
Conc: 20.81 ng/ml

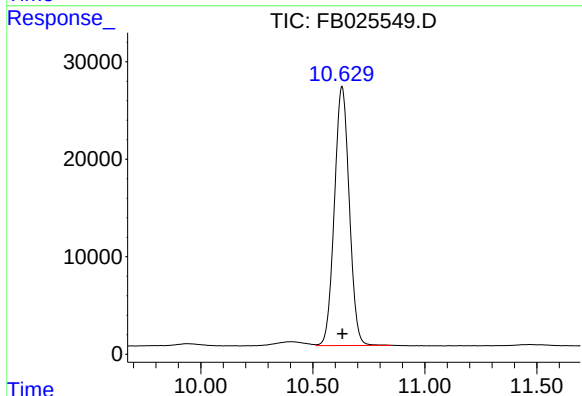


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 1221340
Conc: 32.34 ng/ml

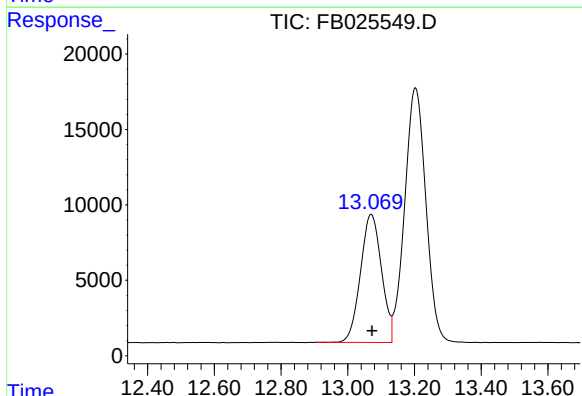


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: -0.002 min
Response: 370663
Conc: 10.73 ng/ml

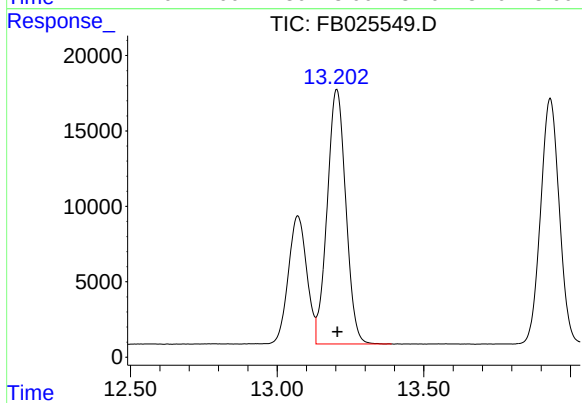


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: -0.002 min
Response: 745392
Conc: 21.73 ng/ml

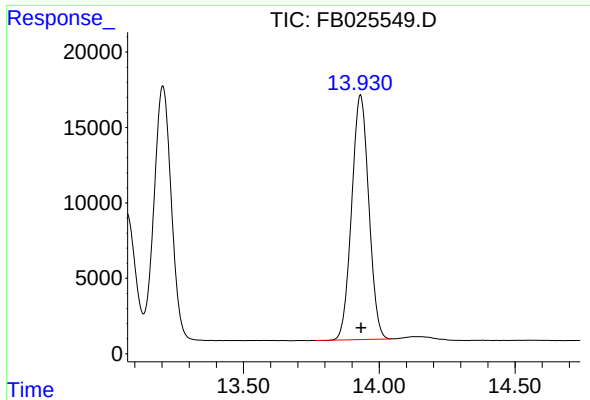

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.002 min
Response: 710961
Conc: 21.47 ng/ml

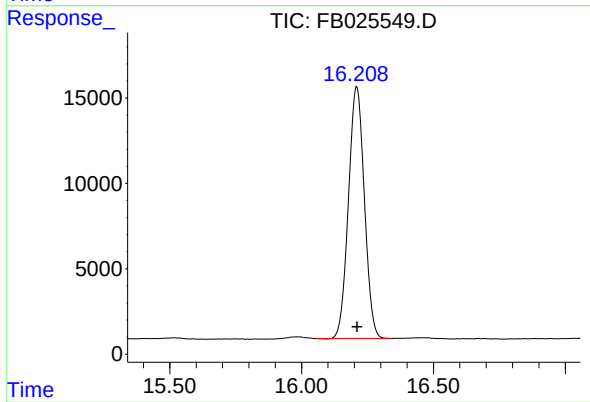

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 617415
Conc: 21.39 ng/ml