

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032321\
 Data File : FB025552.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2021 13:25
 Operator : DD/AJ
 Sample : M1751-01MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 24 01:17:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
 Quant Title :
 QLast Update : Wed Mar 17 08:44:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	322195	15.392 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	593424	19.916 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	503536	15.875 ng/ml
3) t n-Heptane	7.758	122472	3.945 ng/ml
4) t Benzene	7.892	332512	8.557 ng/ml
6) t Toluene	10.630	902632	23.904 ng/ml
7) t Ethylbenzene	13.070	262200	7.590 ng/ml
8) t m-Xylene	13.203	525864	15.331 ng/ml
9) t O-Xylene	13.931	517176	15.617 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	385954	13.374 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032321\
Data File : FB025552.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2021 13:25
Operator : DD/AJ
Sample : M1751-01MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 24 01:17:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
Quant Title :
QLast Update : Wed Mar 17 08:44:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

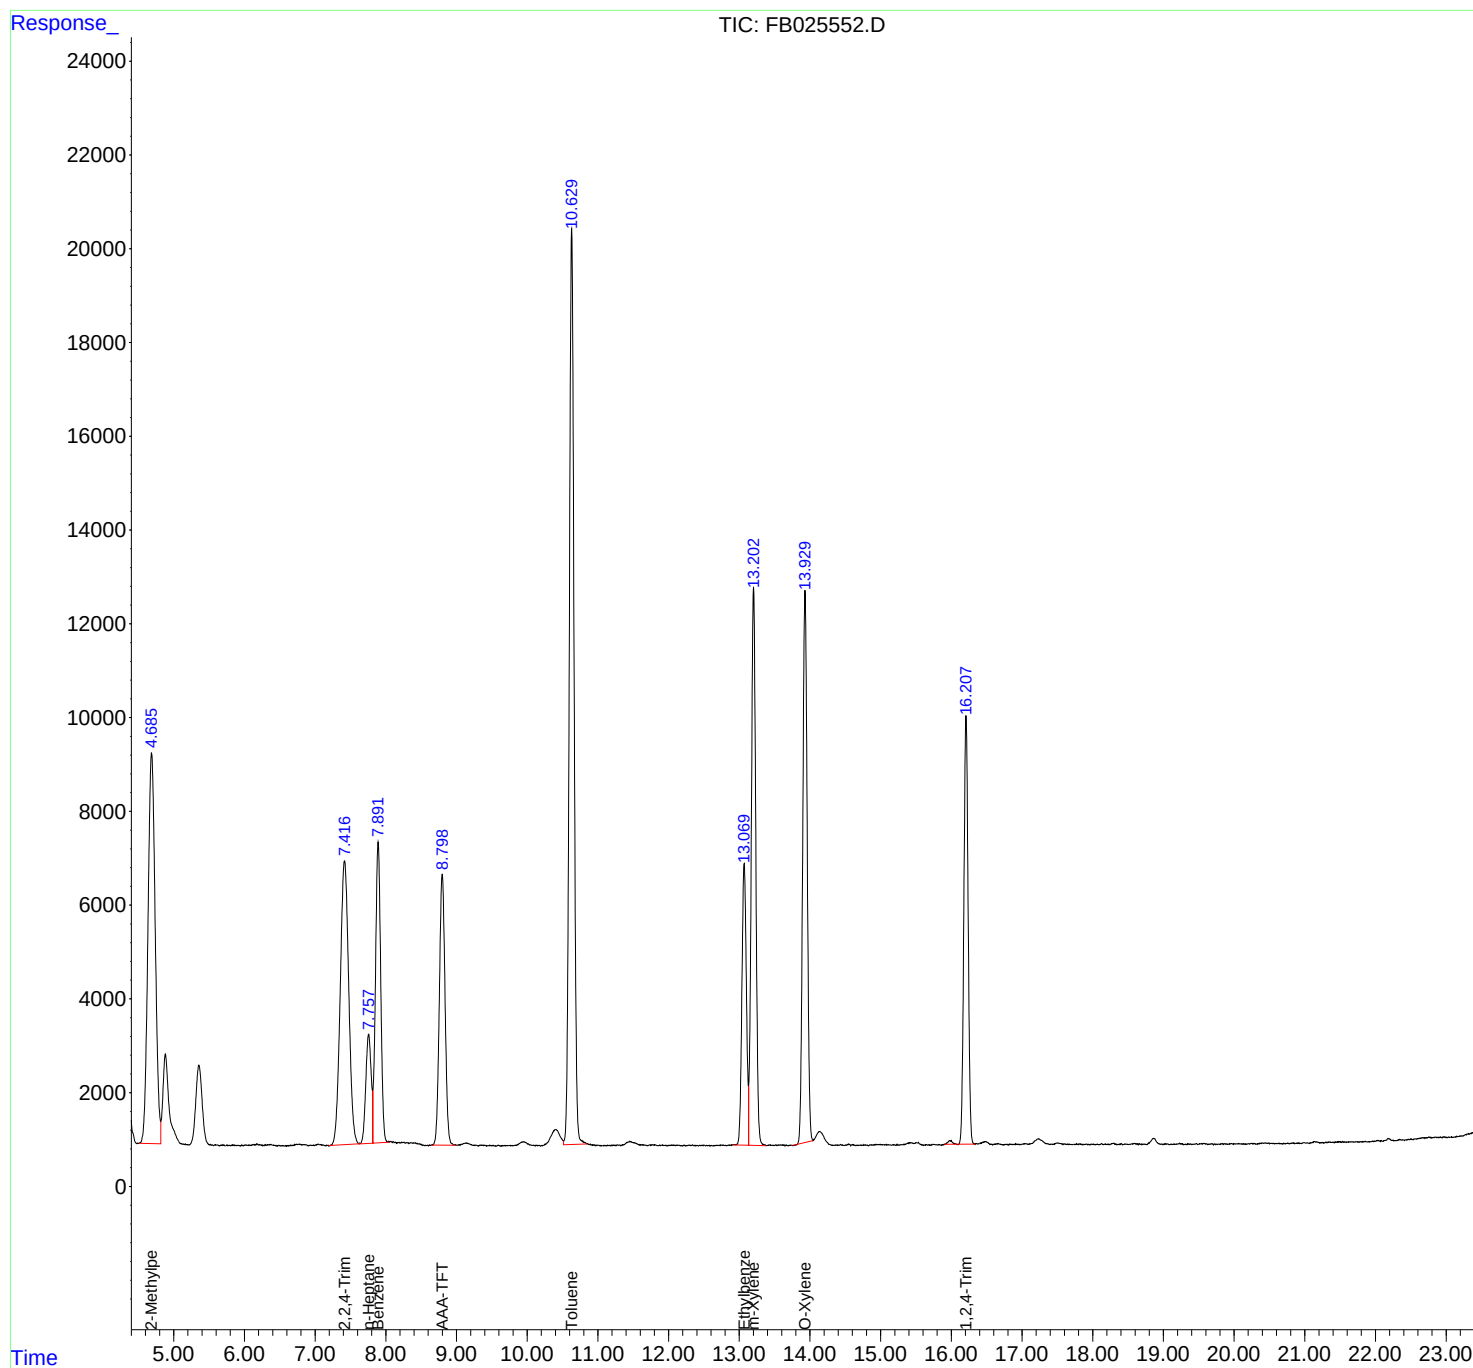

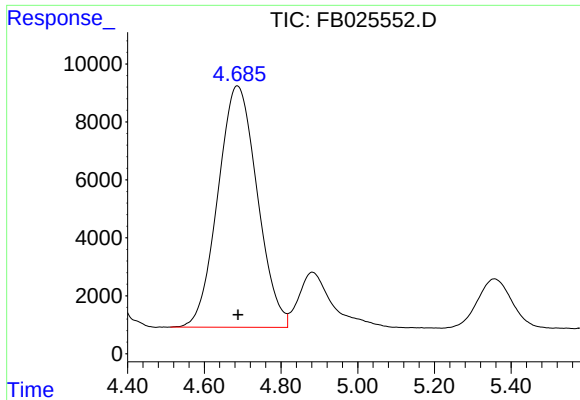


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.001 min
Response: 593424
Conc: 19.92 ng/ml

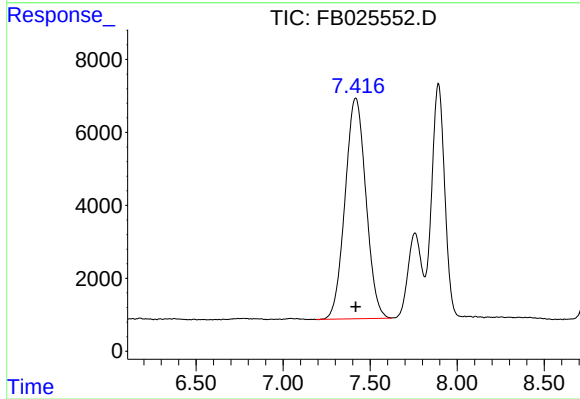


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 503536
Conc: 15.87 ng/ml

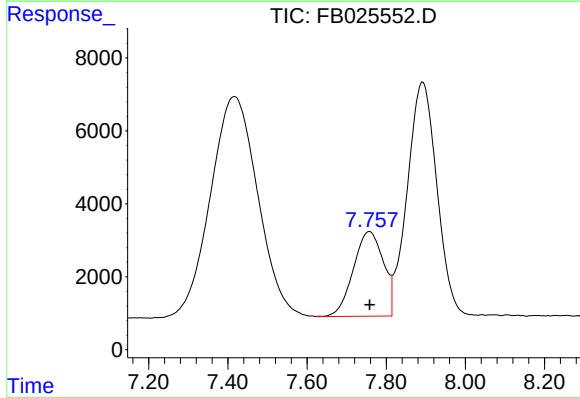


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 122472
Conc: 3.95 ng/ml

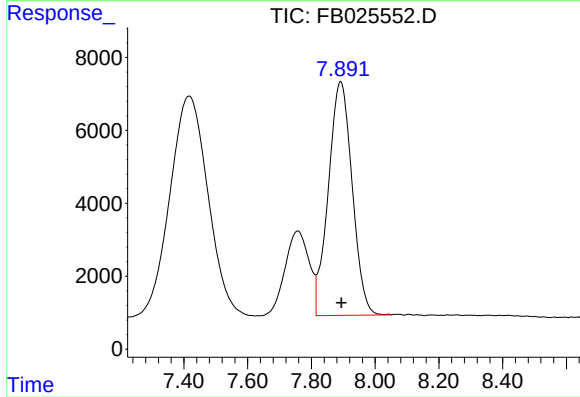


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 332512
Conc: 8.56 ng/ml

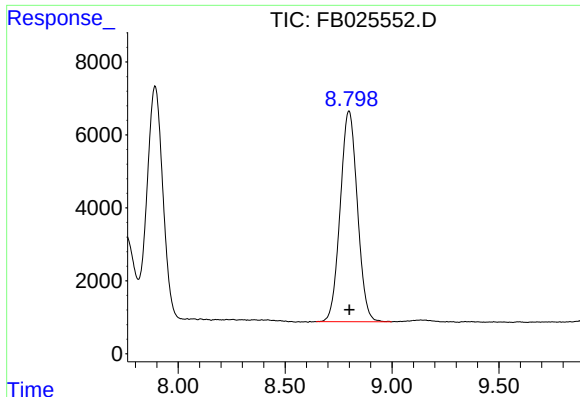


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.002 min
Response: 322195
Conc: 15.39 ng/ml

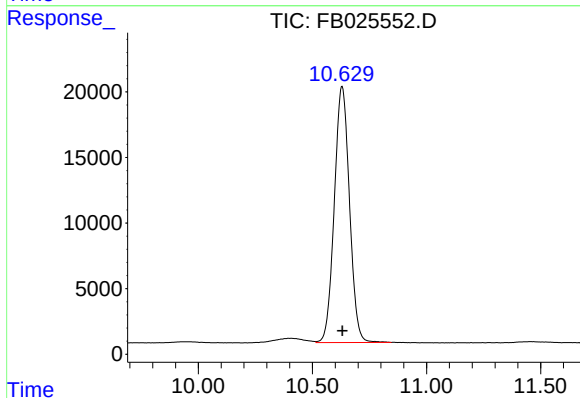


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.002 min
Response: 902632
Conc: 23.90 ng/ml

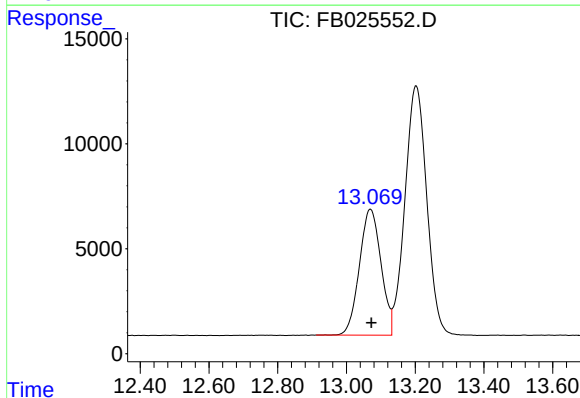


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.003 min
Response: 262200
Conc: 7.59 ng/ml

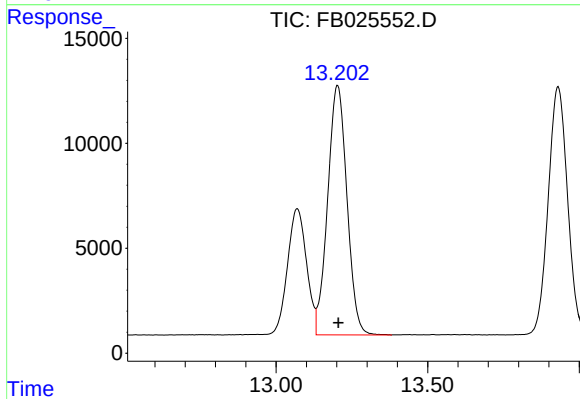


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.002 min
Response: 525864
Conc: 15.33 ng/ml

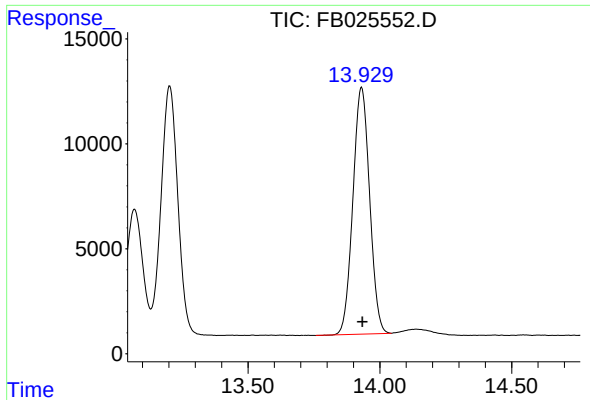

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.003 min
Response: 517176
Conc: 15.62 ng/ml

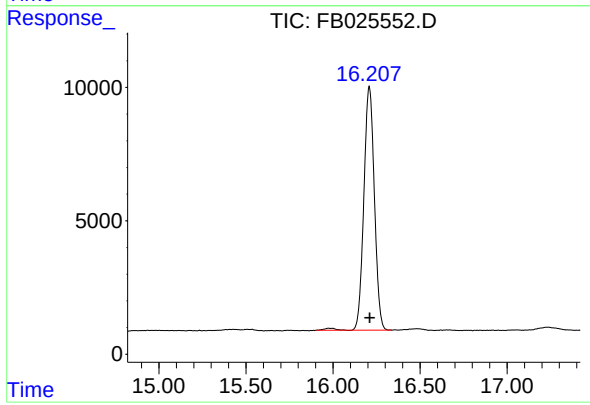

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 385954
Conc: 13.37 ng/ml