

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032321\
 Data File : FB025551.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2021 12:54
 Operator : DD/AJ
 Sample : M1751-01MS
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 24 01:17:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
 Quant Title :
 QLast Update : Wed Mar 17 08:44:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	378382	18.076 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	642016	21.546 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	554212	17.472 ng/ml
3) t n-Heptane	7.756	157152	5.063 ng/ml
4) t Benzene	7.891	358940	9.237 ng/ml
6) t Toluene	10.629	975192	25.826 ng/ml
7) t Ethylbenzene	13.069	283116	8.195 ng/ml
8) t m-Xylene	13.202	561850	16.380 ng/ml
9) t O-Xylene	13.930	547729	16.539 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	404648	14.022 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032321\
Data File : FB025551.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2021 12:54
Operator : DD/AJ
Sample : M1751-01MS
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 24 01:17:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
Quant Title :
QLast Update : Wed Mar 17 08:44:23 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

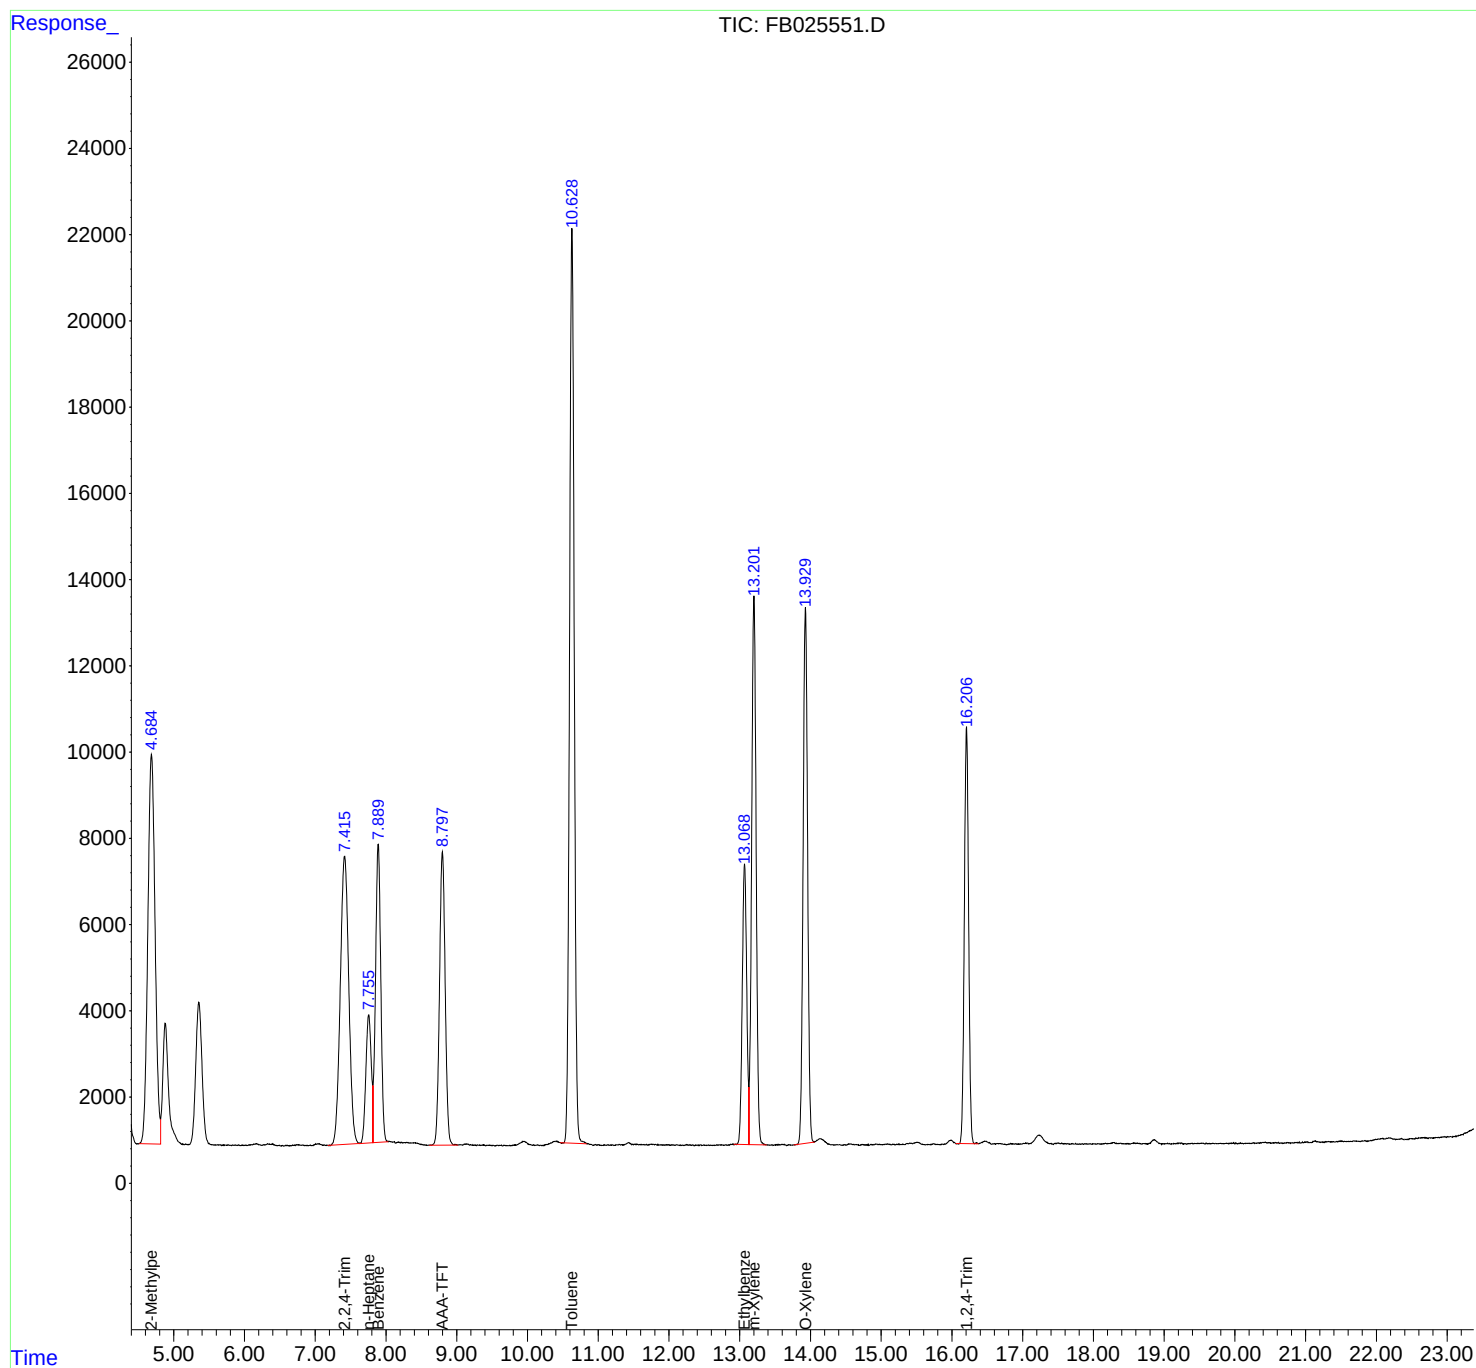

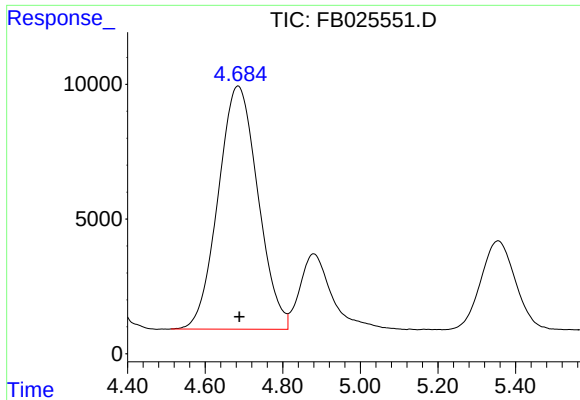


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.003 min
Response: 642016
Conc: 21.55 ng/ml

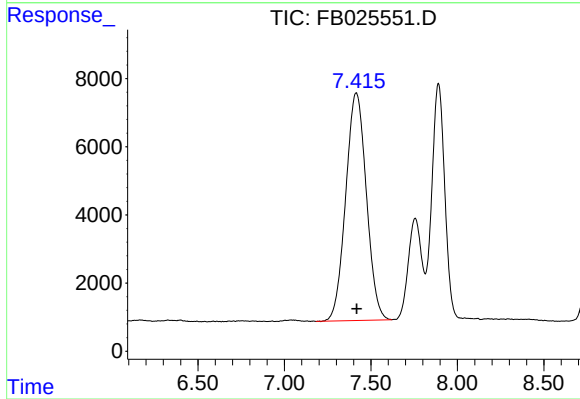


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 554212
Conc: 17.47 ng/ml

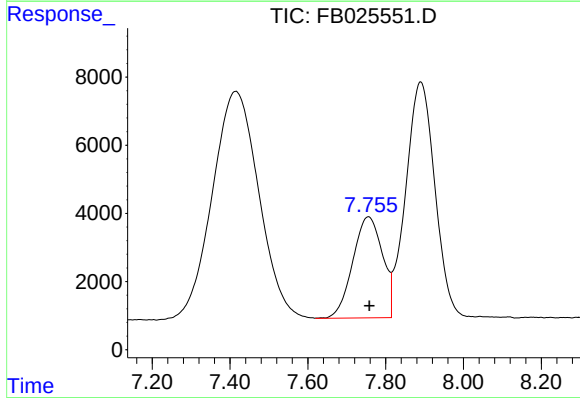


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.003 min
Response: 157152
Conc: 5.06 ng/ml

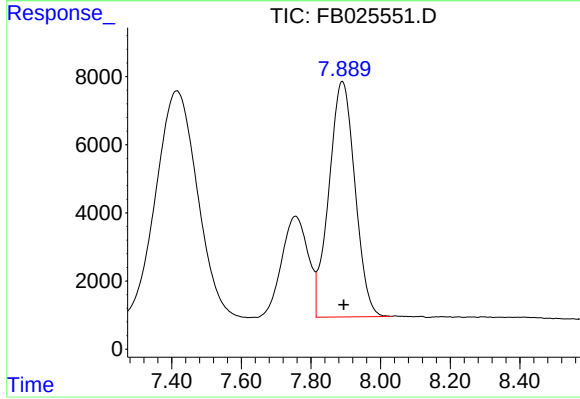


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.003 min
Response: 358940
Conc: 9.24 ng/ml

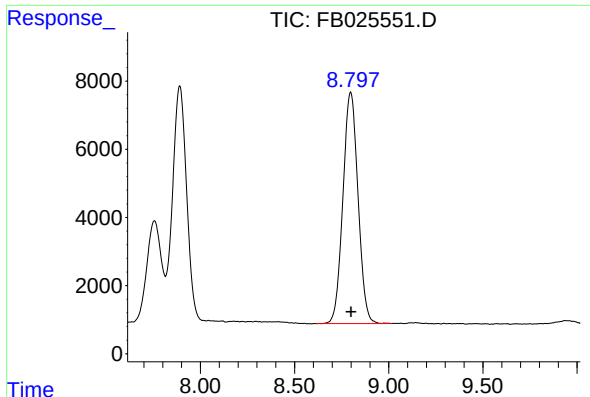


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 378382
Conc: 18.08 ng/ml

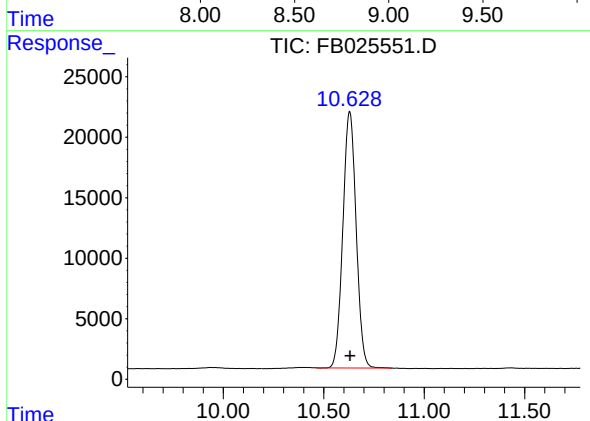


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 975192
Conc: 25.83 ng/ml

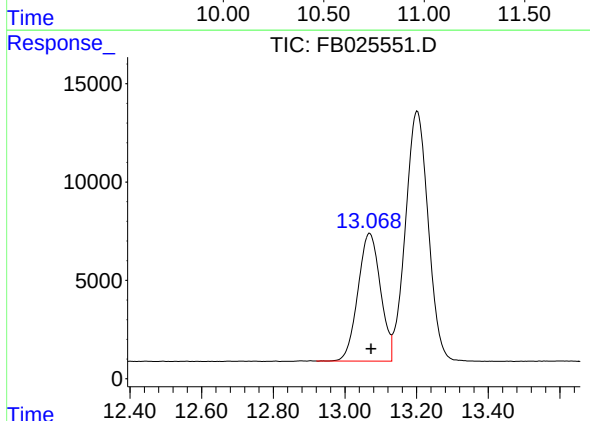


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.004 min
Response: 283116
Conc: 8.20 ng/ml

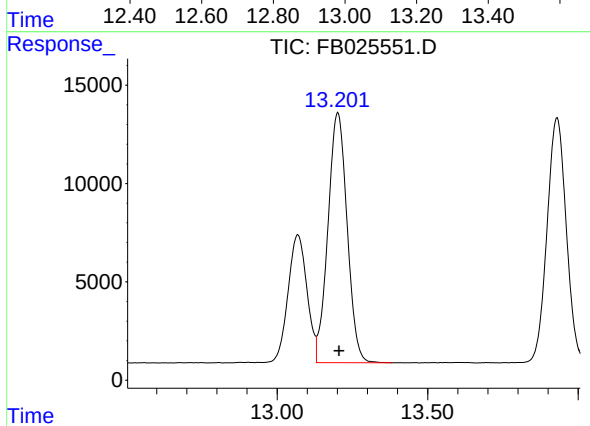


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.004 min
Response: 561850
Conc: 16.38 ng/ml

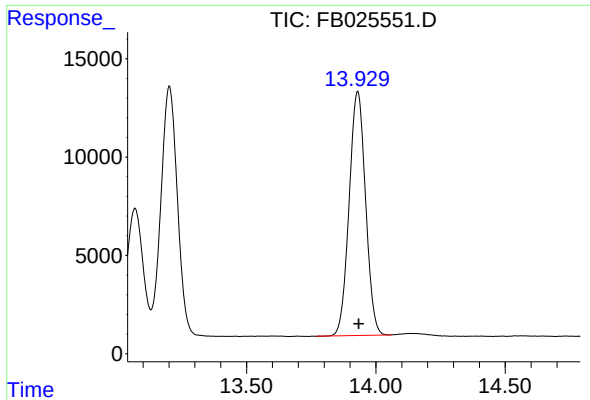

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.004 min
Response: 547729
Conc: 16.54 ng/ml

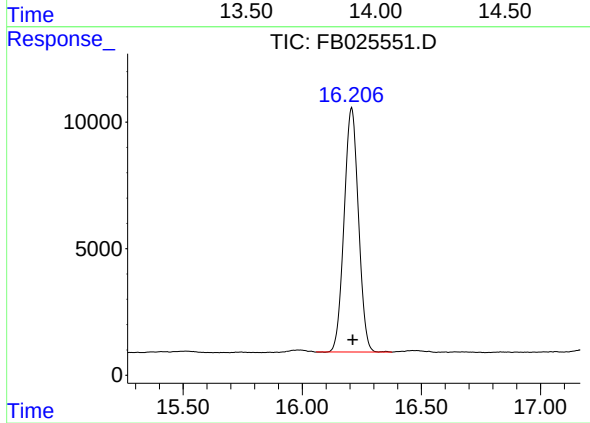

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 404648
Conc: 14.02 ng/ml