

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026786.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 10:30
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 23 16:08:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	249741	23.800 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	449442	23.738 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	521486	25.159 ng/ml
3) t n-Heptane	7.748	163949	8.283 ng/ml
4) t Benzene	7.884	224575	9.733 ng/ml
6) t Toluene	10.617	639945	29.231 ng/ml
7) t Ethylbenzene	13.053	198843	9.894 ng/ml
8) t m-Xylene	13.186	396653	19.682 ng/ml
9) t O-Xylene	13.914	385468	19.322 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	390425	19.595 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026786.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 10:30
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 16:08:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

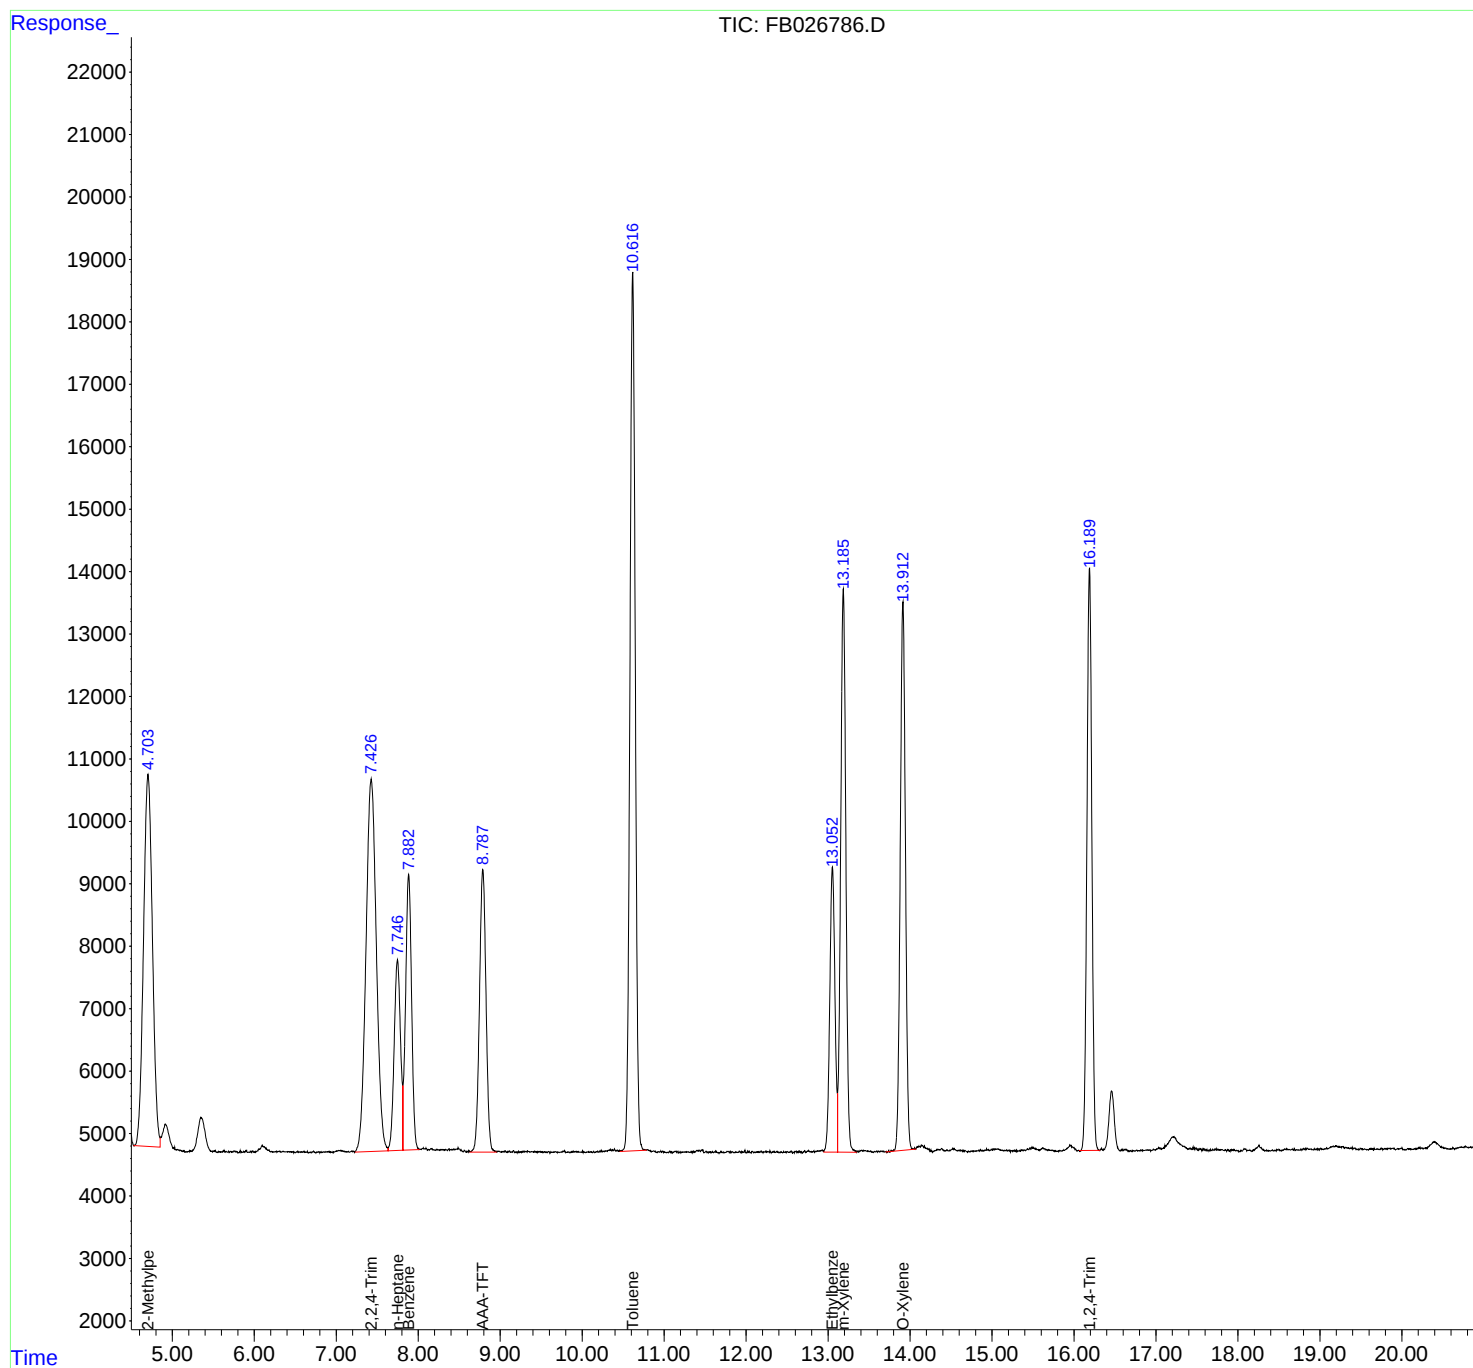


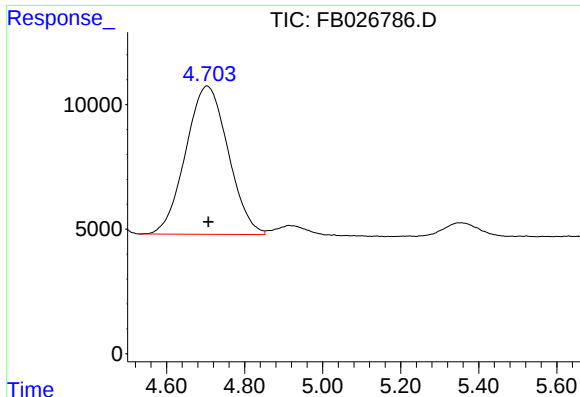

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 449442
Conc: 23.74 ng/ml

Instrument :
FID_B
ClientSampleId :

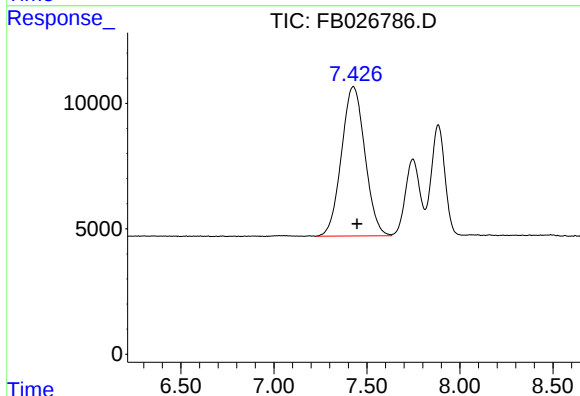


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.020 min
Response: 521486
Conc: 25.16 ng/ml

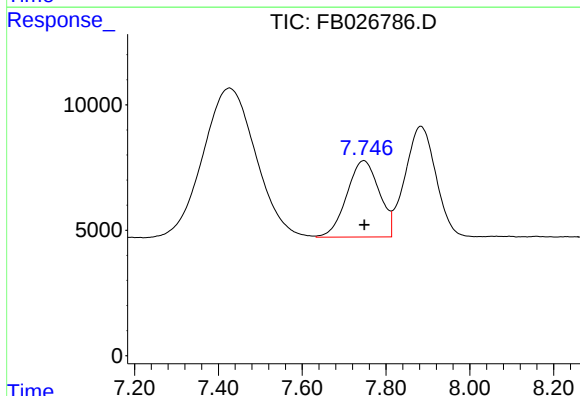


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 163949
Conc: 8.28 ng/ml

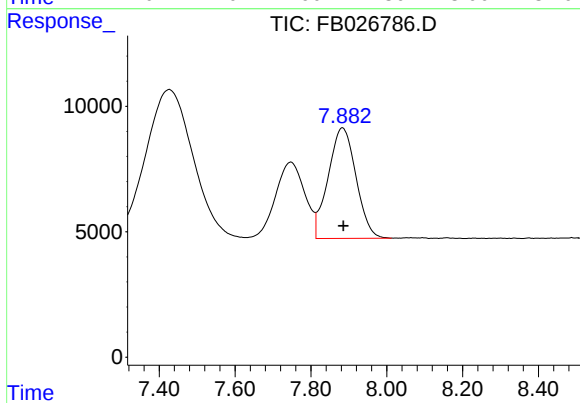

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 224575
Conc: 9.73 ng/ml

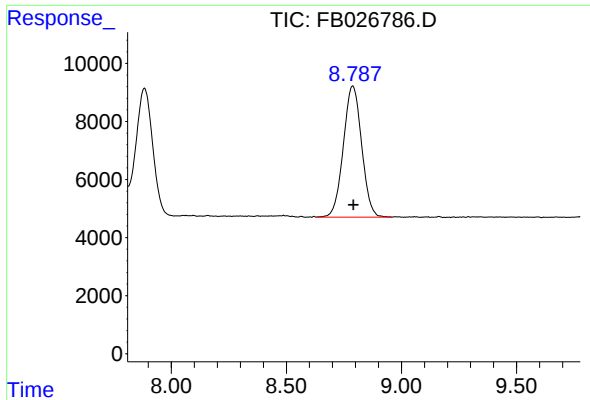

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.003 min
Response: 249741
Conc: 23.80 ng/ml

Instrument :
FID_B
ClientSampleId :

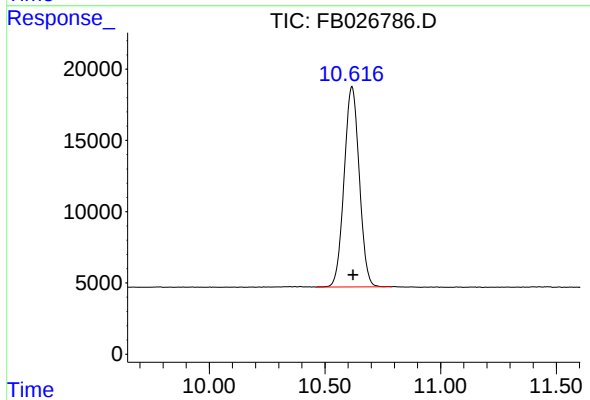


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 639945
Conc: 29.23 ng/ml

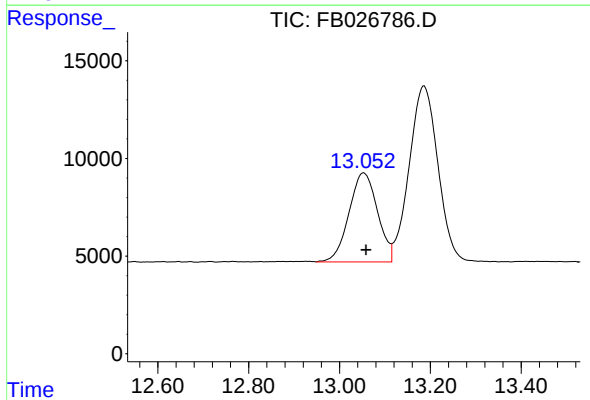


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 198843
Conc: 9.89 ng/ml

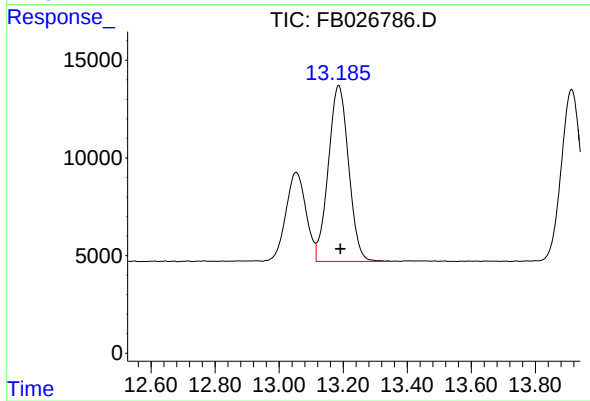

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 396653
Conc: 19.68 ng/ml

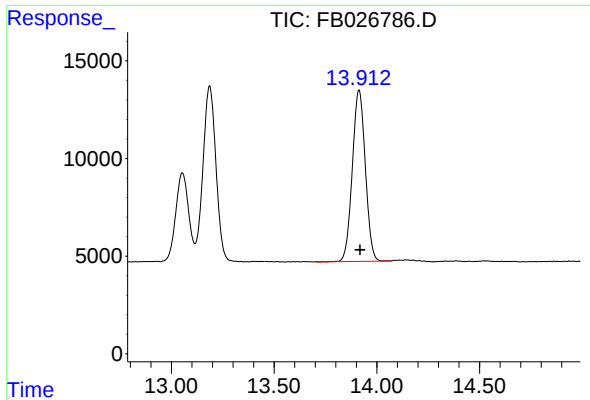

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.005 min
Response: 385468
Conc: 19.32 ng/ml

Instrument :
FID_B
ClientSampleId :

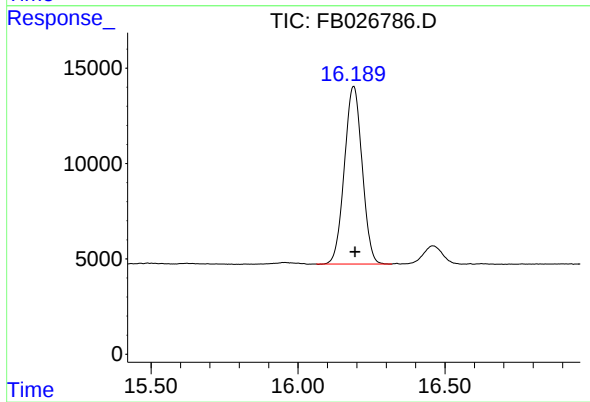

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 390425
Conc: 19.60 ng/ml