

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026794.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 15:36
 Operator : AJ/MA
 Sample : N1974-10
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 23 17:06:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	169748	16.177 ng/ml
Target Compounds			
7) t Ethylbenzene	13.045	10079	0.502 ng/ml
8) t m-Xylene	13.187	7083	0.351 ng/ml
9) t O-Xylene	13.908	6501	0.326 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	9745	0.489 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026794.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 15:36
Operator : AJ/MA
Sample : N1974-10
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 17:06:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

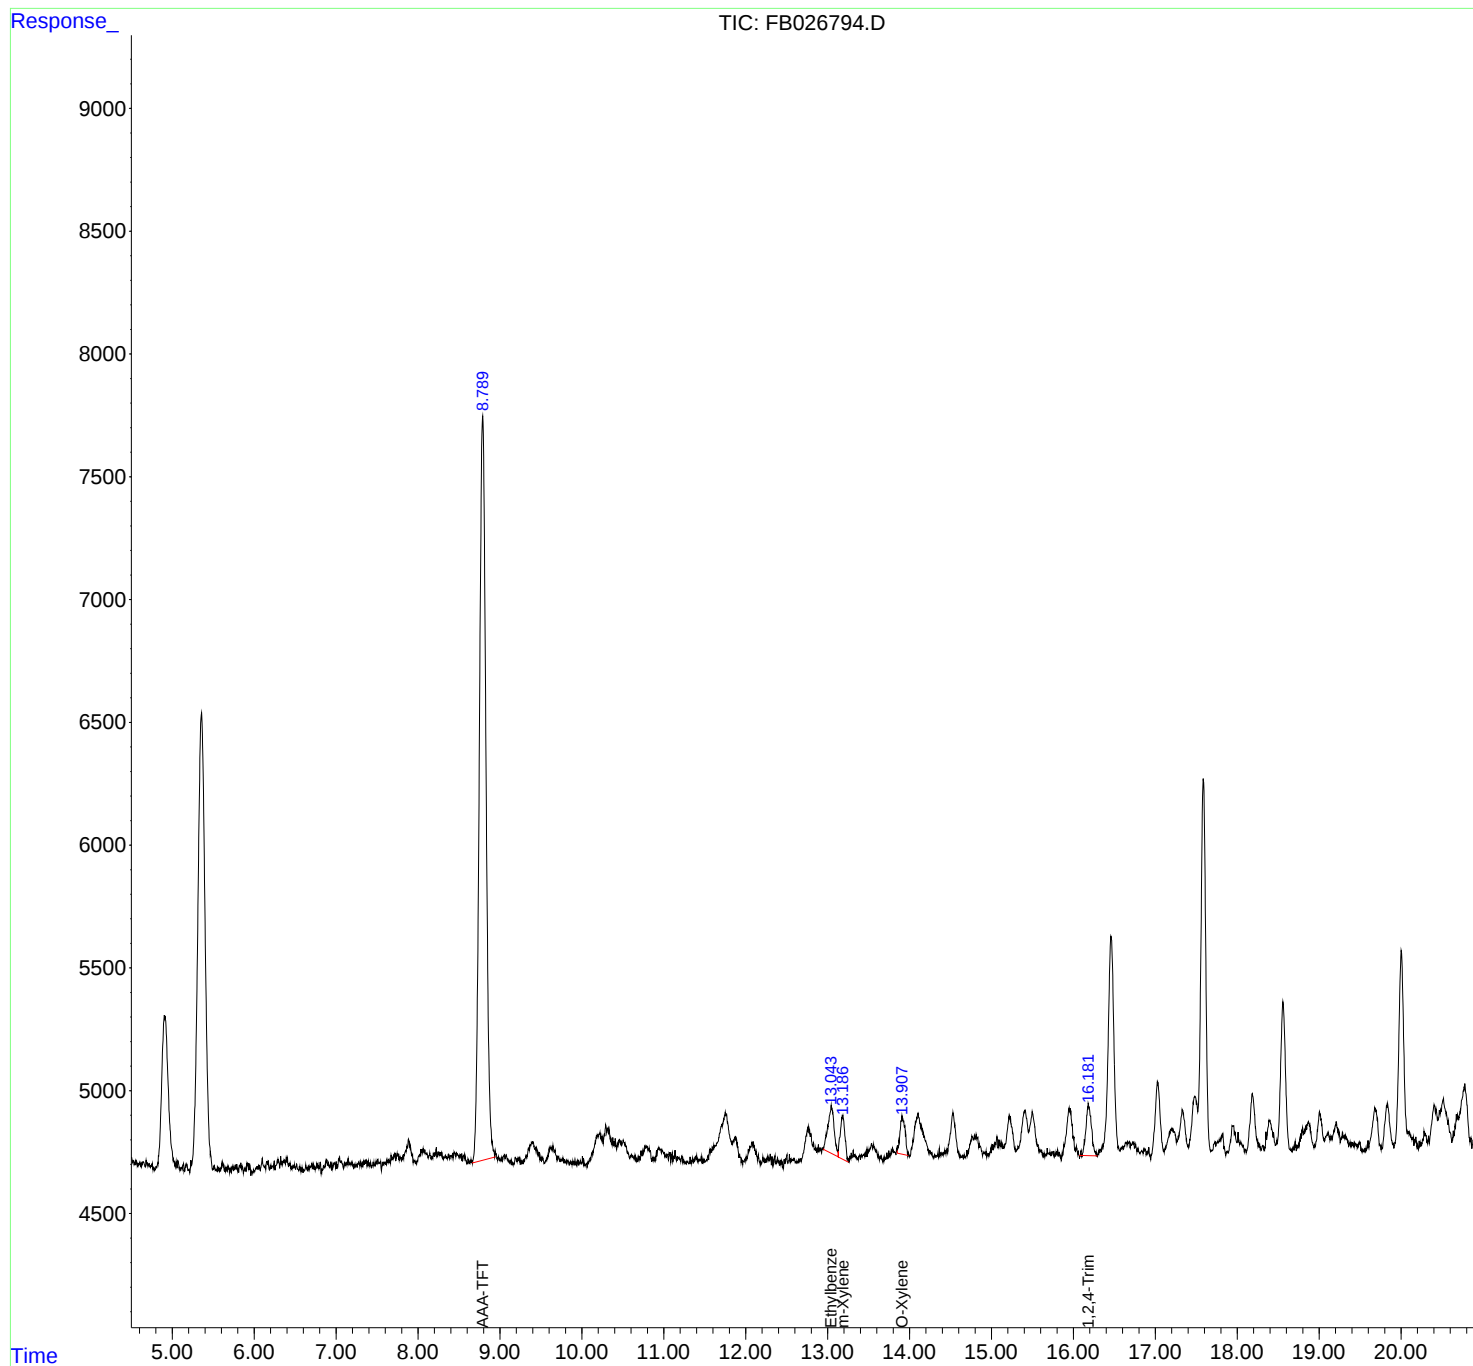


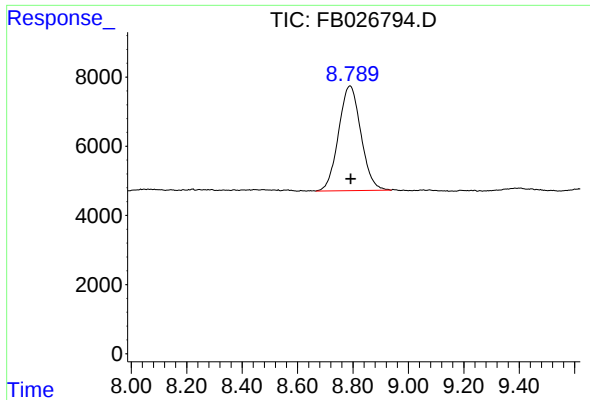

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 169748
Conc: 16.18 ng/ml

Instrument :
FID_B
ClientSampleId :

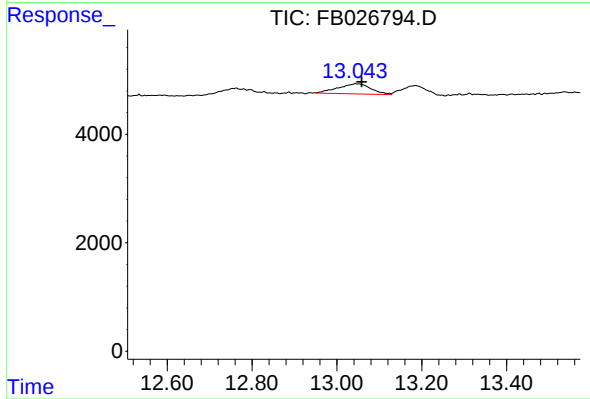


#7 Ethylbenzene

R.T.: 13.045 min
Delta R.T.: -0.014 min
Response: 10079
Conc: 0.50 ng/ml

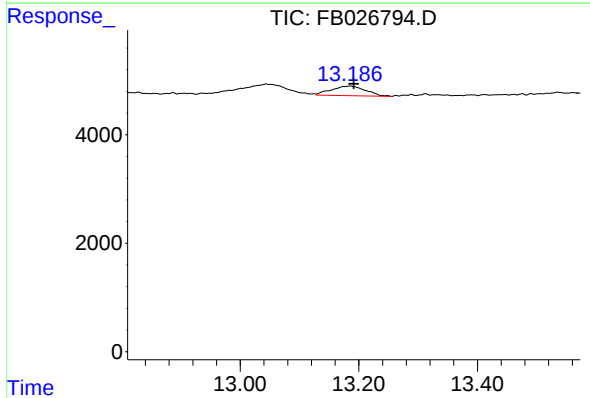


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 7083
Conc: 0.35 ng/ml

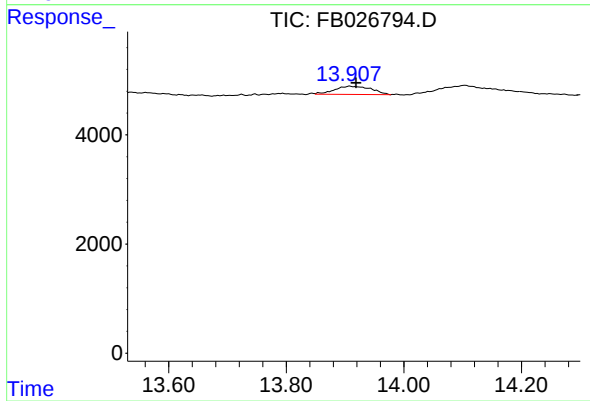

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.011 min
Response: 6501
Conc: 0.33 ng/ml

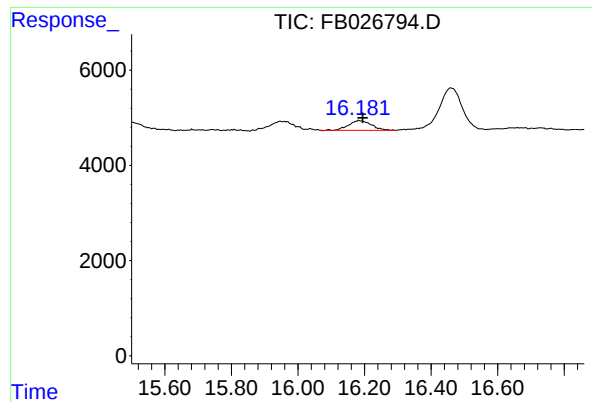

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.012 min
Response: 9745
Conc: 0.49 ng/ml

Instrument :

FID_B

ClientSampleId :